


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091024\
Data File : VW030123.D
Acq On : 10 Sep 2024 08:22
Operator : SY/MD
Sample : BFB556
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB556

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM082624SMA.M
Title : SFAM01.0
Last Update : Wed Sep 11 01:35:57 2024

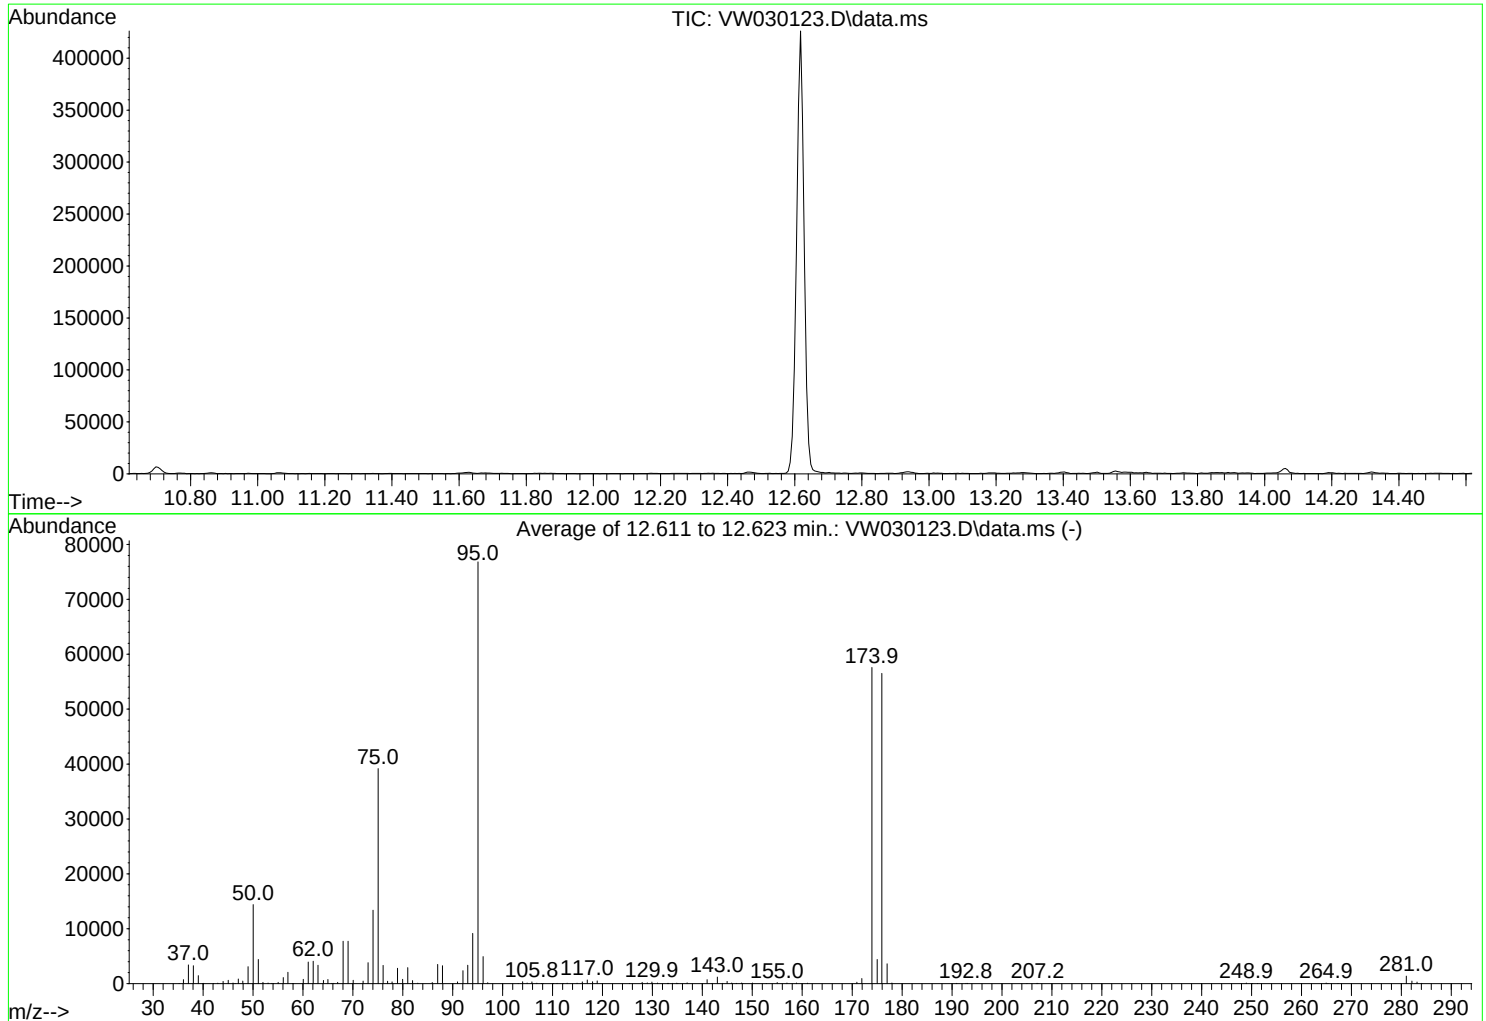

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	14386	PASS
75	95	30	80	51.0	39176	PASS
95	95	100	100	100.0	76832	PASS
96	95	5	9	6.4	4938	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.9	57584	PASS
175	174	5	9	7.7	4417	PASS
176	174	95	101	98.1	56504	PASS
177	176	5	9	6.4	3615	PASS

m/z	Abundance
36.10	89.0
40.00	124.0
44.00	158.0
57.00	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556

m/z	Abundance
36.00	918.0
37.00	3536.0
38.00	2934.0
39.10	1576.0
39.90	208.0
43.00	79.0
44.00	630.0
45.00	649.0
46.10	126.0
47.00	831.0
48.00	497.0
49.00	3251.0
50.10	14312.0
51.00	4598.0
52.00	321.0
53.00	165.0
53.80	70.0
54.10	62.0
55.00	220.0
56.10	1104.0
57.00	2262.0
57.90	100.0
60.10	639.0
61.00	3992.0
62.10	3952.0
63.00	3488.0
64.10	594.0
65.00	709.0
65.80	81.0
67.00	212.0
68.10	7352.0
69.00	7359.0
70.10	726.0
72.10	416.0
73.10	3997.0
74.10	12821.0
75.00	37440.0
76.10	3226.0
76.90	488.0
77.80	345.0
79.00	2774.0
80.00	780.0
81.00	3174.0
81.90	560.0
83.00	84.0
85.90	209.0
87.00	3557.0
87.90	3034.0
91.00	315.0
92.00	2462.0
93.00	3184.0
94.00	8692.0
95.10	71216.0
96.10	4371.0
97.10	238.0
103.10	91.0
104.00	323.0
104.90	161.0
105.90	309.0
106.80	97.0
108.20	53.0
110.20	70.0
110.90	94.0
112.10	73.0
112.80	92.0
114.90	103.0
115.90	298.0
117.00	763.0
118.10	332.0
119.00	463.0
125.40	50.0
128.00	207.0
129.00	107.0
129.90	350.0
131.00	129.0
133.00	158.0
134.00	110.0
134.90	135.0
137.00	139.0
140.90	577.0
141.90	59.0
143.00	1111.0
144.00	85.0
144.90	436.0
146.00	125.0
146.80	52.0
147.90	148.0
150.00	78.0
155.10	161.0
156.90	130.0
158.90	70.0
161.00	83.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556

171.00	236.0
171.90	943.0
174.00	52168.0
175.00	3881.0
176.00	50272.0
177.00	3298.0
178.00	98.0
191.00	135.0
192.80	206.0
205.00	73.0
207.00	175.0
248.90	186.0
250.20	73.0
251.20	90.0
265.00	216.0
267.30	53.0
281.00	1524.0
282.10	722.0
283.10	446.0
284.10	111.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556

m/z	Abundance
36.00	915.0
37.00	3667.0
38.10	3947.0
39.00	1604.0
39.90	183.0
42.10	51.0
42.90	130.0
44.10	549.0
45.00	718.0
45.90	141.0
47.00	971.0
47.90	614.0
49.00	3182.0
50.10	16368.0
51.10	5282.0
52.00	220.0
52.90	109.0
53.80	78.0
55.00	242.0
56.00	1244.0
57.10	2353.0
58.10	127.0
60.00	901.0
61.00	4281.0
62.10	4770.0
63.00	3853.0
64.10	679.0
65.00	779.0
66.20	87.0
67.00	275.0
68.00	8685.0
69.10	8860.0
70.00	643.0
72.00	503.0
73.10	4215.0
74.10	15128.0
75.10	45256.0
76.00	4161.0
76.90	434.0
77.90	308.0
79.00	3142.0
79.90	893.0
81.00	3078.0
82.00	653.0
83.00	84.0
85.90	193.0
87.00	3827.0
88.00	3918.0
90.80	333.0
92.10	2557.0
93.00	3734.0
94.00	10211.0
95.00	87264.0
96.10	5848.0
97.00	171.0
104.00	446.0
104.90	108.0
105.80	373.0
106.90	110.0
107.80	55.0
110.90	89.0
112.90	113.0
114.90	116.0
116.00	304.0
116.90	721.0
117.90	449.0
119.00	522.0
127.80	308.0
128.90	201.0
129.90	326.0
131.00	112.0
133.20	154.0
134.00	58.0
135.10	173.0
136.90	201.0
140.90	791.0
141.90	66.0
143.00	1411.0
144.00	62.0
145.00	433.0
146.00	121.0
146.80	106.0
148.10	191.0
150.00	162.0
152.80	61.0
155.00	211.0
157.00	138.0
158.80	148.0
161.10	106.0
170.80	198.0
171.10	198.0
172.00	926.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556

174.00	67928.0
175.00	5212.0
175.90	63160.0
177.00	3666.0
177.90	187.0
190.90	62.0
193.10	119.0
207.20	126.0
249.00	81.0
264.80	102.0
265.30	131.0
281.00	1830.0
282.10	466.0
283.20	319.0
284.10	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556

m/z	Abundance
35.20	61.0
36.10	671.0
37.10	3051.0
38.10	2879.0
39.00	1200.0
40.10	157.0
42.10	55.0
42.90	55.0
44.00	490.0
45.10	480.0
46.00	109.0
46.40	114.0
47.10	723.0
48.00	291.0
49.00	2864.0
50.00	12478.0
51.10	3362.0
52.10	164.0
53.10	103.0
53.80	64.0
55.10	216.0
56.00	963.0
57.00	1809.0
60.10	856.0
61.10	3513.0
62.00	3482.0
63.00	2724.0
64.10	482.0
65.00	772.0
65.80	62.0
66.20	70.0
66.80	209.0
68.00	7156.0
69.10	6919.0
70.00	503.0
72.00	513.0
73.00	3251.0
74.00	12177.0
75.10	34832.0
76.10	2605.0
77.00	426.0
77.80	305.0
78.90	2500.0
80.00	695.0
81.00	2482.0
82.00	492.0
83.00	95.0
85.90	178.0
87.00	3102.0
88.00	2810.0
91.00	333.0
92.00	2080.0
93.00	3175.0
94.00	8571.0
95.00	72016.0
96.10	4594.0
96.90	106.0
104.00	307.0
104.90	86.0
105.90	278.0
106.90	96.0
108.00	70.0
113.00	87.0
114.90	80.0
115.90	356.0
116.90	509.0
118.00	308.0
118.90	514.0
128.00	232.0
128.90	143.0
129.90	225.0
131.00	163.0
134.80	106.0
137.00	146.0
141.00	820.0
142.00	80.0
143.00	1057.0
144.10	63.0
144.90	398.0
145.80	153.0
147.80	210.0
150.10	133.0
152.80	56.0
154.90	285.0
156.90	121.0
158.90	124.0
161.10	120.0
170.90	180.0
172.00	962.0
173.90	52656.0
175.00	4157.0
175.90	56080.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556

177.00	3881.0
177.90	93.0
193.10	86.0
207.20	74.0
249.10	52.0
281.10	732.0
282.00	188.0
283.10	92.0

Instrument :
MSVOA_W
ClientSampleId :
BFB556