

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091123\
 Data File : VW027034.D
 Acq On : 11 Sep 2023 17:12
 Operator : SY/MD
 Sample : 04332-16
 Misc : 4.26g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 12 01:15:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	717669	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	575442	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	191524	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	142117	11.084	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	44.320%
7) Chloroethane-d5	2.893	69	148021	14.304	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.200%
11) 1,1-Dichloroethene-d2	4.021	65	60926	12.894	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.560%
21) 2-Butanone-d5	7.075	46	69724	28.223	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.440%
24) Chloroform-d	7.648	84	392579	18.383	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.520%
26) 1,2-Dichloroethane-d4	8.307	65	207359	18.473	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.880%
32) Benzene-d6	8.276	84	703157	18.629	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.520%
36) 1,2-Dichloropropane-d6	9.276	67	238822	21.553	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.200%
41) Toluene-d8	10.325	98	565362	16.544	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	66.160%
43) trans-1,3-Dichloroprop...	10.581	79	55880	12.995	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	52.000%
47) 2-Hexanone-d5	10.928	63	17713	17.122	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	34.240%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	187866	21.847	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.400%
66) 1,2-Dichlorobenzene-d4	13.854	152	125432	18.936	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.760%
Target Compounds					Qvalue	
13) Acetone	4.124	43	8859	4.095	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091123\
Data File : VW027034.D
Acq On : 11 Sep 2023 17:12
Operator : SY/MD
Sample : 04332-16
Misc : 4.26g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 12 01:15:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

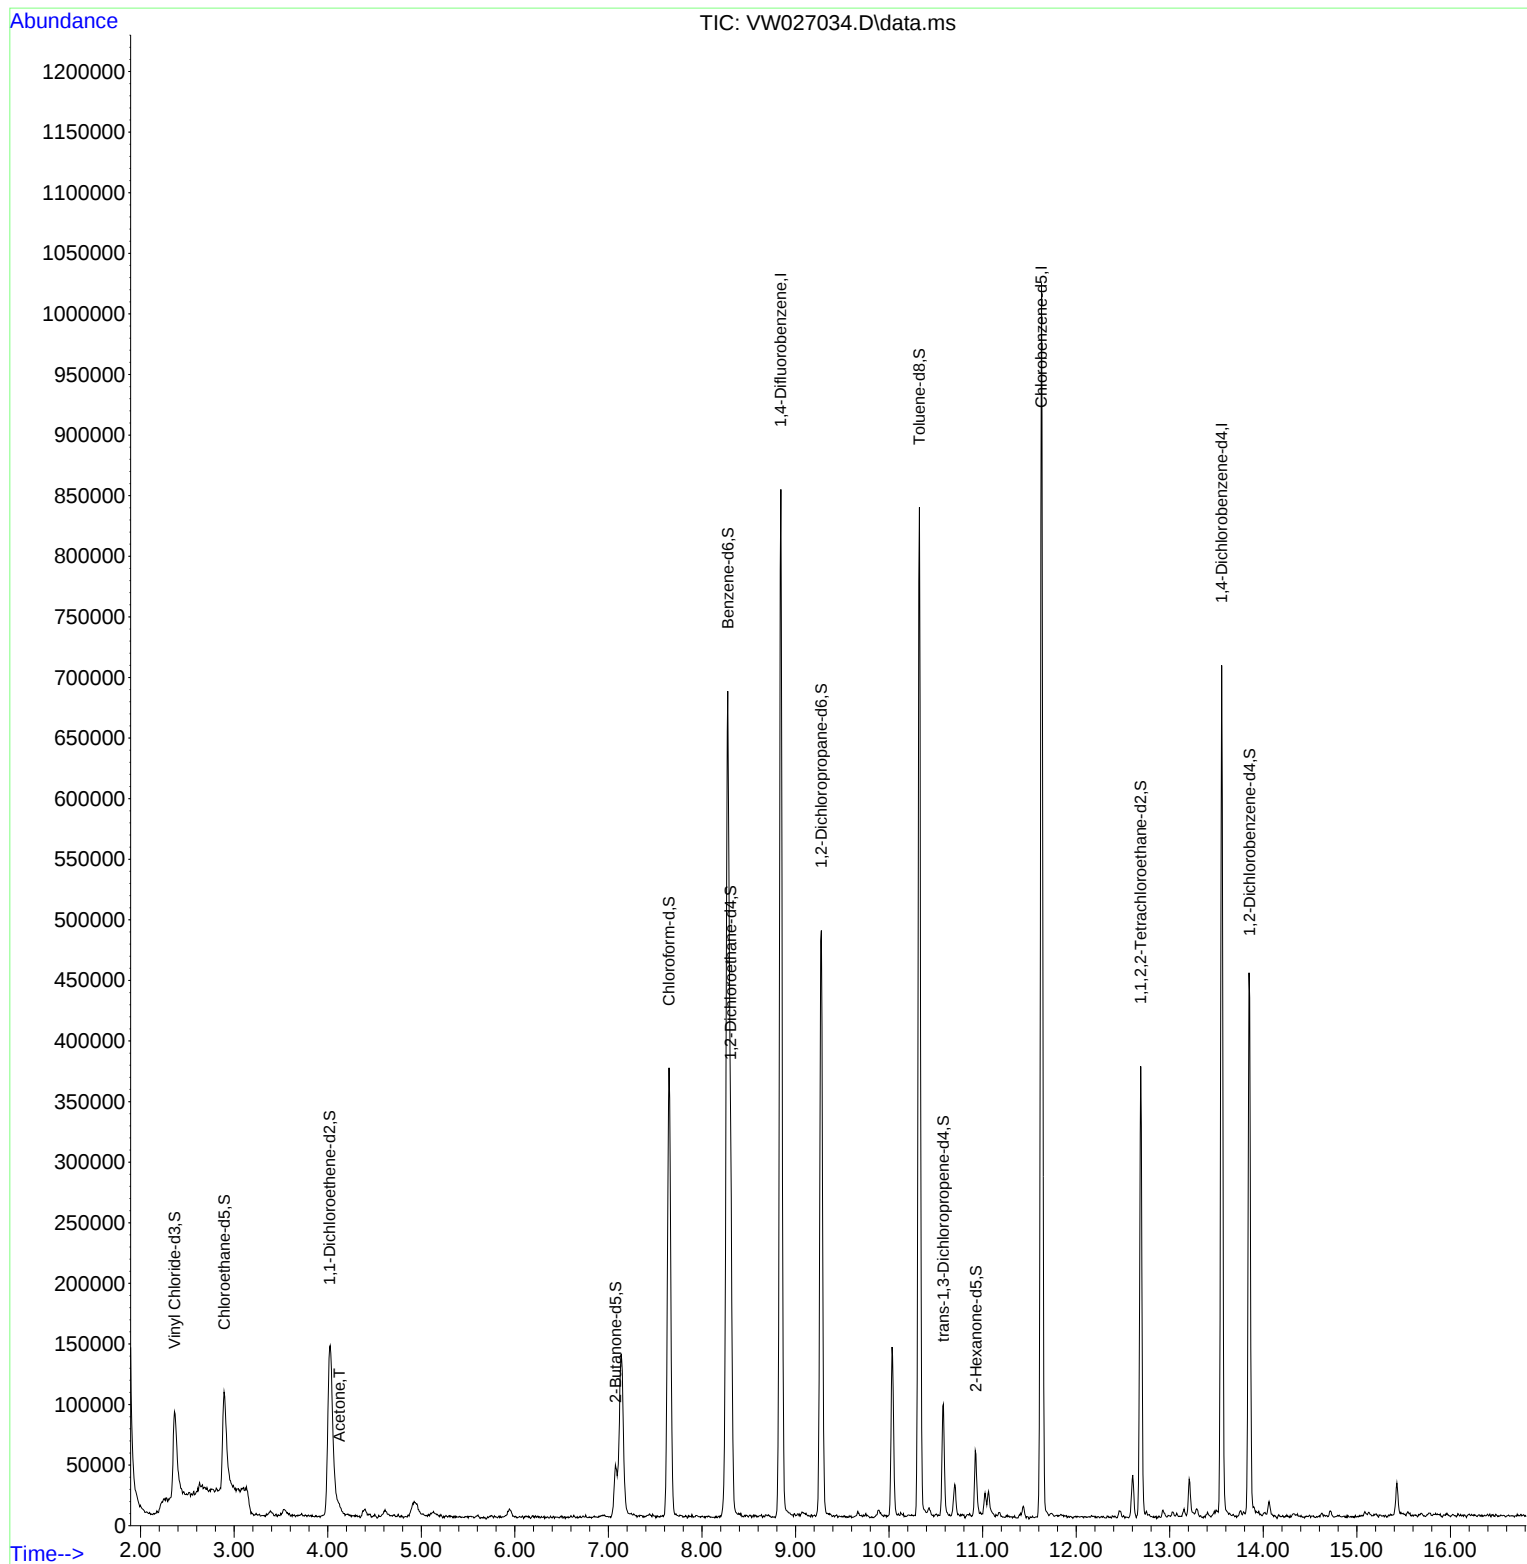

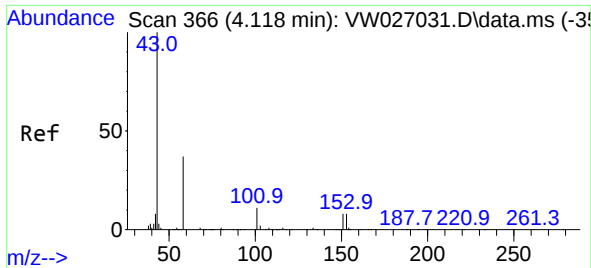

#13
Acetone
Concen: 4.095 ug/L
RT: 4.124 min Scan# 30
Delta R.T. 0.006 min
Lab File: VW027034.D
Acq: 11 Sep 2023 17:12

Instrument :
MSVOA_W
ClientSampleId :

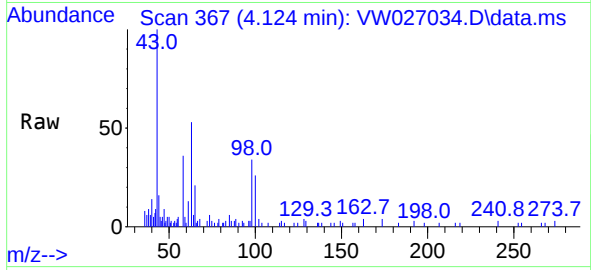

Tgt Ion: 43 Resp: 8859
Ion Ratio Lower Upper
43 100
58 42.2 0.0 66.4

