

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091123\
 Data File : VW027040.D
 Acq On : 11 Sep 2023 19:36
 Operator : SY/MD
 Sample : 04332-22
 Misc : 2.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 COAN1

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 09/12/2023
 Supervised By : Mahesh Dadoda 09/13/2023

Quant Time: Sep 12 01:15:58 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	621902	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	406151	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	113434	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	143229	12.891	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	51.560%		
7) Chloroethane-d5	2.893	69	152637	17.022	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	68.080%		
11) 1,1-Dichloroethene-d2	4.027	65	55054	13.445	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	53.800%		
21) 2-Butanone-d5	7.081	46	37070m	17.316	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	34.640%		
24) Chloroform-d	7.648	84	386226	20.871	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	83.480%		
26) 1,2-Dichloroethane-d4	8.307	65	202694	20.838	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	83.360%		
32) Benzene-d6	8.276	84	607906	22.819	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	91.280%		
36) 1,2-Dichloropropane-d6	9.270	67	226629	28.977	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	115.920%		
41) Toluene-d8	10.325	98	414618	17.190	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	68.760%		
43) trans-1,3-Dichloroprop...	10.581	79	23281	7.671	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	30.680%		
47) 2-Hexanone-d5	10.928	63	4397	6.022	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	12.040%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	155831	25.675	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	102.720%		
66) 1,2-Dichlorobenzene-d4	13.849	152	76106	19.399	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	77.600%		
Target Compounds						
13) Acetone	4.131	43	20888	11.143	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091123\
Data File : VW027040.D
Acq On : 11 Sep 2023 19:36
Operator : SY/MD
Sample : 04332-22
Misc : 2.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AN1

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 09/12/2023
Supervised By : Mahesh Dadoda 09/13/2023

Quant Time: Sep 12 01:15:58 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

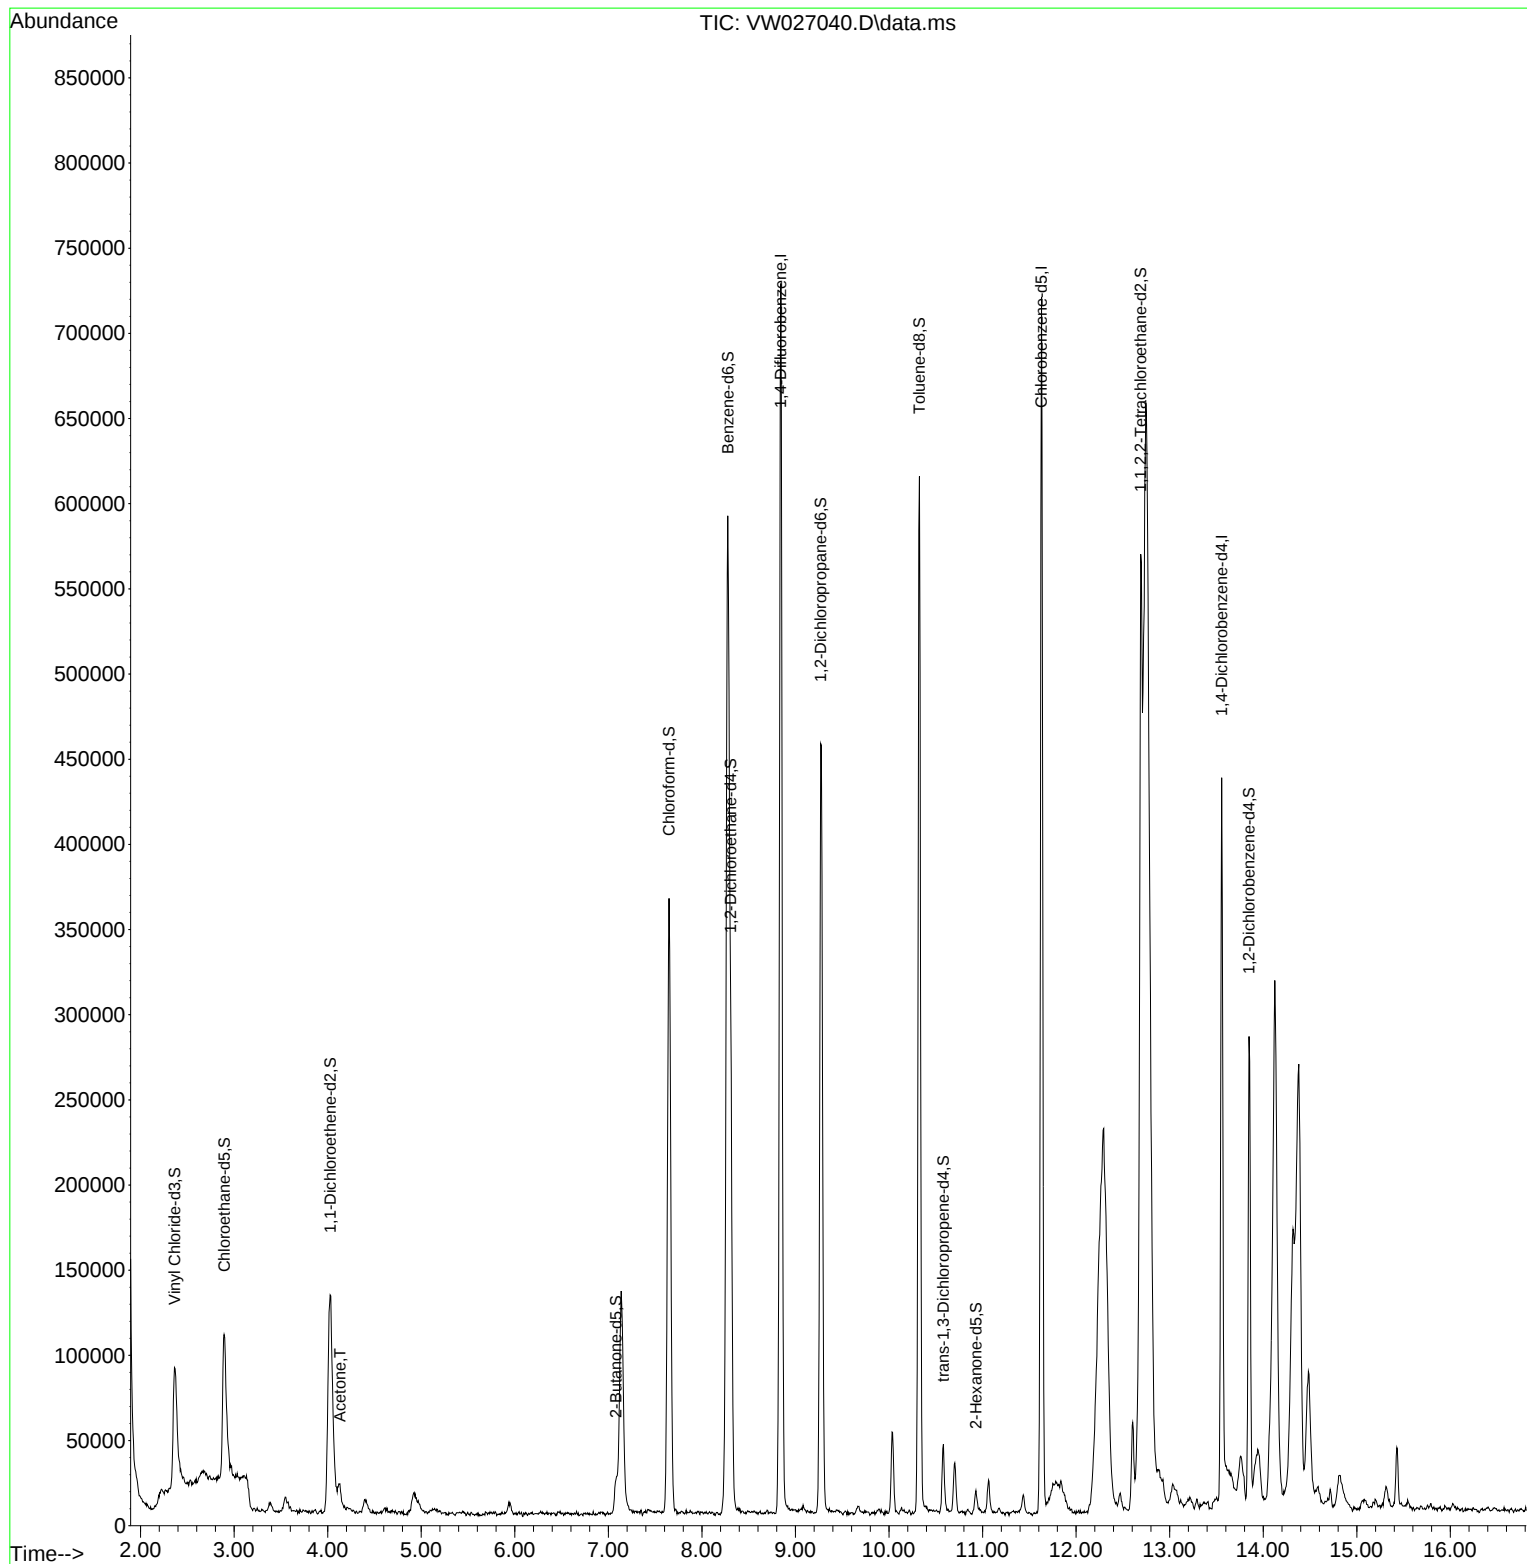

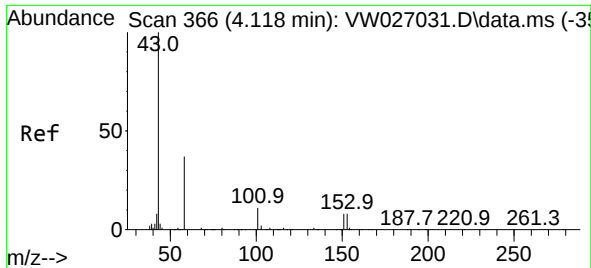

#13

Acetone

Concen: 11.143 ug/L

RT: 4.131 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW027040.D

Acq: 11 Sep 2023 19:36

Instrument :

MSVOA_W

ClientSampleId :

C0AN1

Tgt Ion: 43 Resp: 2088

Ion Ratio Lower Upper

43 100

58 36.2 0.0 66.4

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 09/12/2023

Supervised By :Mahesh Dadoda 09/13/2023

