

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091219\

Quantitation Report (QT Reviewed)

Data File : VW012934.D

Acq On : 12 Sep 2019 14:27

Operator : SY/VA

Sample : VW0912SBL01

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 03:00:15 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091219S.M

Quant Title : VOC Analysis

QLast Update : Fri Sep 13 02:47:59 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :


VBLK01

Manual Integrations

APPROVED

MMDadoda

9/13/2019 11:33:19 AM

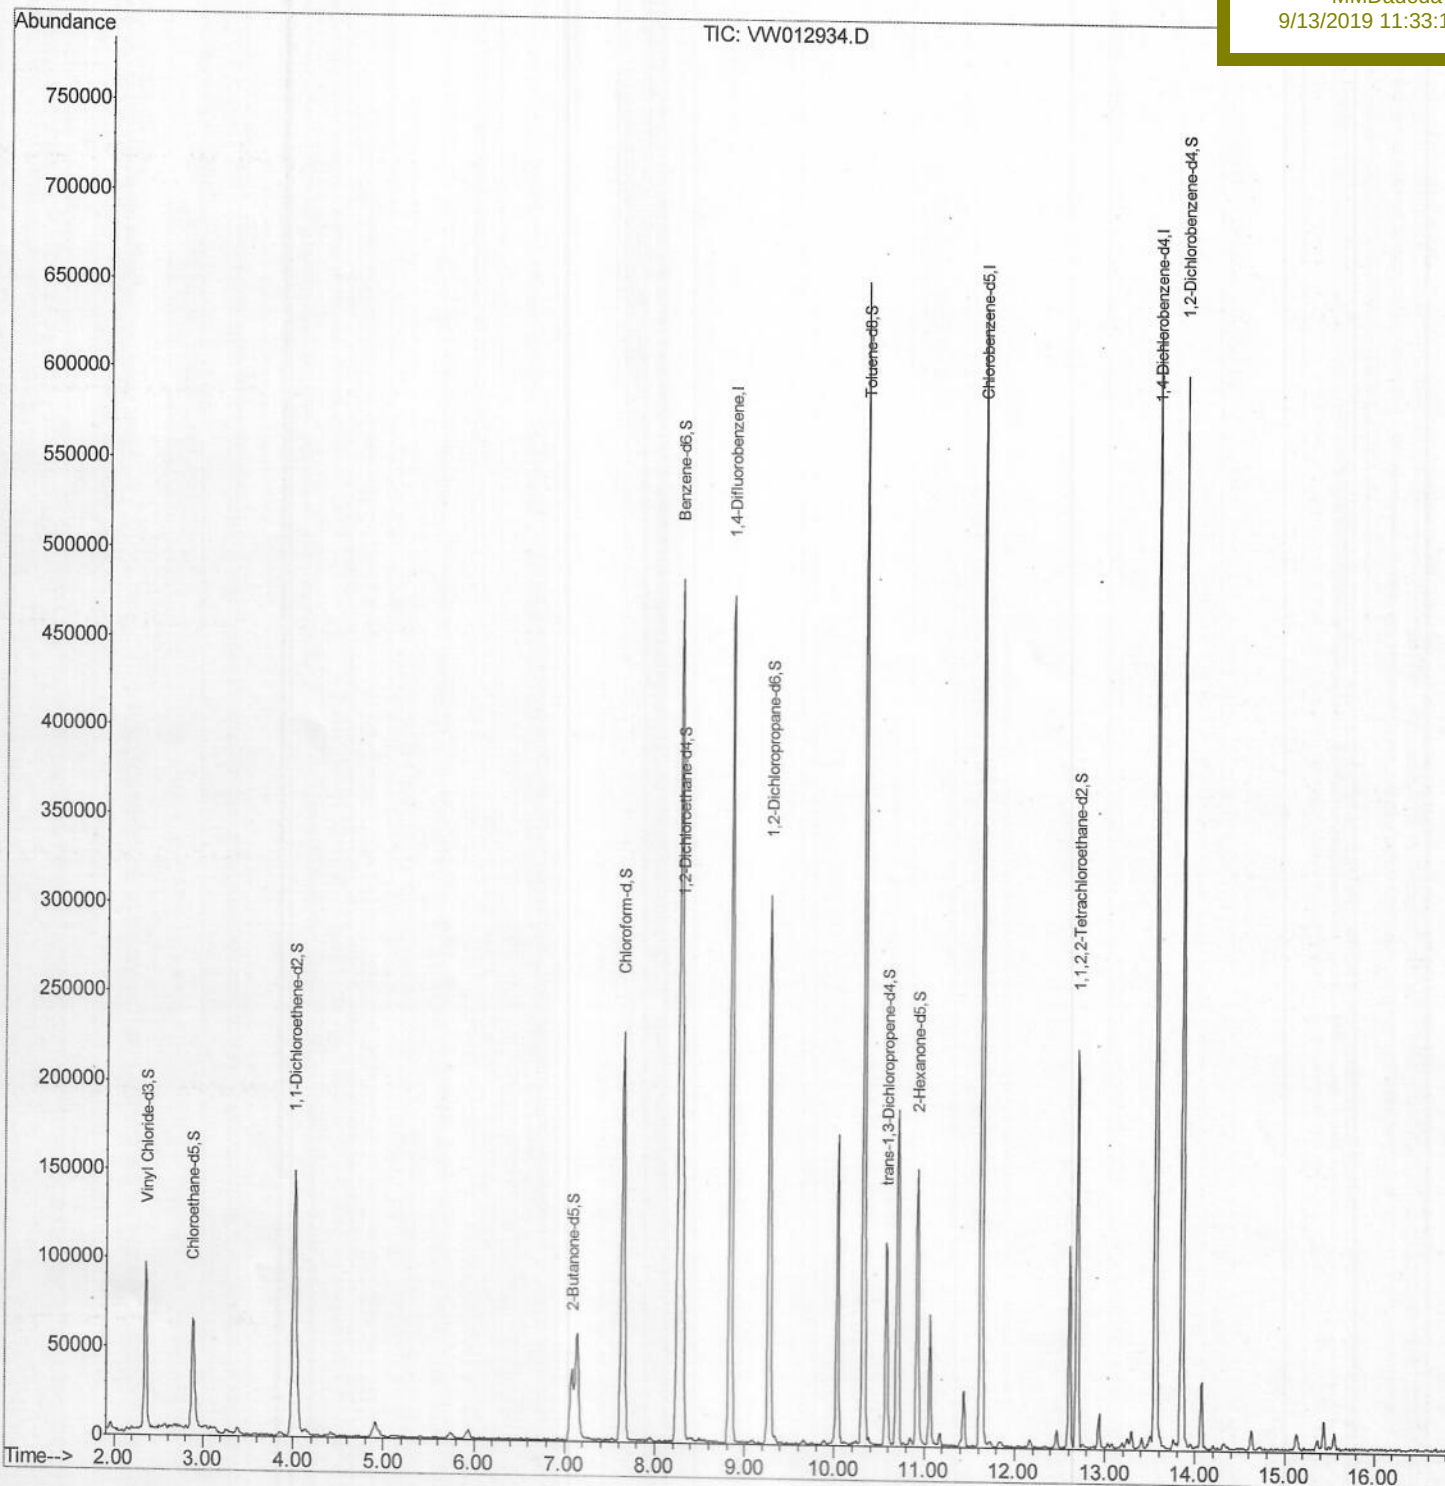

SOM2WLM091219S.M Fri Sep 13 02:58:31 2019

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091219\
Quantitation Report (Qedit)




Data File : VW012934.D
Acq On : 12 Sep 2019 14:27
Operator : SY/VA
Sample : VW0912SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 02:51:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091219S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 13 02:47:59 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
VBLK01

Manual Integrations
APPROVED

MMDadoda
9/13/2019 11:33:19 AM

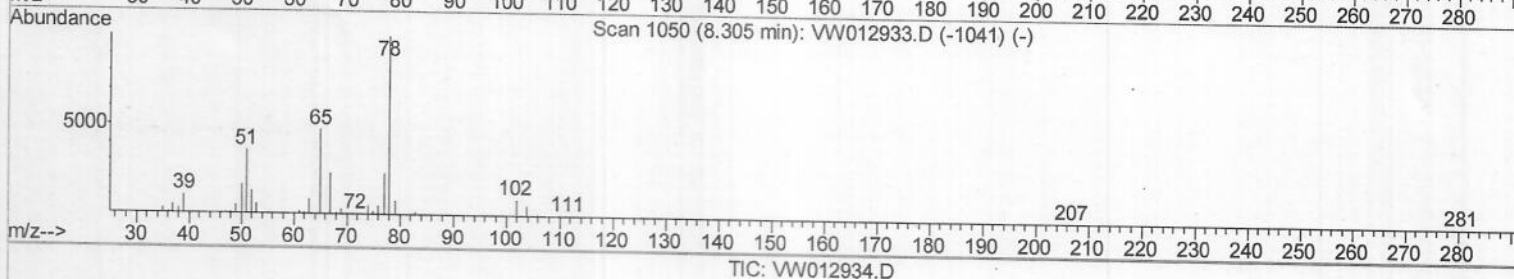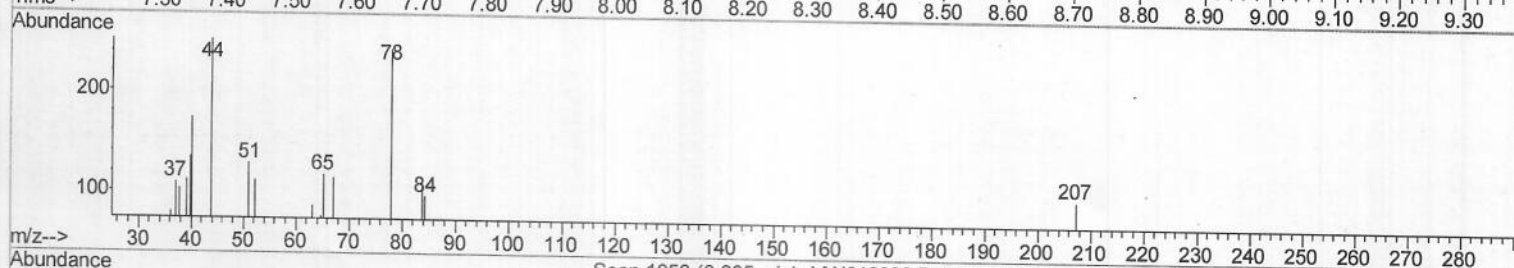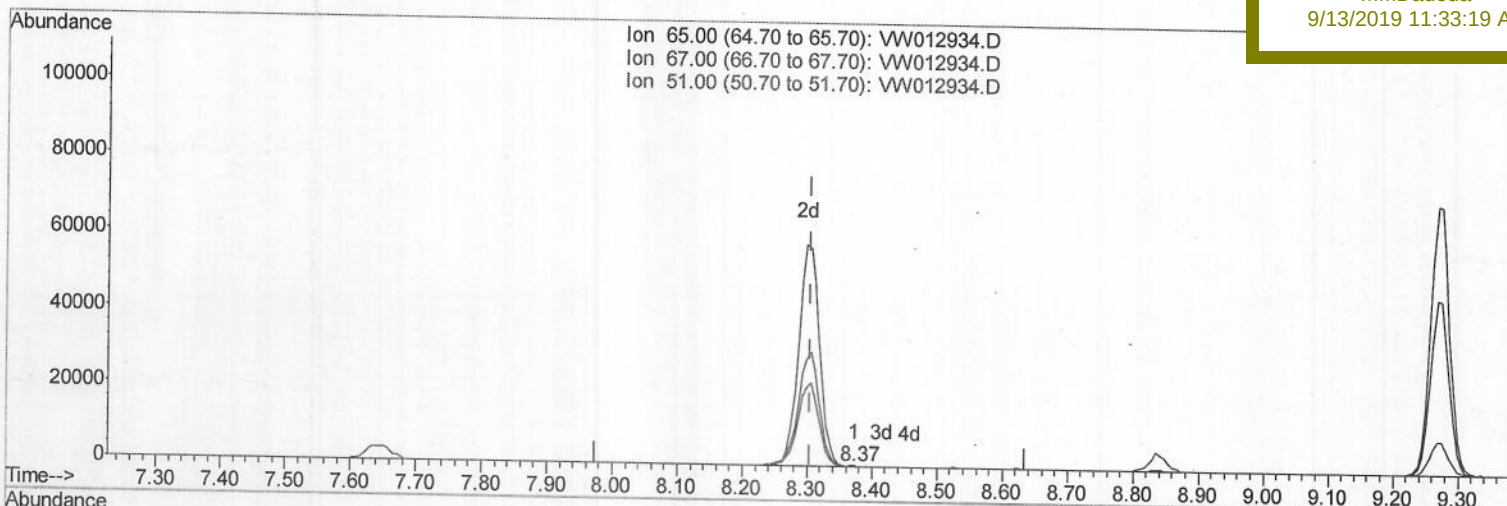

(26) 1,2-Dichloroethane-d4 (S)

8.372min (+0.067) 0.03ug/L

response 180

Ion	Exp%	Act%
65.00	100	100
67.00	51.50	47.78
51.00	111.50	90.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091219\

Quantitation Report (Qedit)

Data File : VW012934.D

Acq On : 12 Sep 2019 14:27

Operator : SY/VA

Sample : VW0912SBL01

Misc : 5.00G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 02:51:06 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091219S.M

Quant Title : VOC Analysis

QLast Update : Fri Sep 13 02:47:59 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampled :




VBLK01

Manual Integrations

APPROVED

MMDadoda

9/13/2019 11:33:19 AM

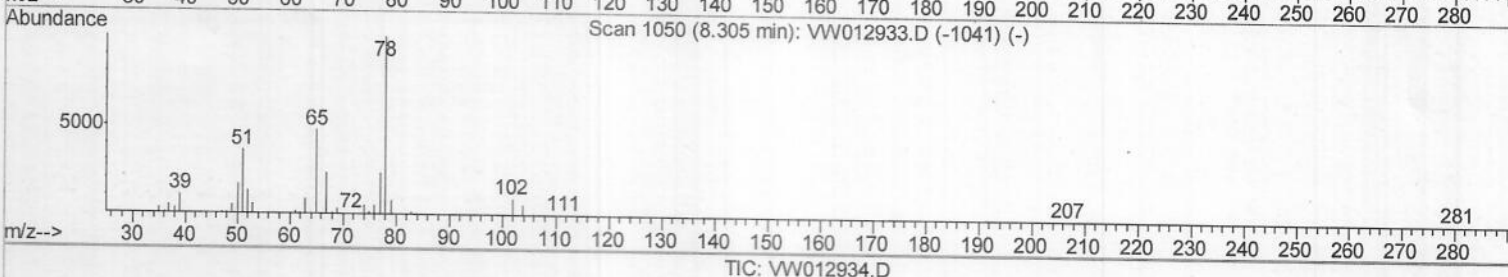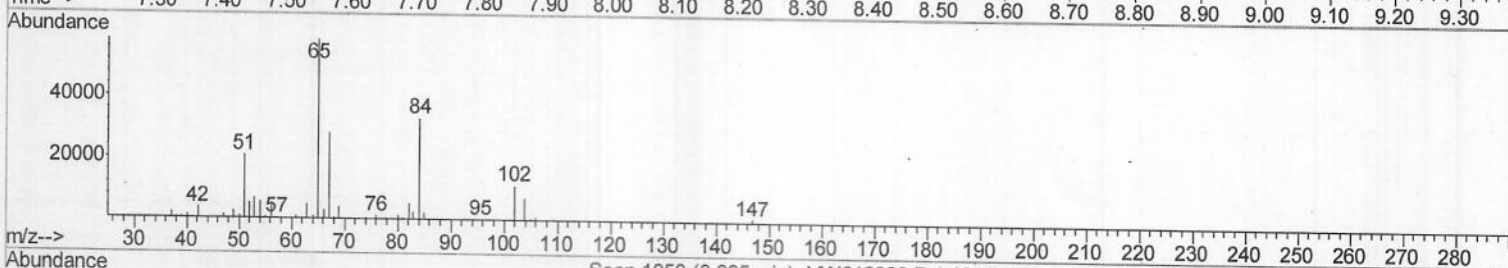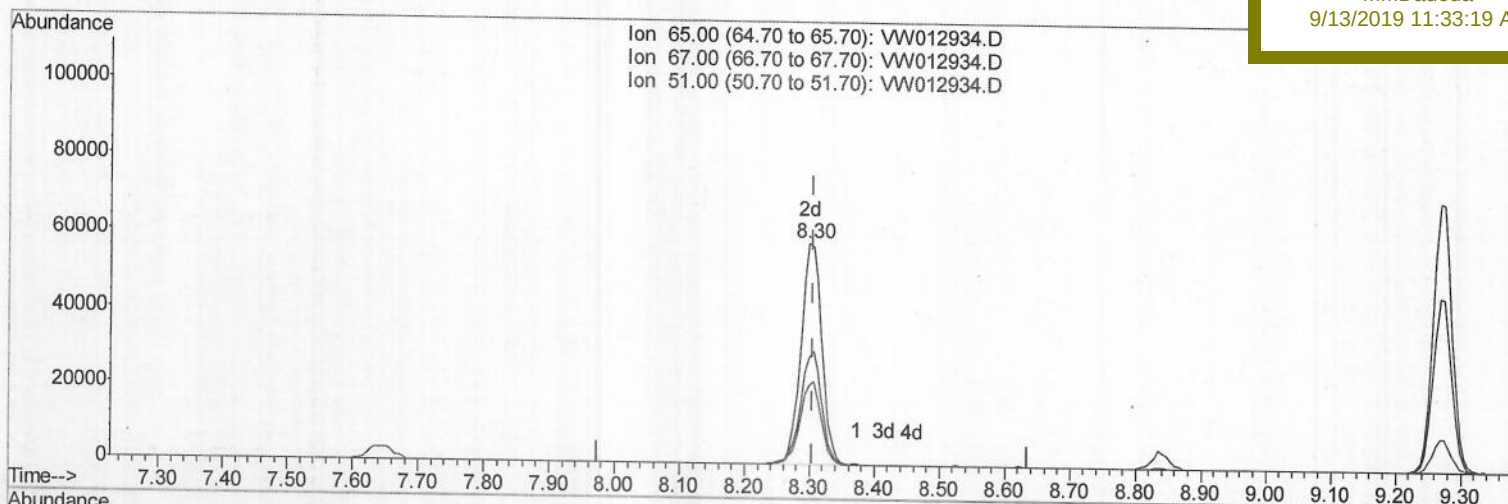

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 24.39ug/L m > MD 09/16/19

response 129653

Ion	Exp%	Act%
-----	------	------

65.00	100	100
-------	-----	-----

67.00	51.50	0.07#
-------	-------	-------

51.00	111.50	0.12#
-------	--------	-------

0.00	0.00	0.00
------	------	------

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091219\
Quantitation Report (QT Reviewed)

Data File : VW012934.D
Acq On : 12 Sep 2019 14:27
Operator : SY/VA
Sample : VW0912SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 03:00:15 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091219S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 13 02:47:59 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
VBLK01

Manual Integrations
APPROVED

MMDadoda
9/13/2019 11:33:19 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	393472	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	350165	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	169690	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	102678	25.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.80%
7) Chloroethane-d5	2.89	69	83108	25.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.12%
10) 1,1-Dichloroethene-d2	4.01	63	176305	18.63	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.52%
20) 2-Butanone-d5	7.07	46	72338	48.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.78%
24) Chloroform-d	7.65	84	231791	23.29	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.16%
26) 1,2-Dichloroethane-d4	8.30	65	129653m	24.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.56%
29) Benzene-d6	8.27	84	445284	24.92	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.68%
33) 1,2-Dichloropropane-d6	9.27	67	142252	24.12	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.48%
37) Toluene-d8	10.32	98	422191	24.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.28%
38) trans-1,3-Dichloropropene-	10.57	79	61454	23.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.60%
39) 2-Hexanone-d5	10.92	63	52367	47.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.10%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	107368	24.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	162345	25.12	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.48%

MD
09/16/19

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed