

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW091219\
 Data File : VW012941.D
 Acq On : 12 Sep 2019 18:32
 Operator : SY/VA
 Sample : K4811-07
 Misc : 5.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 ETOG6

Quant Time: Sep 13 03:54:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091219S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 13 02:47:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	383771	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	331161	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	134466	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	78507	20.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.36%
7) Chloroethane-d5	2.89	69	63248	19.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.68%
10) 1,1-Dichloroethene-d2	4.01	63	133100	14.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.68%
20) 2-Butanone-d5	7.07	46	88061	61.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.04%
24) Chloroform-d	7.65	84	192624	19.85	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.40%
26) 1,2-Dichloroethane-d4	8.30	65	119000	22.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.84%
29) Benzene-d6	8.27	84	349513	20.69	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.76%
33) 1,2-Dichloropropane-d6	9.27	67	120118	21.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.12%
37) Toluene-d8	10.32	98	326344	20.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.12%
38) trans-1,3-Dichloropropene-	10.57	79	54537	22.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.76%
39) 2-Hexanone-d5	10.92	63	61680	58.60	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.20%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	106149	25.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.84%
61) 1,2-Dichlorobenzene-d4	13.85	152	114137	22.29	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.16%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.12	43	3262	2.623	ug/L	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW091219\
Data File : VW012941.D
Acq On : 12 Sep 2019 18:32
Operator : SY/VA
Sample : K4811-07
Misc : 5.38G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETOG6

Quant Time: Sep 13 03:54:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM091219S.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 13 02:47:59 2019
Response via : Initial Calibration

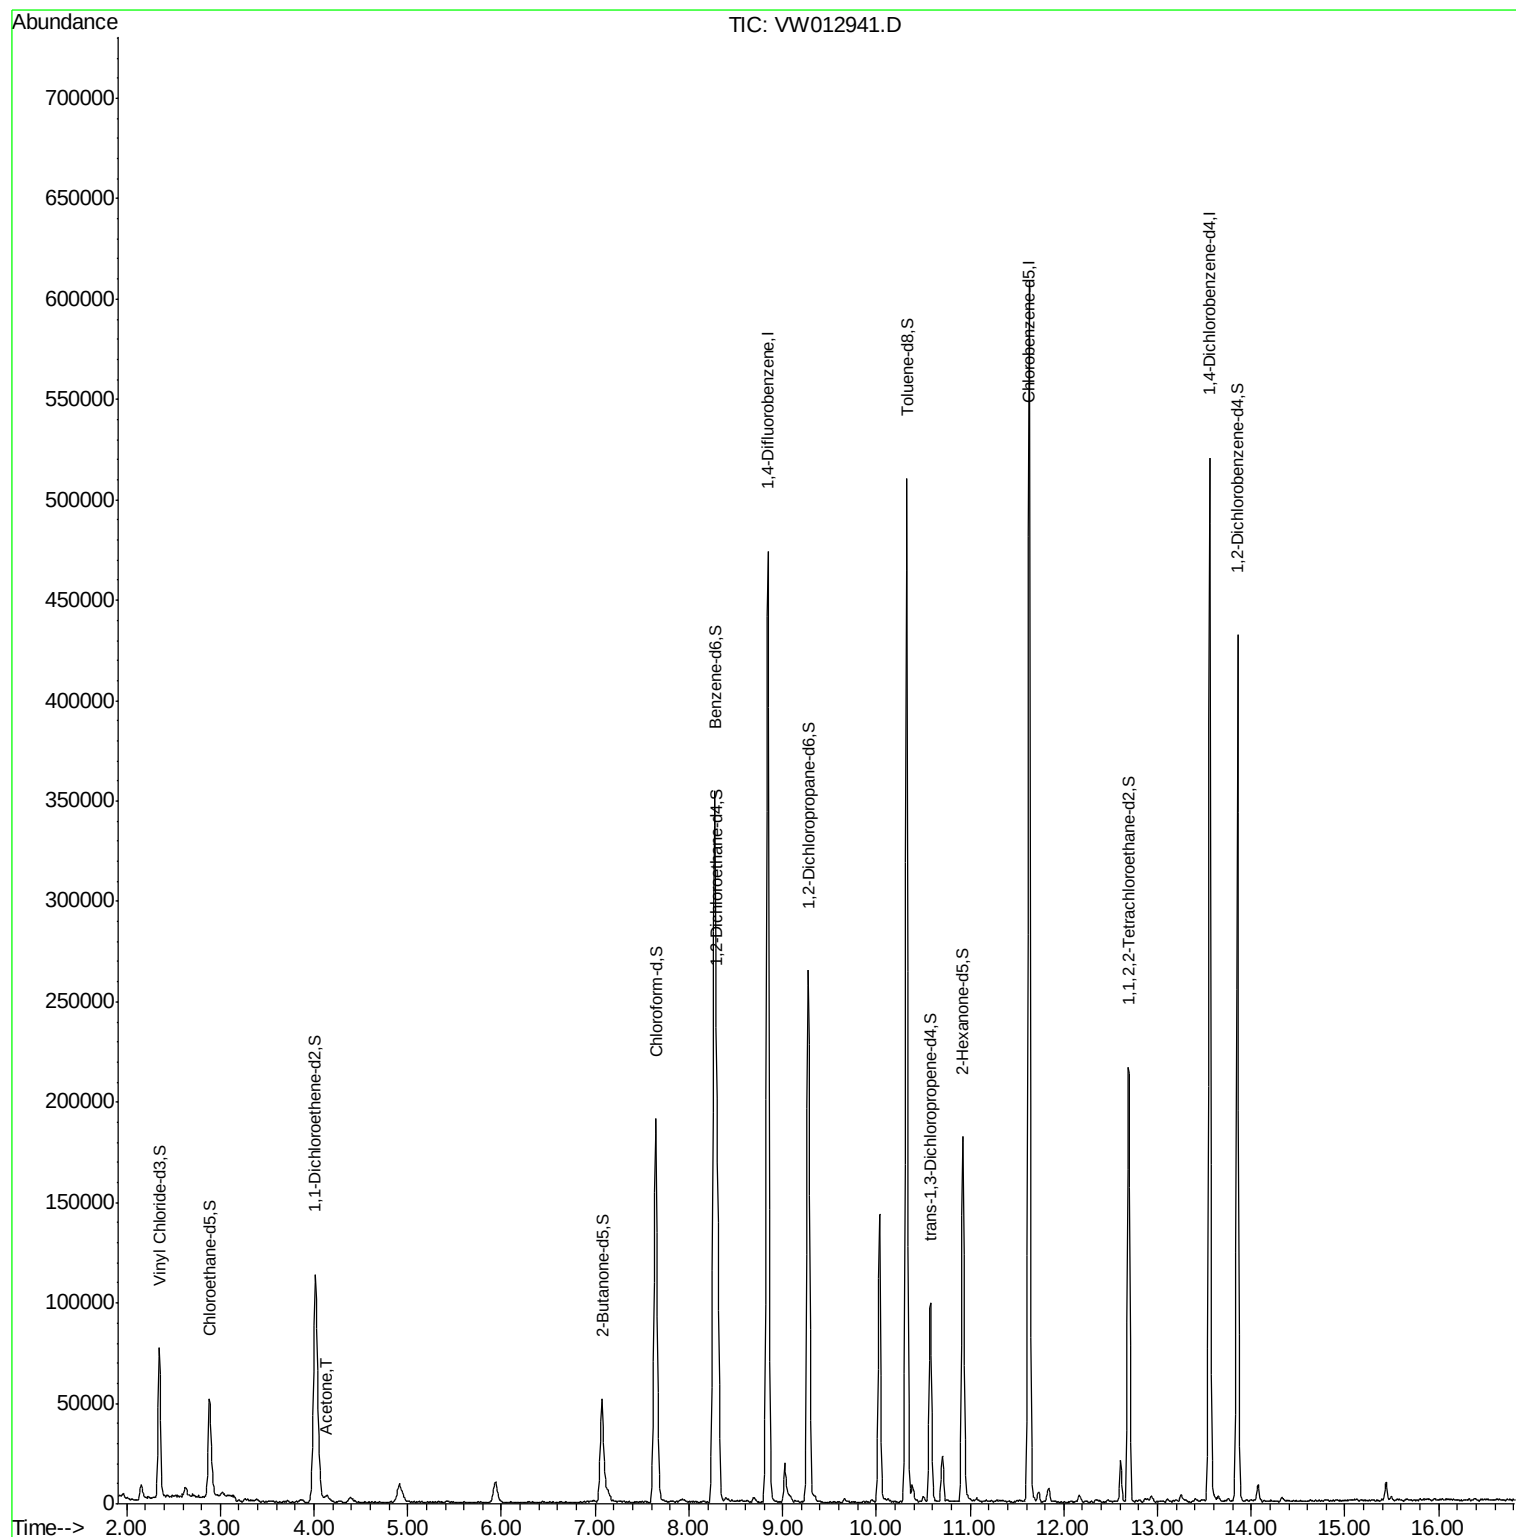

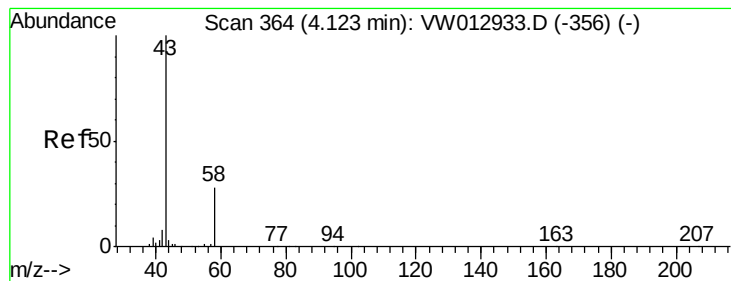

#13

Acetone

Concen: 2.623 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.00 min

Lab File: VW012941.D

Acq: 12 Sep 2019 18:32

Instrument :
MSVOA_W
ClientSampleId :
ETOG6

Tgt Ion: 43 Resp: 3262

Ion Ratio Lower Upper

43 100

58 13.1 0.0 59.4

