

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027067.D
 Acq On : 12 Sep 2023 14:41
 Operator : SY/MD
 Sample : 04387-10RE
 Misc : 2.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6RE




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
 Dadoda

09/13/2023

Quant Time: Sep 13 03:08:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

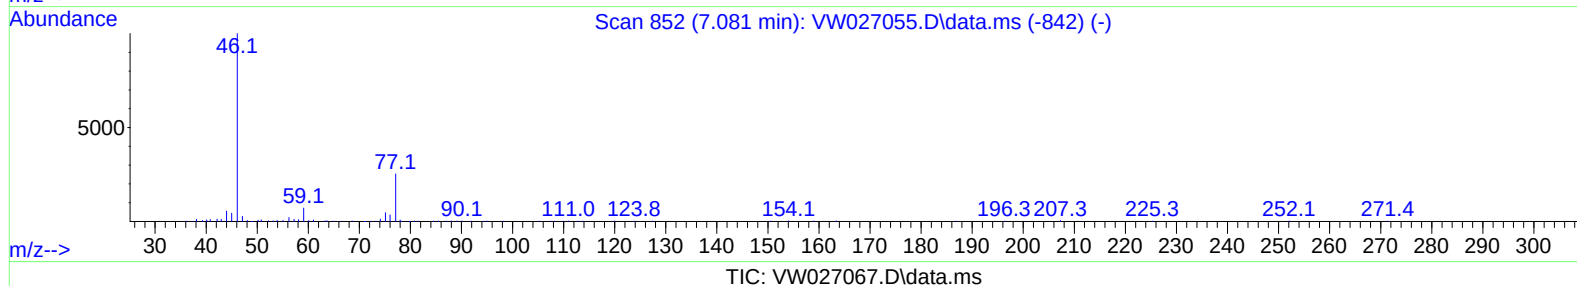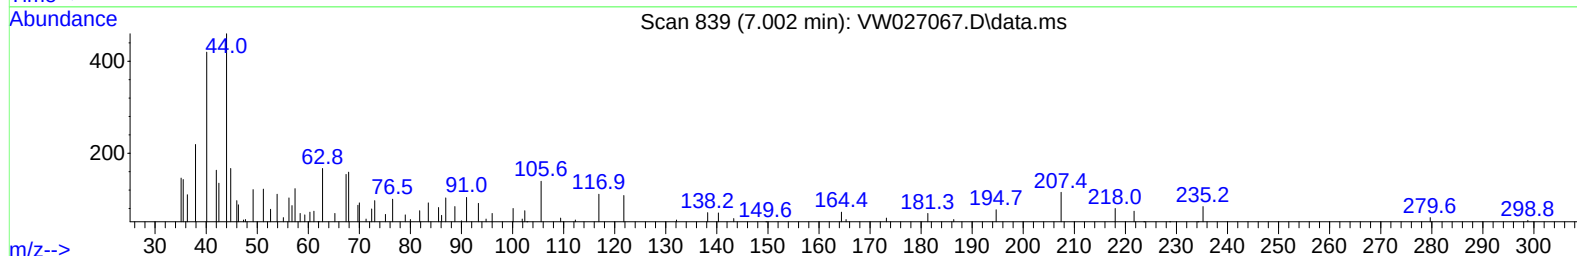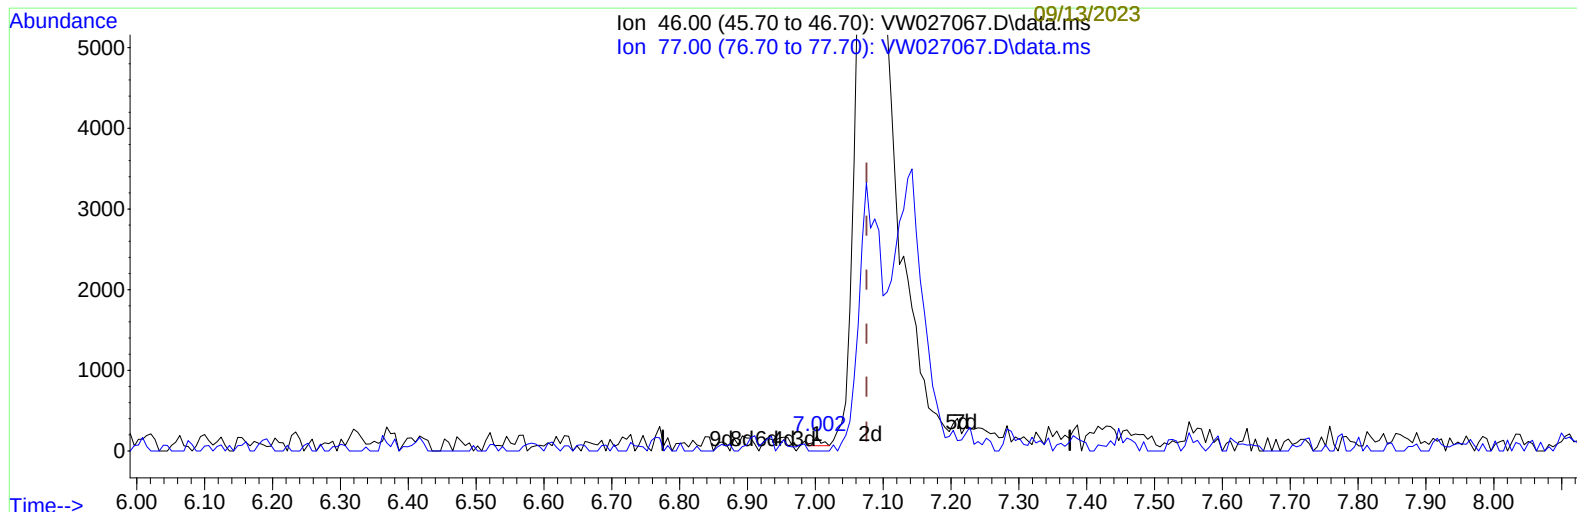

(21) 2-Butanone-d5 (S)

7.002min (-0.073) 0.03 ug/L

response	85	
Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.40	32.94
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027067.D
 Acq On : 12 Sep 2023 14:41
 Operator : SY/MD
 Sample : 04387-10RE
 Misc : 2.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
 Dadoda

Quant Time: Sep 13 03:08:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

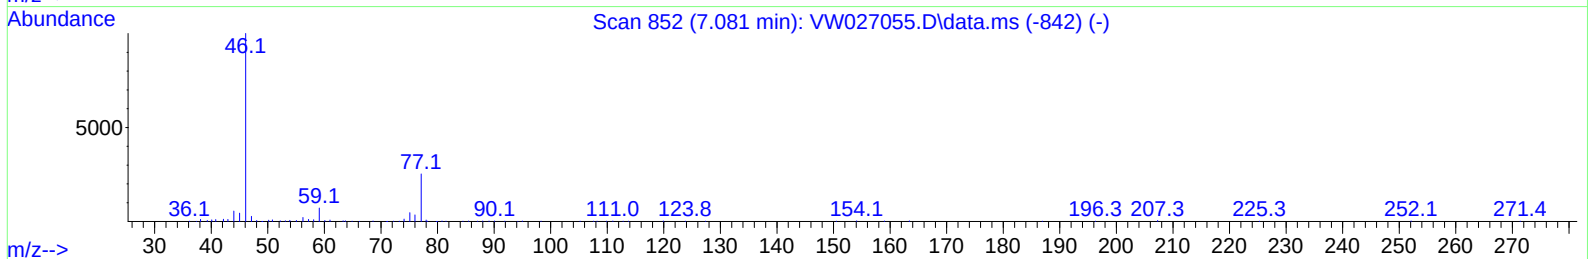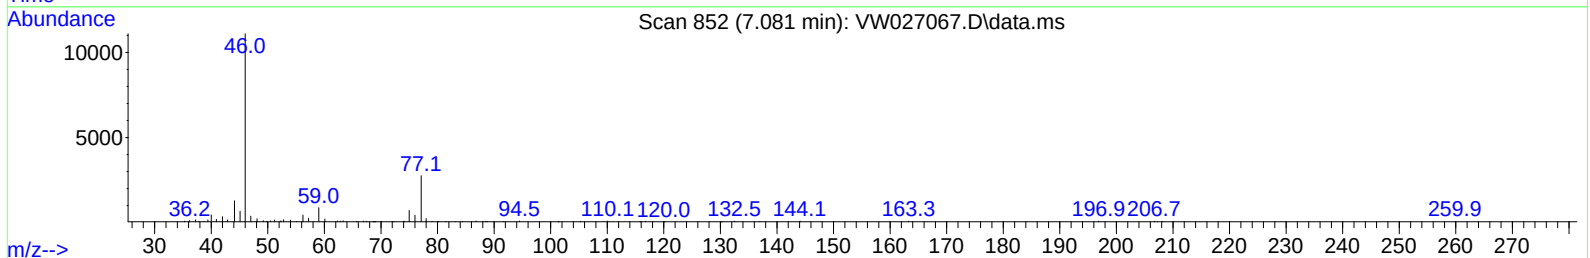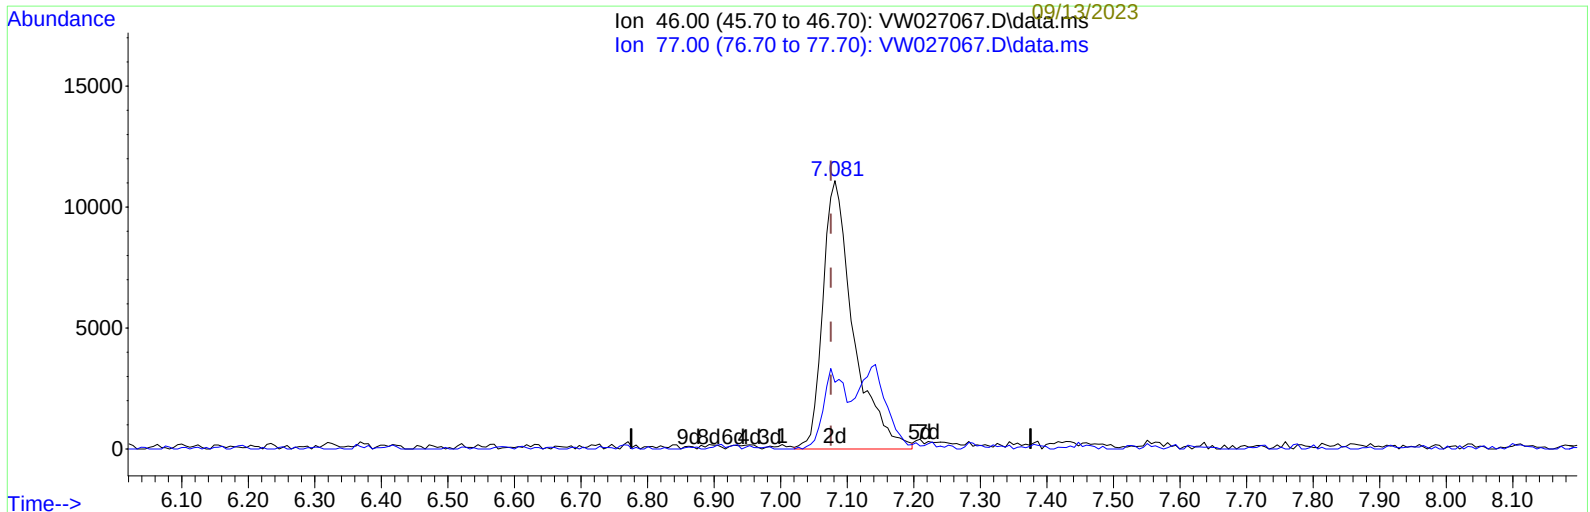

TIC: VW027067.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (+ 0.006) 13.37 ug/L m

response 35326

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.40	0.08#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027067.D
 Acq On : 12 Sep 2023 14:41
 Operator : SY/MD
 Sample : 04387-10RE
 Misc : 2.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6RE




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
 Dadoda

09/13/2023

Quant Time: Sep 13 03:08:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

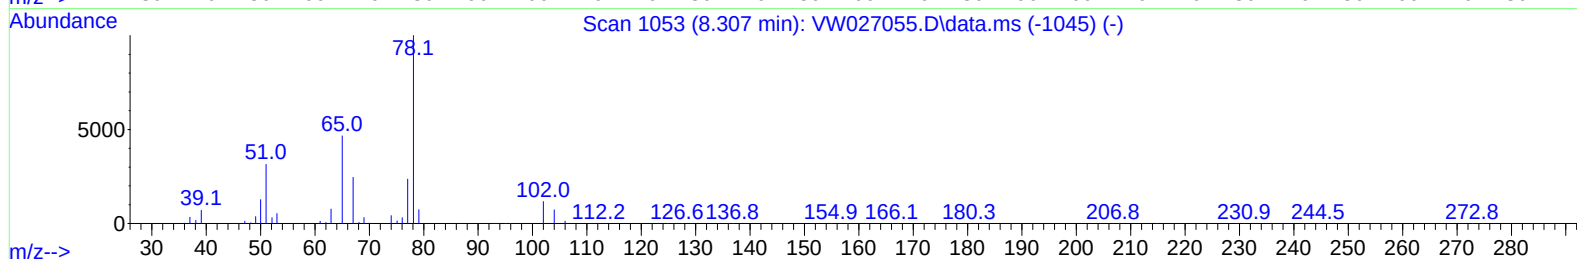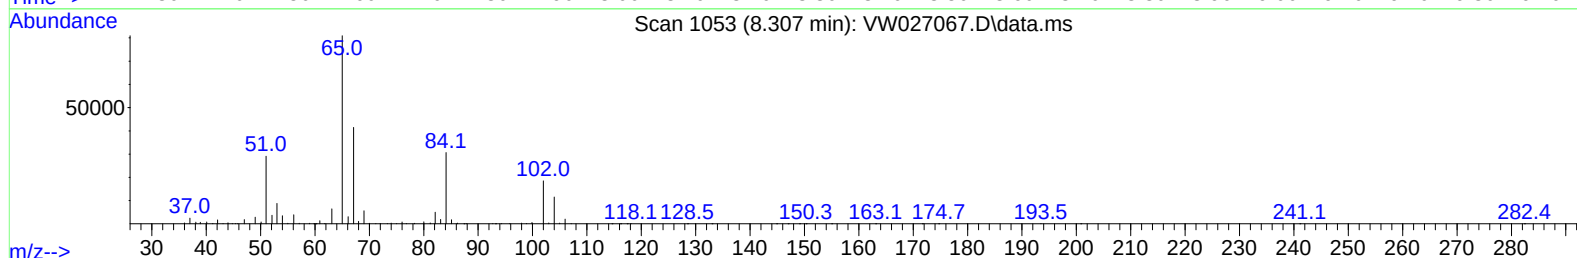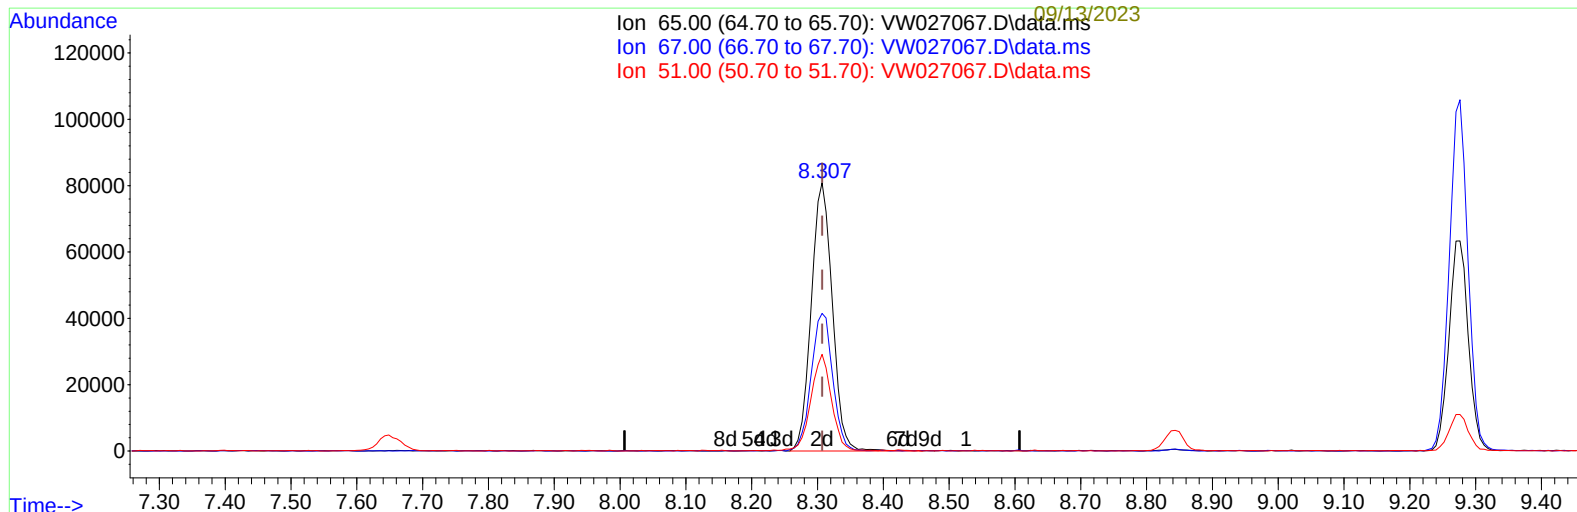

TIC: VW027067.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 14.99 ug/L m

response 180024

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.04#
51.00	110.30	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027067.D
 Acq On : 12 Sep 2023 14:41
 Operator : SY/MD
 Sample : 04387-10RE
 Misc : 2.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6RE




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
 Dadoda

09/13/2023

Quant Time: Sep 13 03:08:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

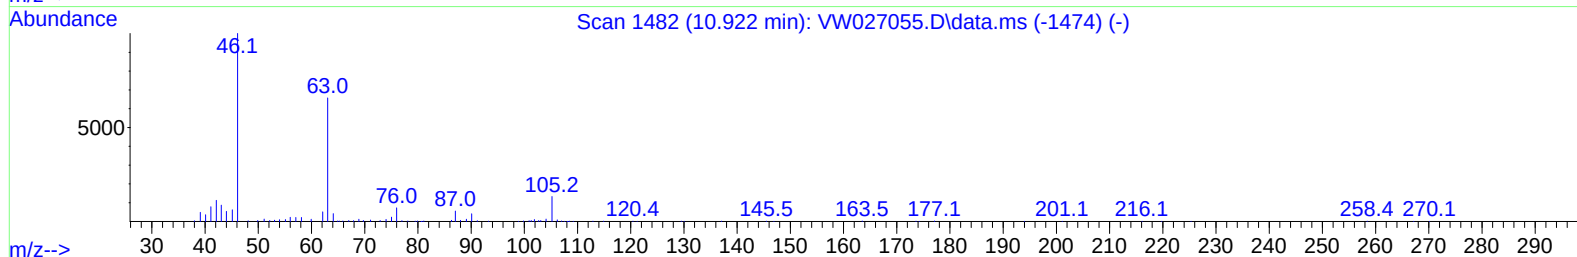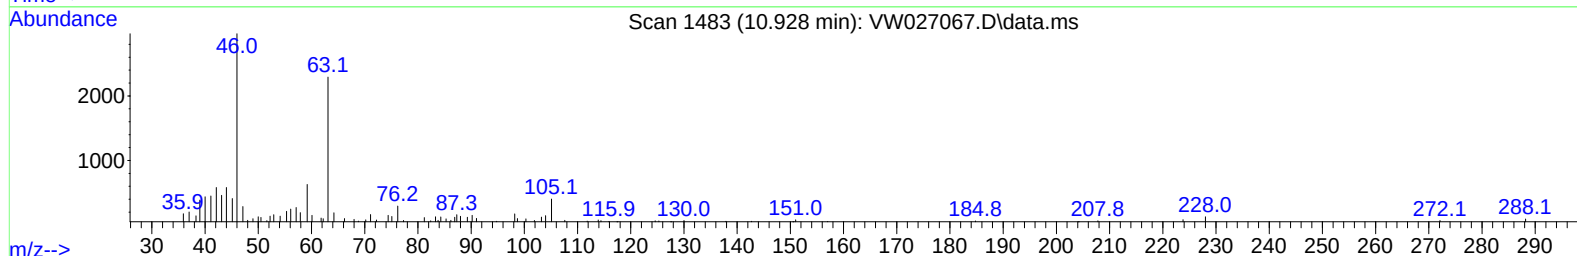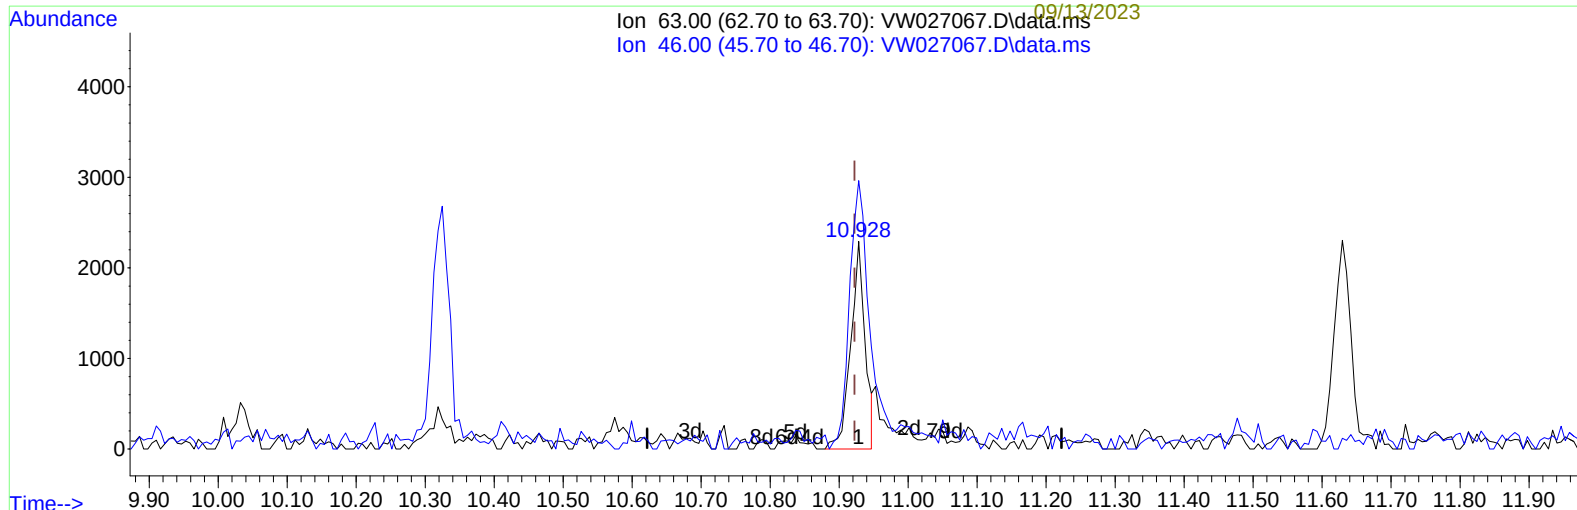

TIC: VW027067.D\data.ms

(47) 2-Hexanone-d5 (S)

10.928min (+ 0.006) 3.15 ug/L

response 3344

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	173.60	180.23
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027067.D
 Acq On : 12 Sep 2023 14:41
 Operator : SY/MD
 Sample : 04387-10RE
 Misc : 2.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6RE




Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
 Dadoda

09/13/2023

Quant Time: Sep 13 03:08:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

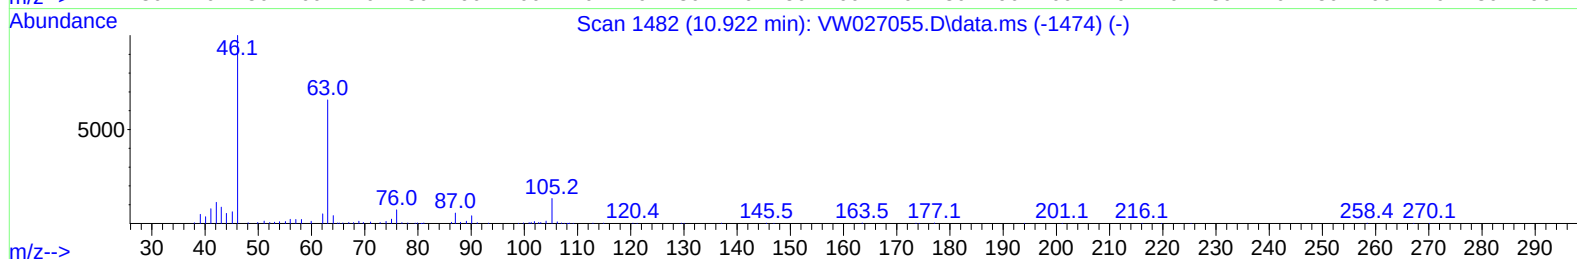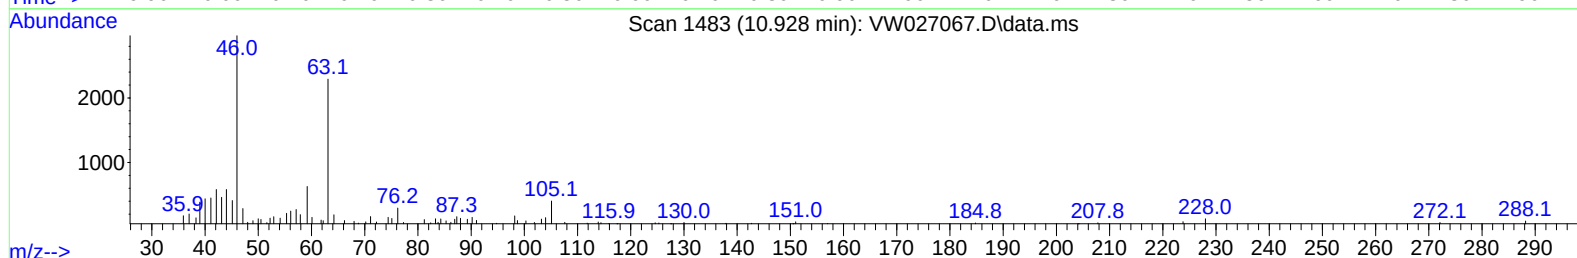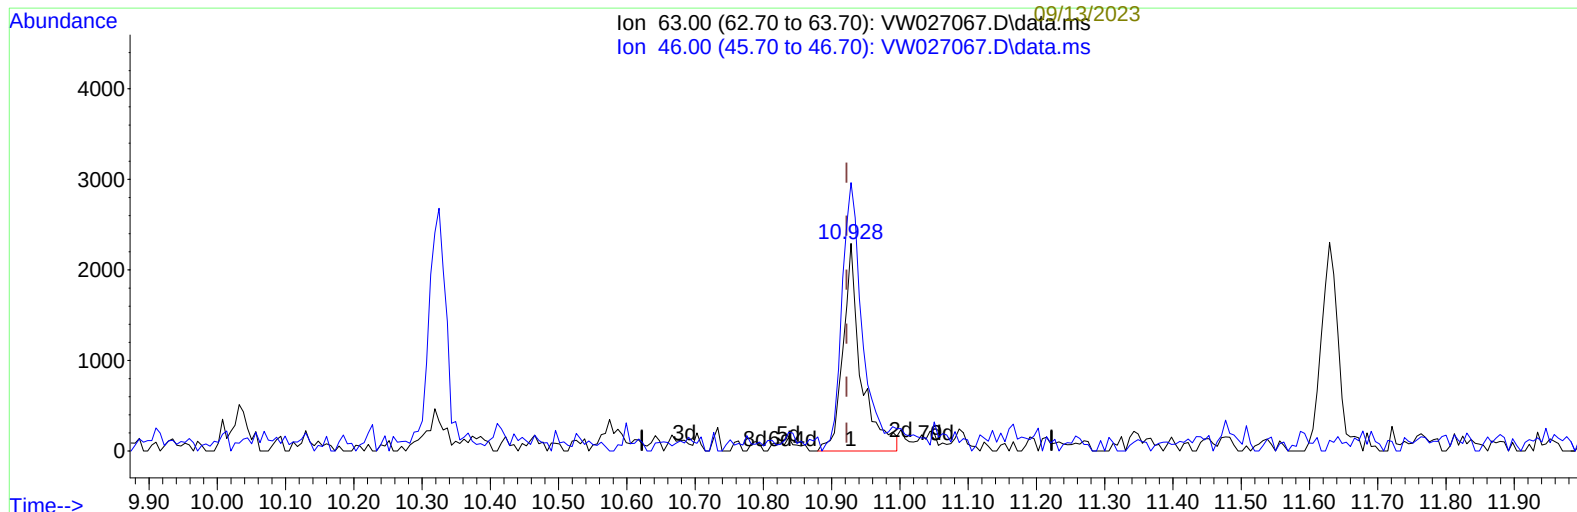

TIC: VW027067.D\data.ms

(47) 2-Hexanone-d5 (S)

10.928min (+ 0.006) 3.96 ug/L m

response 4207

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	173.60	143.26
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027067.D
 Acq On : 12 Sep 2023 14:41
 Operator : SY/MD
 Sample : 04387-10RE
 Misc : 2.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
 Dadoda
 09/13/2023

Quant Time: Sep 13 03:08:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	767683	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	590878	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	163549	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	124064	9.046	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	36.200%	
7) Chloroethane-d5	2.899	69	126362	11.416	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	45.680%	
11) 1,1-Dichloroethene-d2	4.027	65	47521	9.402	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	37.600%#	
21) 2-Butanone-d5	7.081	46	35326m	13.368	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	26.740%	
24) Chloroform-d	7.648	84	348999	15.278	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	61.120%	
26) 1,2-Dichloroethane-d4	8.307	65	180024m	14.993	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	59.960%#	
32) Benzene-d6	8.270	84	596115	15.381	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	61.520%	
36) 1,2-Dichloropropane-d6	9.276	67	210238	18.477	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	73.920%	
41) Toluene-d8	10.325	98	458587	13.069	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	52.280%	
43) trans-1,3-Dichloroprop...	10.575	79	22282	5.046	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	20.200%#	
47) 2-Hexanone-d5	10.928	63	4207m	3.960	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	7.920%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	150828	17.082	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	68.320%	
66) 1,2-Dichlorobenzene-d4	13.849	152	86603	15.310	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	61.240%#	
Target Compounds					Qvalue	
13) Acetone	4.125	43	20876	9.022	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
Data File : VW027067.D
Acq On : 12 Sep 2023 14:41
Operator : SY/MD
Sample : 04387-10RE
Misc : 2.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
Supervised By :Mahesh Dadoda 09/13/2023

Supervised By :Mahesh
Dadoda
09/13/2023

Quant Time: Sep 13 03:08:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

