

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027056.D
 Acq On : 12 Sep 2023 10:17
 Operator : SY/MD
 Sample : VW0912SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Quant Time: Sep 13 03:49:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	525330	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	520299	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	256544	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	168637	17.968	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.880%
7) Chloroethane-d5	2.899	69	152609	20.147	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.600%
11) 1,1-Dichloroethene-d2	4.027	65	73211	21.166	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.680%
21) 2-Butanone-d5	7.075	46	80979	44.779	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.560%
24) Chloroform-d	7.648	84	398168	25.471	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.880%
26) 1,2-Dichloroethane-d4	8.307	65	204059	24.835	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.360%
32) Benzene-d6	8.276	84	827090	24.235	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.960%
36) 1,2-Dichloropropane-d6	9.276	67	243603	24.314	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.240%
41) Toluene-d8	10.325	98	726035	23.498	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.000%
43) trans-1,3-Dichloroprop...	10.581	79	87306	22.455	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.800%
47) 2-Hexanone-d5	10.922	63	41811	44.700	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.400%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	205925	26.485	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.960%
66) 1,2-Dichlorobenzene-d4	13.849	152	253995	28.626	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	114.520%
Target Compounds						
13) Acetone	4.125	43	5301	3.348	ug/L	Qvalue 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
Data File : VW027056.D
Acq On : 12 Sep 2023 10:17
Operator : SY/MD
Sample : VW0912SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK569

Quant Time: Sep 13 03:49:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

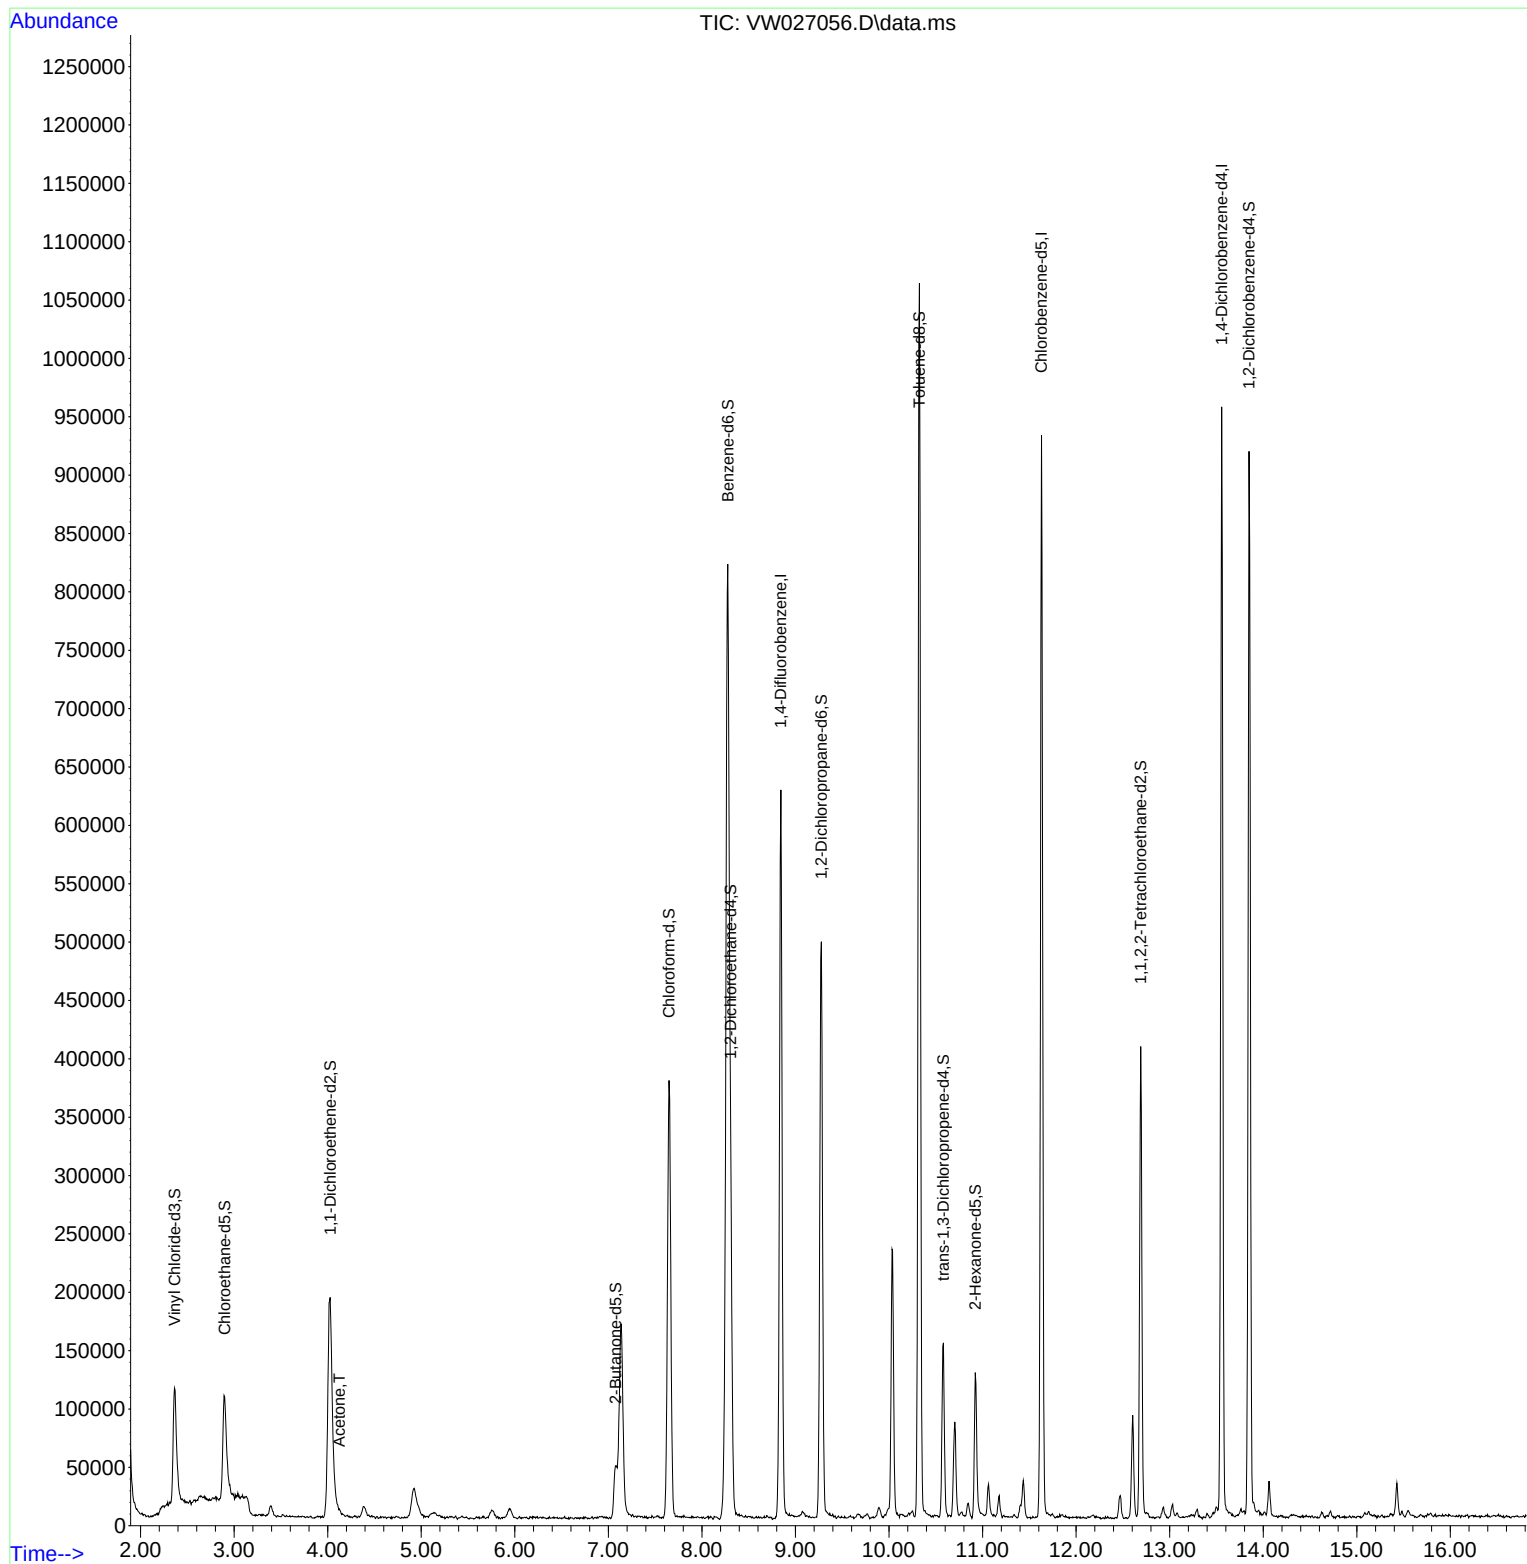

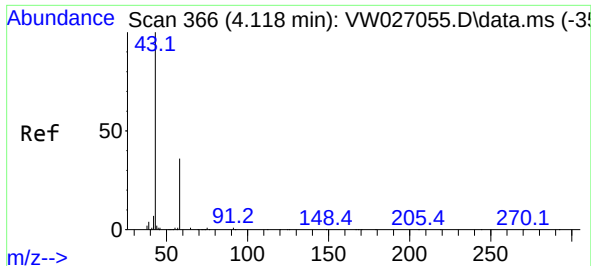

#13
 Acetone
 Concen: 3.348 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW027056.D
 Acq: 12 Sep 2023 10:17

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK569

Tgt Ion: 43 Resp: 5301
 Ion Ratio Lower Upper
 43 100
 58 15.1 0.0 66.4

