

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027059.D
 Acq On : 12 Sep 2023 11:29
 Operator : SY/MD
 Sample : 04332-22RE
 Misc : 2.70g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AN1RE

Quant Time: Sep 13 03:07:10 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	586550	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	409941	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	108898	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	139822	13.343	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	53.360%
7) Chloroethane-d5	2.893	69	146293	17.298	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.200%
11) 1,1-Dichloroethene-d2	4.021	65	56393	14.602	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.400%
21) 2-Butanone-d5	7.075	46	49934	24.730	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	49.460%
24) Chloroform-d	7.648	84	369528	21.172	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.680%
26) 1,2-Dichloroethane-d4	8.307	65	194718	21.225	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.880%
32) Benzene-d6	8.276	84	609603	22.671	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.680%
36) 1,2-Dichloropropane-d6	9.276	67	219220	27.771	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.080%
41) Toluene-d8	10.325	98	431506	17.725	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.920%
43) trans-1,3-Dichloroprop...	10.581	79	36926	12.054	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	48.200%
47) 2-Hexanone-d5	10.928	63	8240	11.181	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	22.360%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	154073	25.151	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	77214	20.501	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.000%
Target Compounds					Qvalue	
13) Acetone	4.131	43	15017	8.494	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
Data File : VW027059.D
Acq On : 12 Sep 2023 11:29
Operator : SY/MD
Sample : 04332-22RE
Misc : 2.70g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AN1RE

Quant Time: Sep 13 03:07:10 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

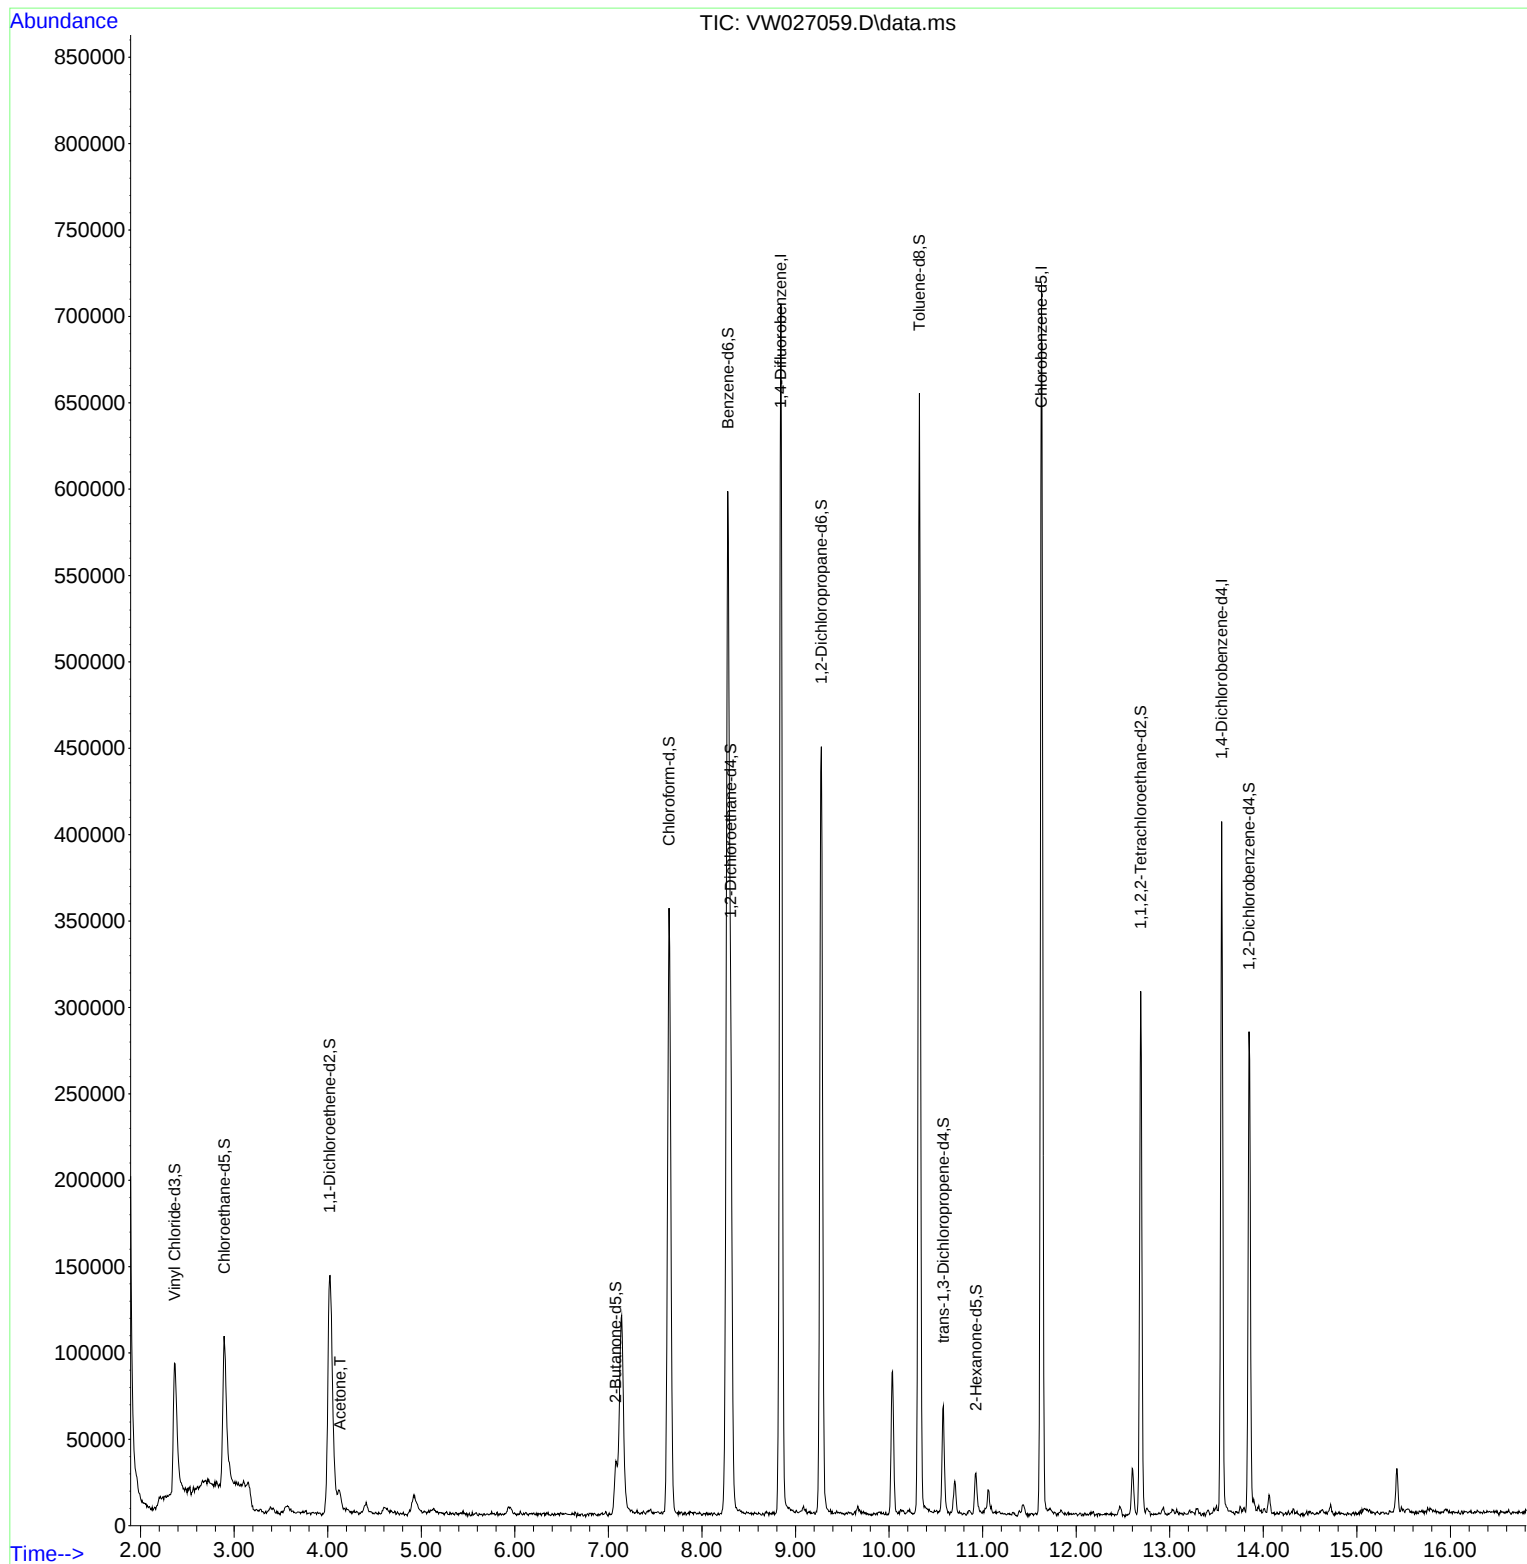

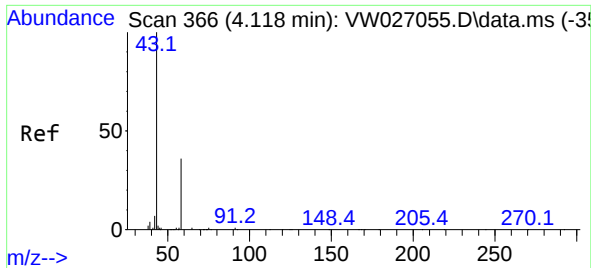

#13
Acetone
Concen: 8.494 ug/L
RT: 4.131 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW027059.D
Acq: 12 Sep 2023 11:29

Instrument :
MSVOA_W
ClientSampleId :
C0AN1RE

Tgt Ion: 43 Resp: 15017
Ion Ratio Lower Upper
43 100
58 35.8 0.0 66.4

