

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027064.D
 Acq On : 12 Sep 2023 13:29
 Operator : SY/MD
 Sample : 04387-06RE
 Misc : 2.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB1RE

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
 Supervised By :Mahesh Dadoda 09/13/2023

Quant Time: Sep 13 03:07:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	677694	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	457001	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	99271	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	122079	10.083	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	40.320%		
7) Chloroethane-d5	2.893	69	140015	14.329	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	57.320%		
11) 1,1-Dichloroethene-d2	4.027	65	45325	10.158	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	40.640%#		
21) 2-Butanone-d5	7.081	46	38817m	16.639	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	33.280%		
24) Chloroform-d	7.648	84	374782	18.585	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	74.320%		
26) 1,2-Dichloroethane-d4	8.307	65	193445	18.250	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	73.000%		
32) Benzene-d6	8.276	84	610260	20.359	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	81.440%		
36) 1,2-Dichloropropane-d6	9.276	67	216334	24.583	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	98.320%		
41) Toluene-d8	10.325	98	422122	15.554	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	62.200%		
43) trans-1,3-Dichloroprop...	10.581	79	23589	6.907	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	27.640%#		
47) 2-Hexanone-d5	10.922	63	4461	5.430	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	10.860%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	137386	20.117	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.480%		
66) 1,2-Dichlorobenzene-d4	13.848	152	58406	17.011	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	68.040%#		
Target Compounds					Qvalue	
13) Acetone	4.118	43	36393	17.816	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
Data File : VW027064.D
Acq On : 12 Sep 2023 13:29
Operator : SY/MD
Sample : 04387-06RE
Misc : 2.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AB1RE

Quant Time: Sep 13 03:07:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 09/13/2023
Supervised By :Mahesh Dadoda 09/13/2023

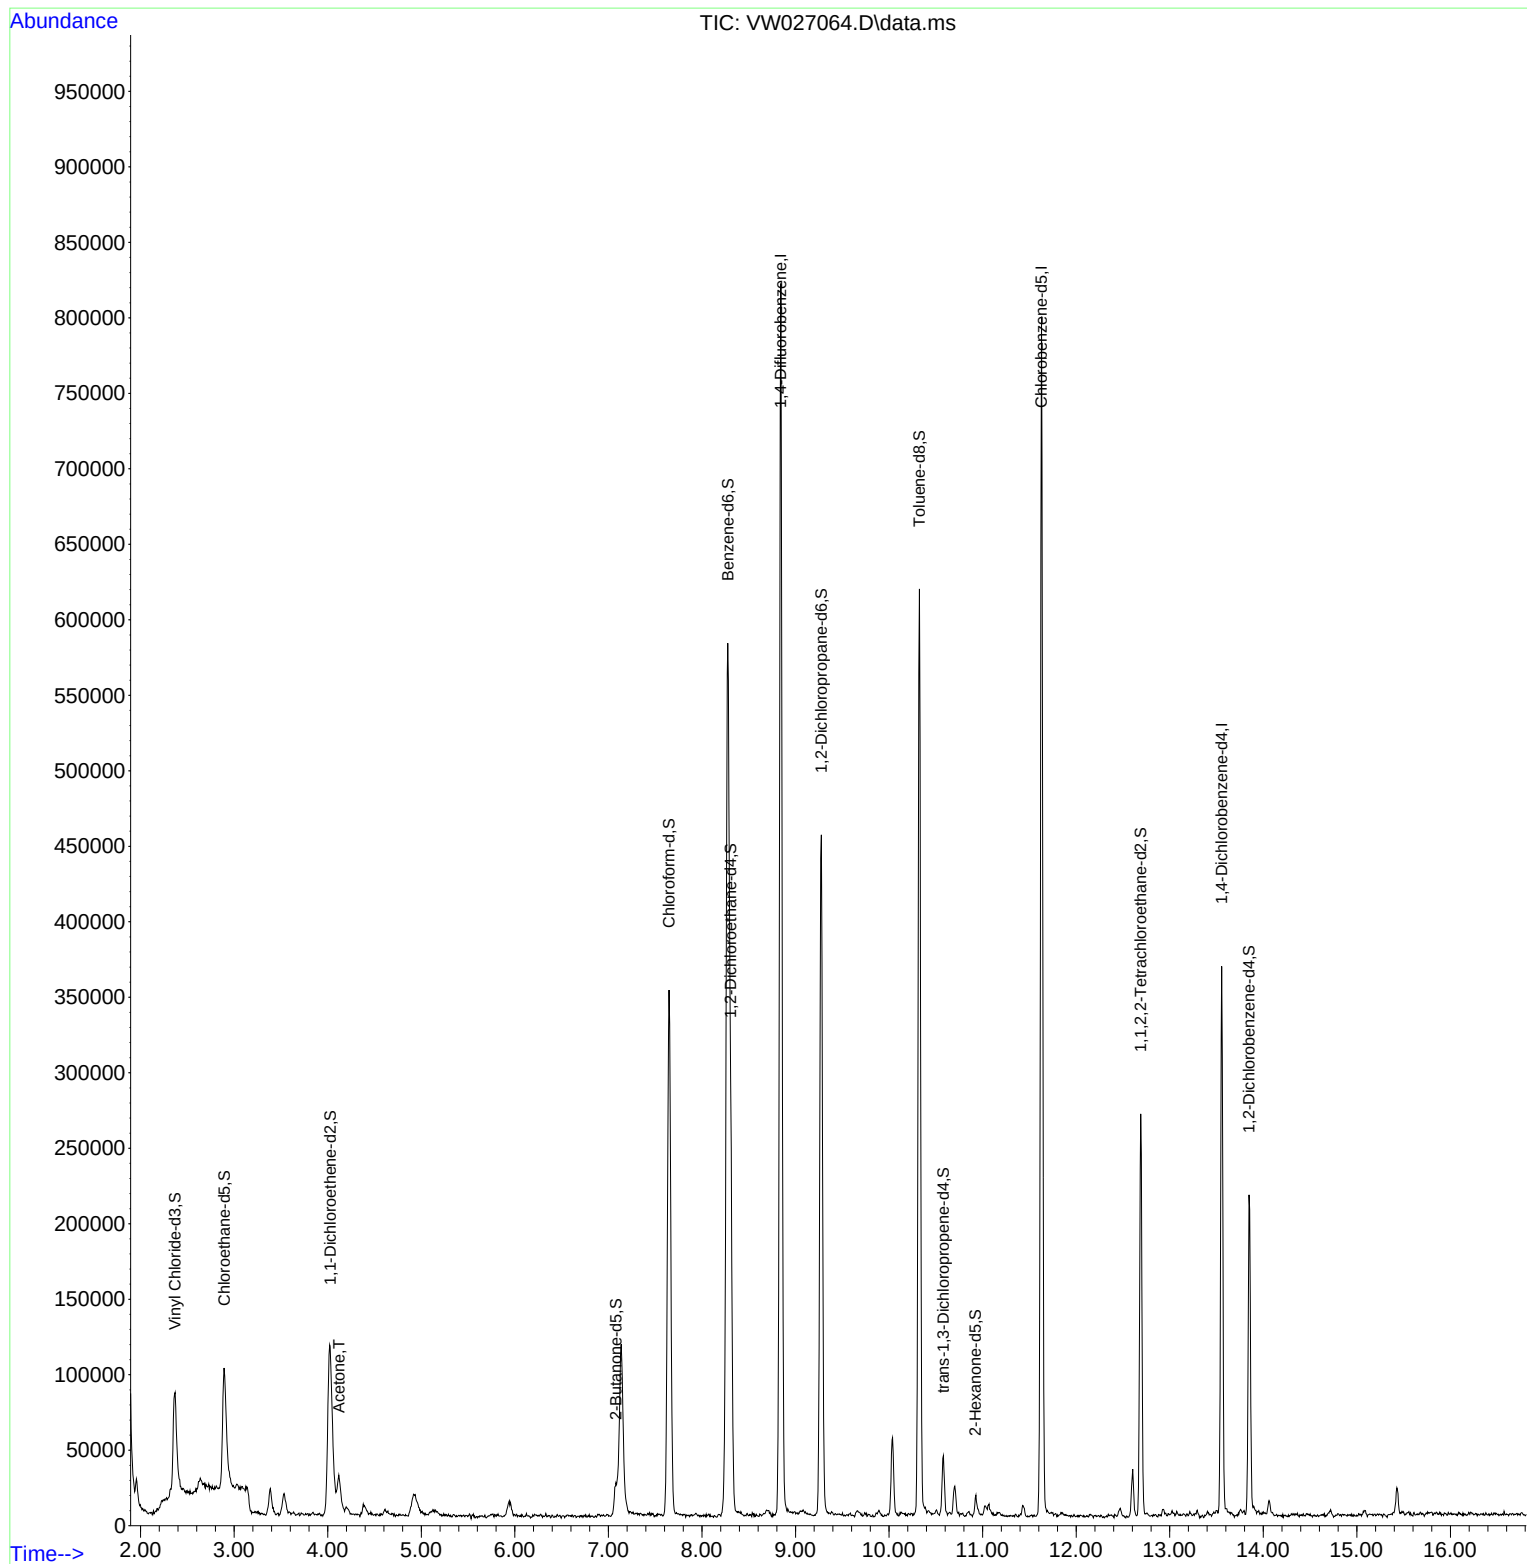

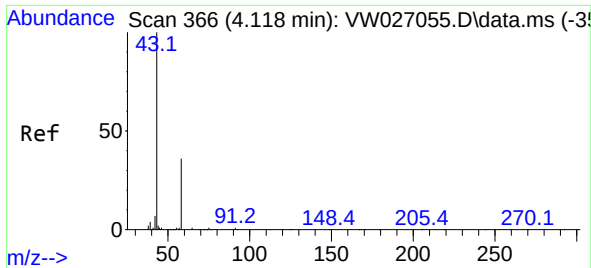

#13
Acetone
Concen: 17.816 ug/L
RT: 4.118 min Scan# 30
Delta R.T. -0.000 min
Lab File: VW027064.D
Acq: 12 Sep 2023 13:29

Instrument :
MSVOA_W
ClientSampleId :
C0AB1RE

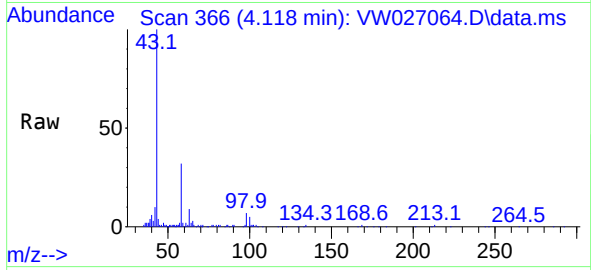

Tgt Ion: 43 Resp: 3639
Ion Ratio Lower Upper
43 100
58 36.6 0.0 66.4

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 09/13/2023
Supervised By :Mahesh Dadoda 09/13/2023

