

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
 Data File : VW027066.D
 Acq On : 12 Sep 2023 14:17
 Operator : SY/MD
 Sample : 04387-08RE
 Misc : 3.19g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB4RE

Quant Time: Sep 13 03:08:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	645450	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	459694	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	131088	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	131756	11.426	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	45.720%
7) Chloroethane-d5	2.899	69	138790	14.913	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.640%
11) 1,1-Dichloroethene-d2	4.027	65	46533	10.950	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.800%#
21) 2-Butanone-d5	7.081	46	36210	16.297	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	32.600%
24) Chloroform-d	7.654	84	374537	19.500	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.000%
26) 1,2-Dichloroethane-d4	8.307	65	188152	18.638	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.560%
32) Benzene-d6	8.276	84	609501	20.214	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.840%
36) 1,2-Dichloropropane-d6	9.276	67	220335	24.891	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.560%
41) Toluene-d8	10.325	98	413039	15.130	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	60.520%
43) trans-1,3-Dichloroprop...	10.581	79	23671	6.891	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	27.560%#
47) 2-Hexanone-d5	10.928	63	5942	7.190	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	14.380%#
56) 1,1,2,2-Tetrachloroeth...	12.690	84	163318	23.775	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.080%
66) 1,2-Dichlorobenzene-d4	13.848	152	84665	18.674	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.680%#
Target Compounds					Qvalue	
13) Acetone	4.125	43	13130	6.749	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091223\
Data File : VW027066.D
Acq On : 12 Sep 2023 14:17
Operator : SY/MD
Sample : 04387-08RE
Misc : 3.19g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB4RE

Quant Time: Sep 13 03:08:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

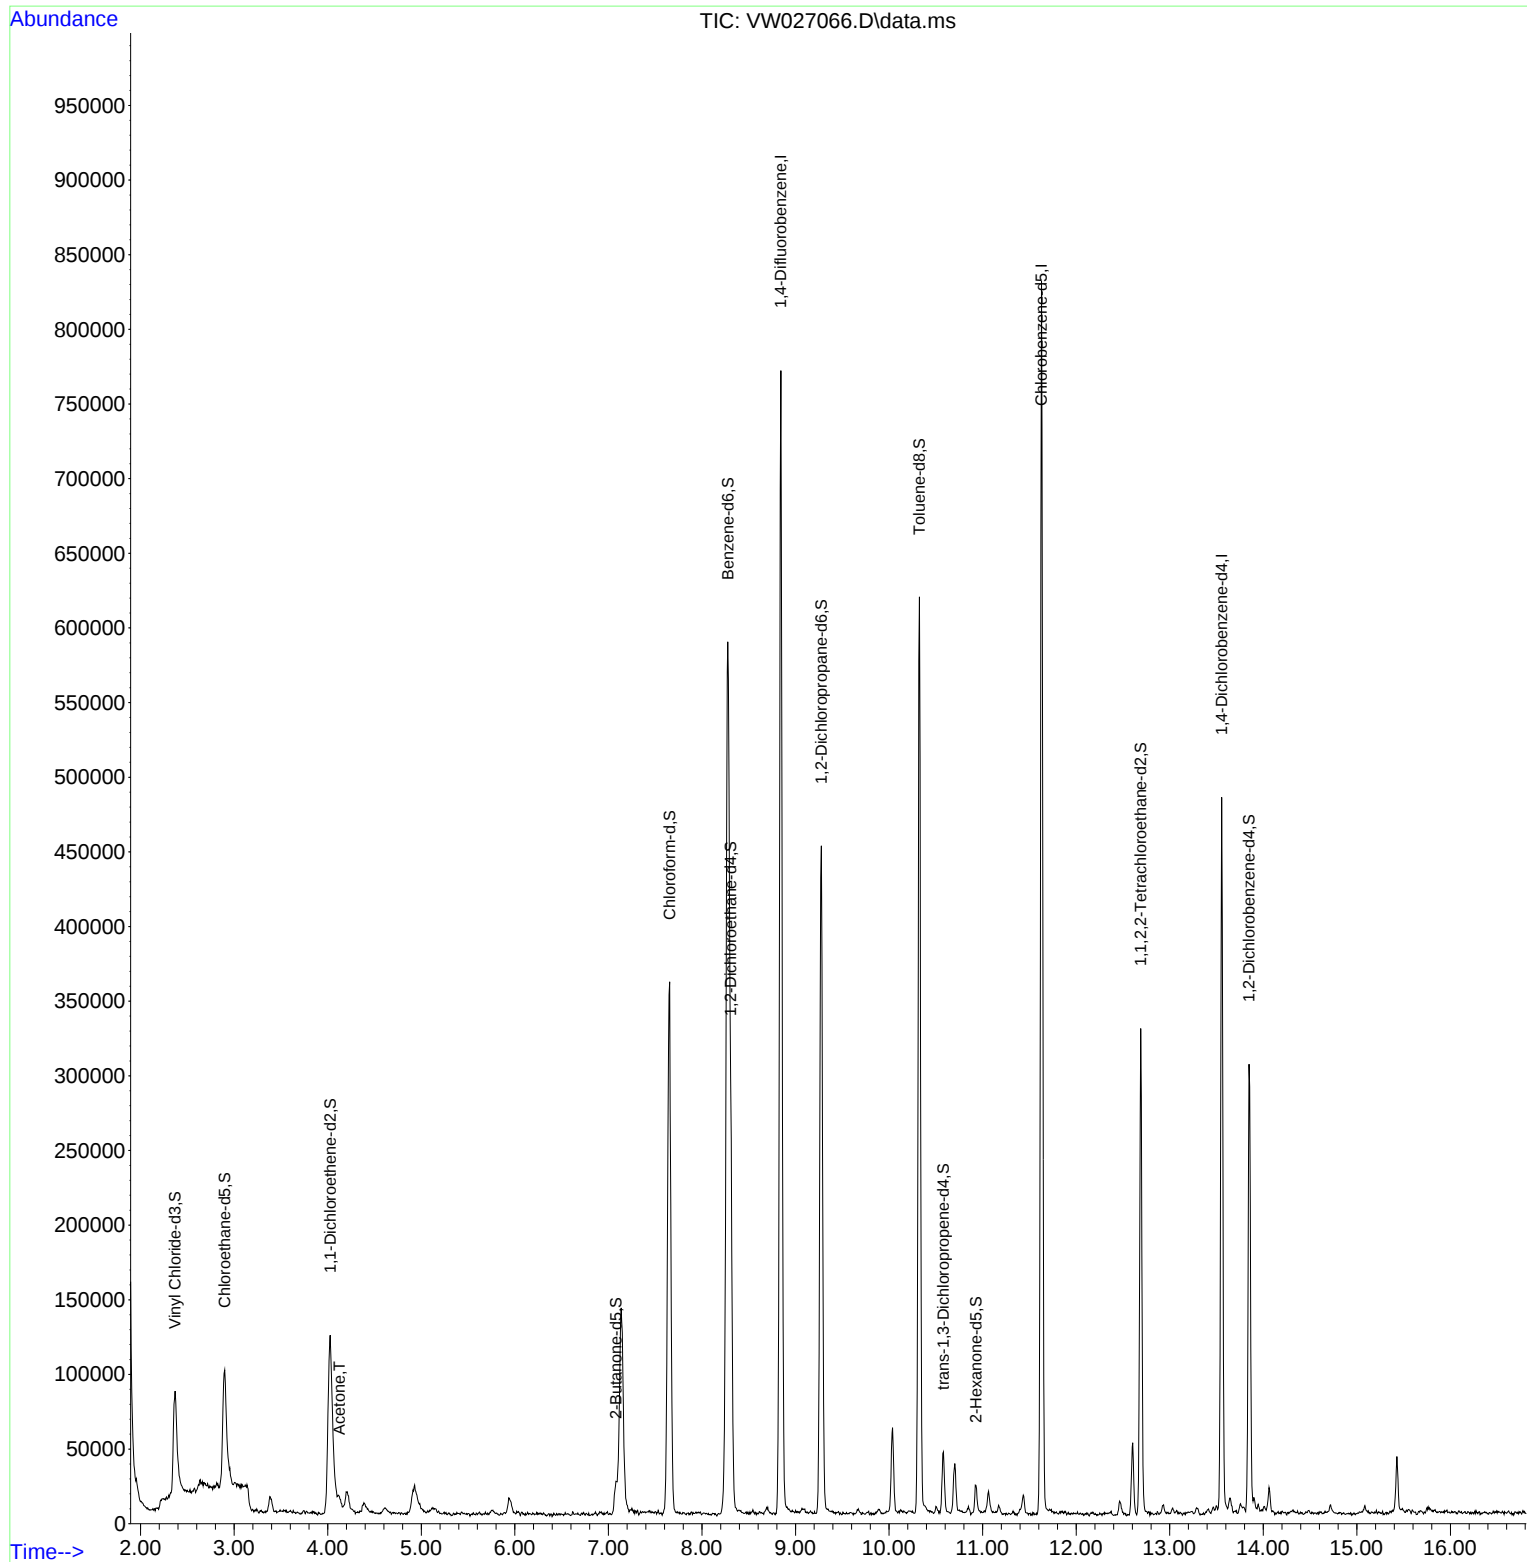

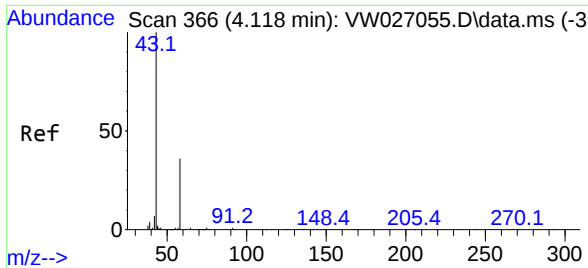

#13
 Acetone
 Concen: 6.749 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW027066.D
 Acq: 12 Sep 2023 14:17

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB4RE

Tgt Ion: 43 Resp: 13130
 Ion Ratio Lower Upper
 43 100
 58 37.7 0.0 66.4

