

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
 Data File : VW027097.D
 Acq On : 14 Sep 2023 13:03
 Operator : SY/MD
 Sample : 04330-09
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 15 00:15:14 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	522744	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	521592	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	262241	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	122978	13.168	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.680%
7) Chloroethane-d5	3.246	69	355	0.047	ug/L	0.35
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.200%#
11) 1,1-Dichloroethene-d2	4.161	65	193	0.056	ug/L	0.14
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.240%#
21) 2-Butanone-d5	7.081	46	59591	33.115	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.240%
24) Chloroform-d	7.648	84	297427	19.121	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.480%
26) 1,2-Dichloroethane-d4	8.307	65	153234	18.742	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	74.960%
32) Benzene-d6	8.276	84	610794	17.853	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.400%
36) 1,2-Dichloropropane-d6	9.276	67	180068	17.928	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	71.720%
41) Toluene-d8	10.324	98	510402	16.478	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.920%
43) trans-1,3-Dichloroprop...	10.581	79	66197	16.984	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.920%
47) 2-Hexanone-d5	10.922	63	30580	32.612	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.220%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	158106	20.285	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.120%
66) 1,2-Dichlorobenzene-d4	13.848	152	193314	21.314	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.240%
Target Compounds						Qvalue
16) Methylene chloride	4.929	84	36215	3.576	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
Data File : VW027097.D
Acq On : 14 Sep 2023 13:03
Operator : SY/MD
Sample : 04330-09
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 15 00:15:14 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

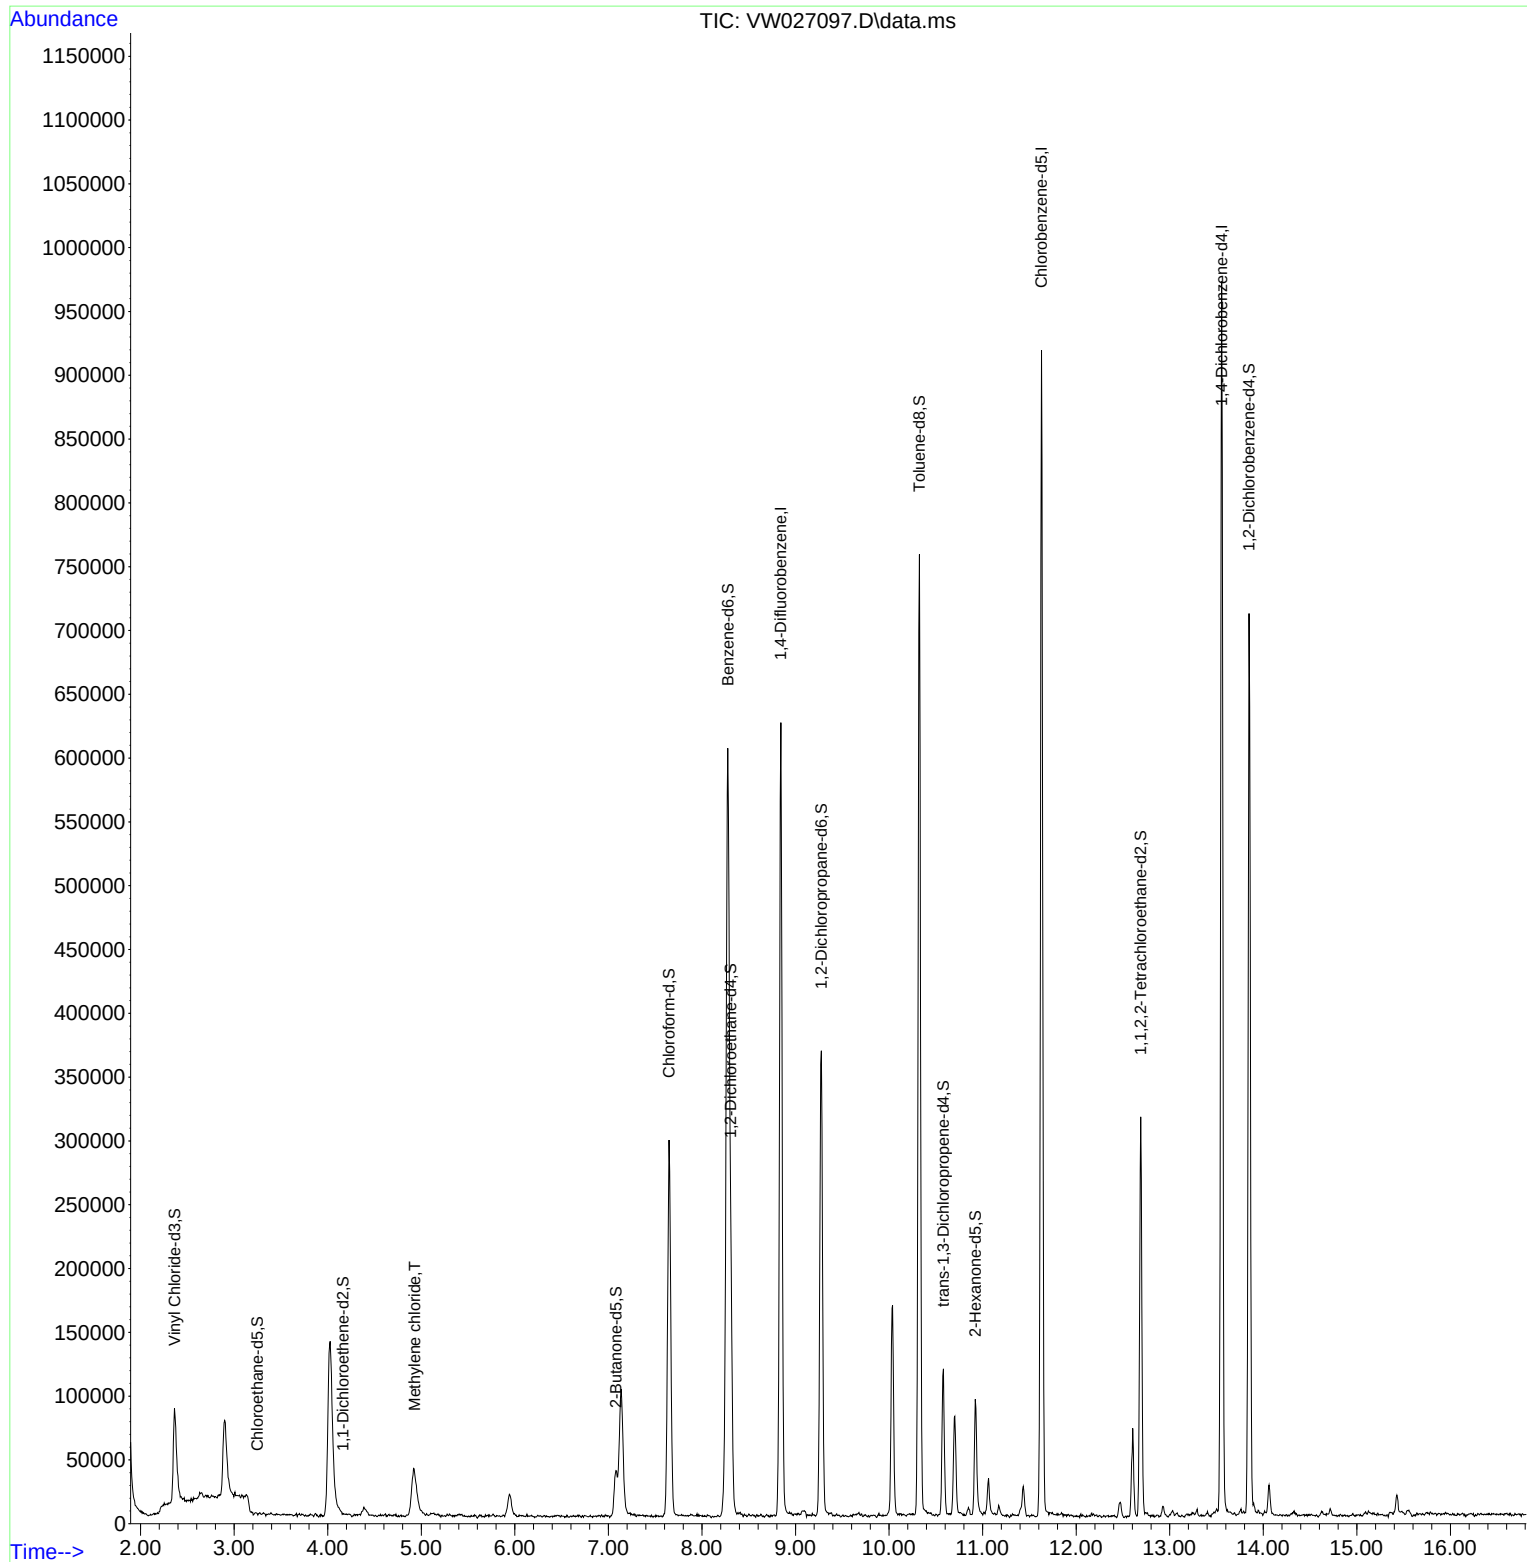

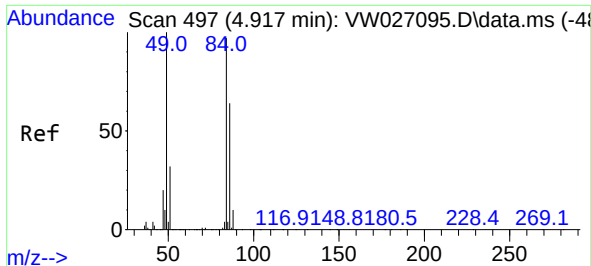

#16
Methylene chloride
Concen: 3.576 ug/L
RT: 4.929 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW027097.D
Acq: 14 Sep 2023 13:03

Instrument :
MSVOA_W
ClientSampleId :

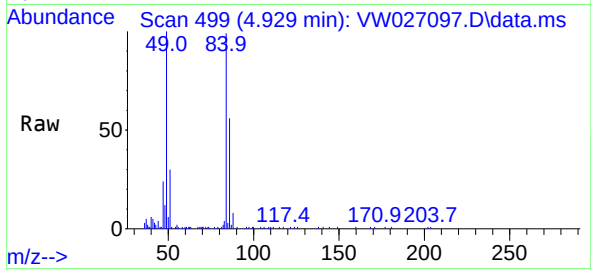

Tgt Ion: 84 Resp: 36215

Ion	Ratio	Lower	Upper
84	100		
86	56.3	44.1	81.9
49	100.6	82.1	152.5

