

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
 Data File : VW027103.D
 Acq On : 14 Sep 2023 15:27
 Operator : SY/MD
 Sample : 04417-16
 Misc : 5.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYN2




Manual IntegrationsAPPROVED

Quant Time: Sep 15 00:16:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

09/15/2023
 Supervised By :Mahesh

Dadoda
 09/15/2023

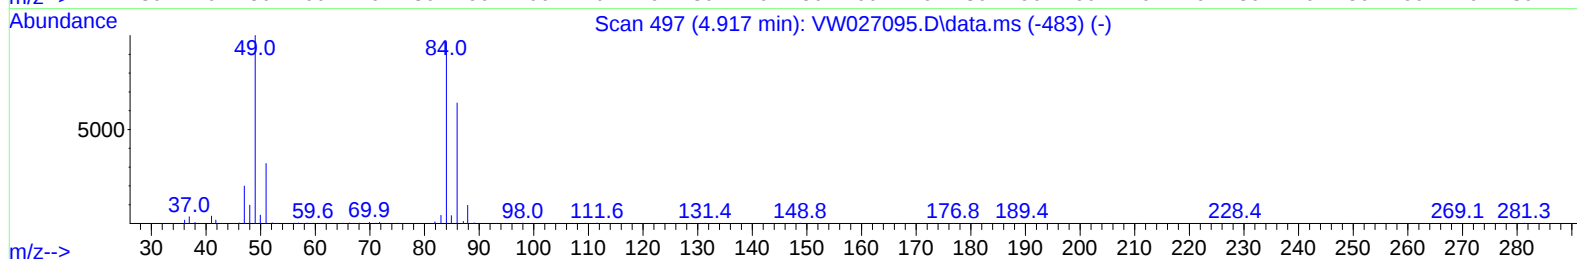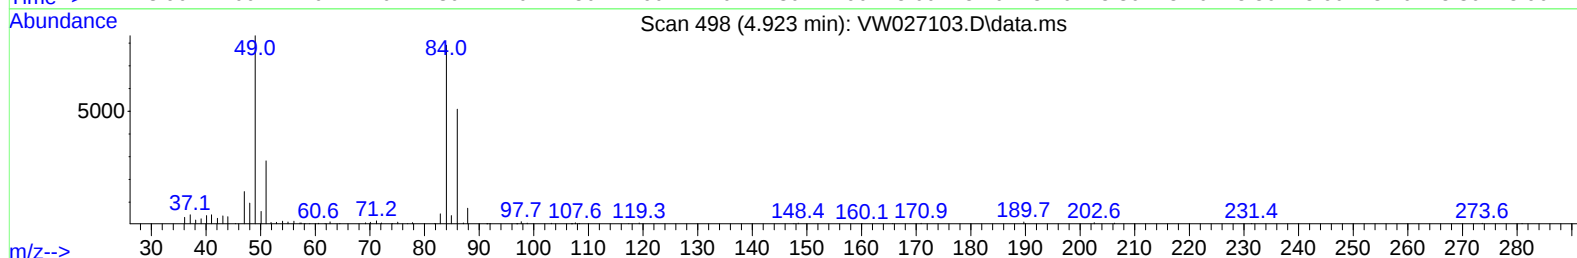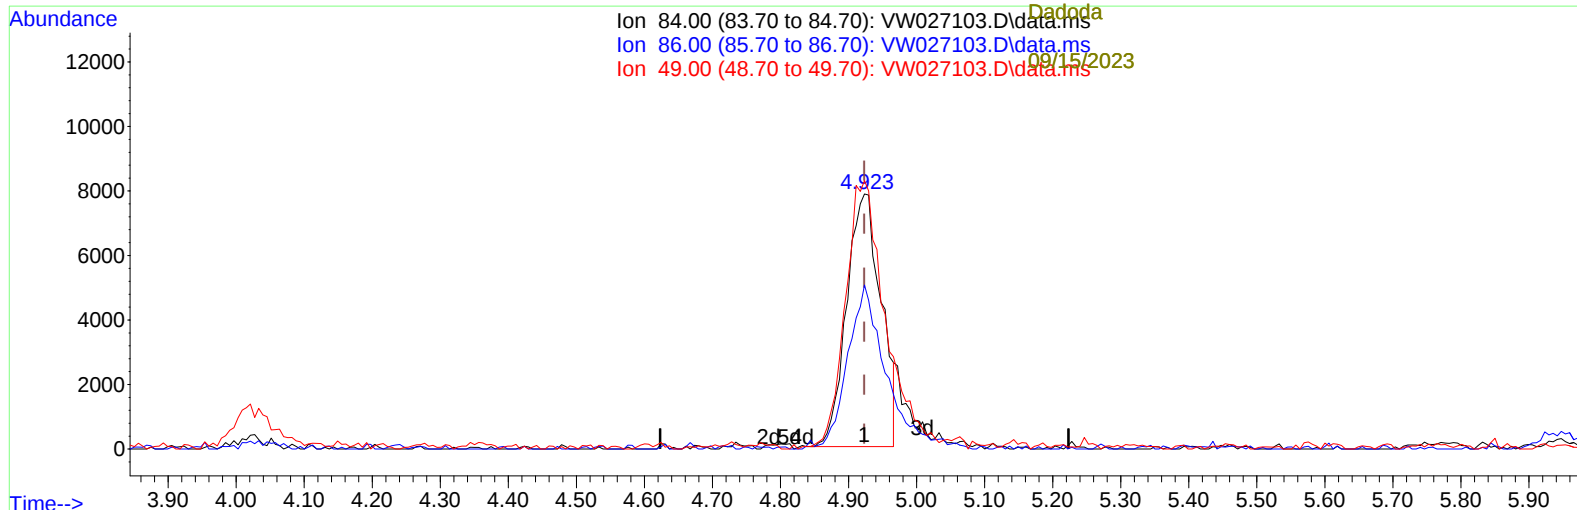

TIC: VW027103.D\data.ms

(16) Methylene chloride (T)

4.923min (+ 0.000) 1.90 ug/L

response 27481

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.00	64.34
49.00	117.30	105.25
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
Data File : VW027103.D
Acq On : 14 Sep 2023 15:27
Operator : SY/MD
Sample : 04417-16
Misc : 5.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Instrument :
MSVOA_W
ClientSampleId :
EZYN2

Manual IntegrationsAPPROVED

Quant Time: Sep 15 00:16:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

09/15/2023
Supervised By :Mahesh
Dadoda

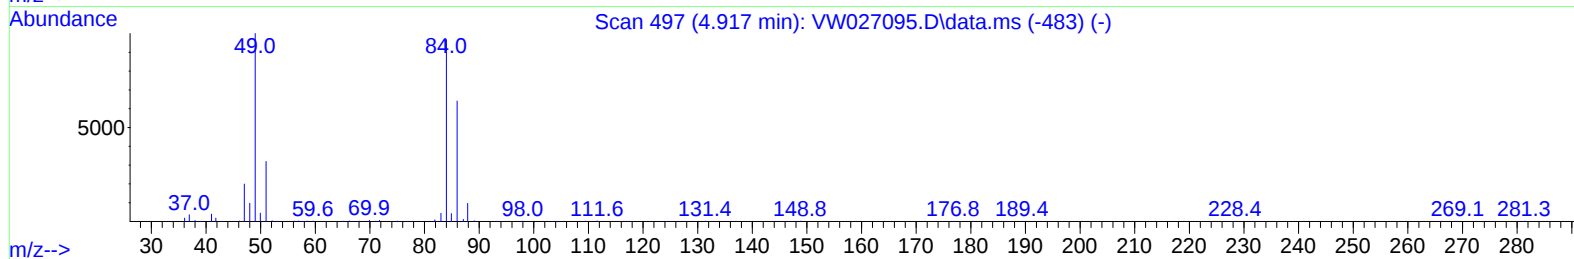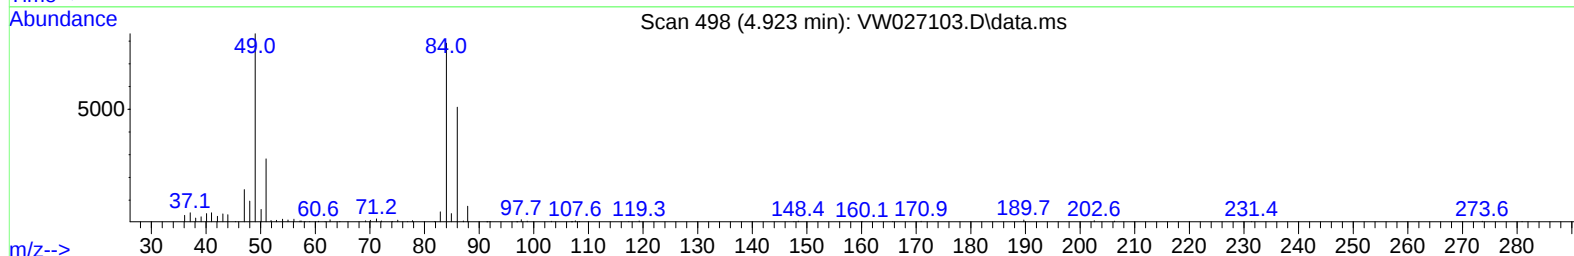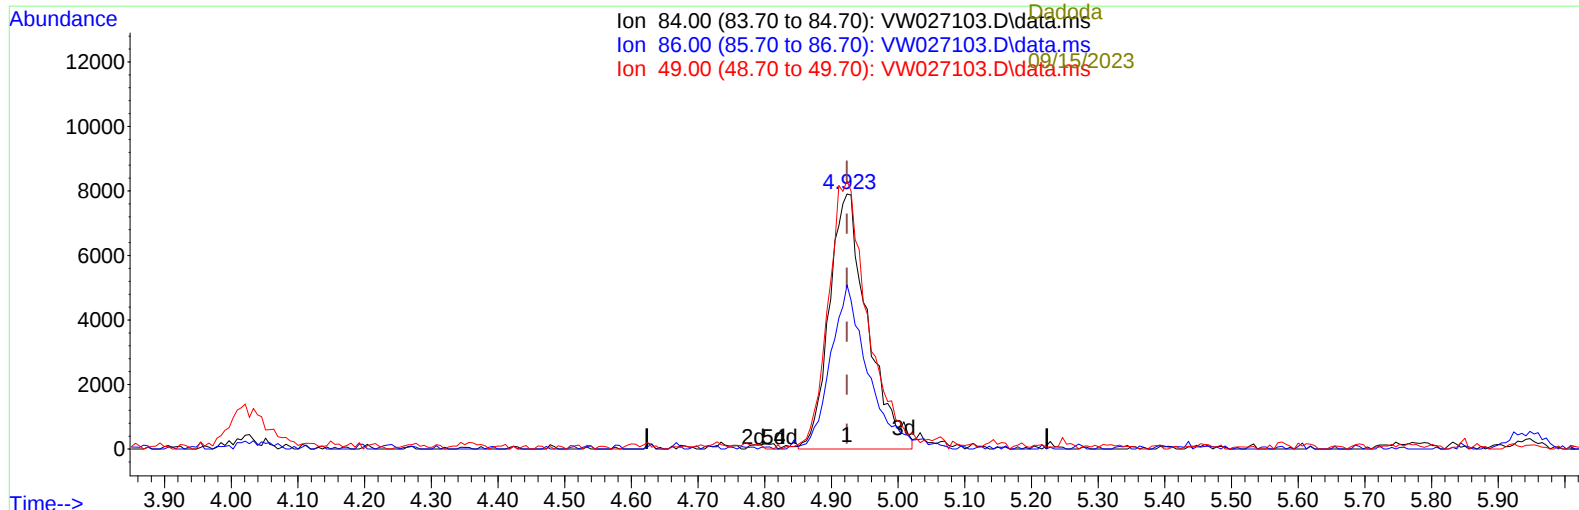

TIC: VW027103.D\data.ms

(16) Methylene chloride (T)

4.923min (+ 0.000) 2.17 ug/L m

response 31491

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.00	64.34
49.00	117.30	105.25
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
 Data File : VW027103.D
 Acq On : 14 Sep 2023 15:27
 Operator : SY/MD
 Sample : 04417-16
 Misc : 5.18g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EZYN2

Manual IntegrationsAPPROVED

Quant Time: Sep 15 00:16:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

09/15/2023
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		747372	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		562138	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		154801	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		133183	9.975	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	39.880%	
7) Chloroethane-d5	2.893	69		141138	13.097	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	52.400%	
11) 1,1-Dichloroethene-d2	4.015	65		62407	12.682	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.720%	
21) 2-Butanone-d5	7.075	46		97982	38.084	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.160%	
24) Chloroform-d	7.648	84		416630	18.734	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.920%	
26) 1,2-Dichloroethane-d4	8.307	65		213618	18.275	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	73.080%	
32) Benzene-d6	8.276	84		760073	20.614	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.440%	
36) 1,2-Dichloropropane-d6	9.270	67		249501	23.049	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.200%	
41) Toluene-d8	10.325	98		577215	17.291	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.160%	
43) trans-1,3-Dichloroprop...	10.575	79		74179	17.659	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.640%	
47) 2-Hexanone-d5	10.922	63		52075	51.530	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.060%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		205520	24.466	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.880%	
66) 1,2-Dichlorobenzene-d4	13.849	152		118009	22.041	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.160%	
Target Compounds							
13) Acetone	4.131	43		6705	2.976	ug/L	97
16) Methylene chloride	4.923	84		31491m	2.175	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
Data File : VW027103.D
Acq On : 14 Sep 2023 15:27
Operator : SY/MD
Sample : 04417-16
Misc : 5.18g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EZYIN2

Manual IntegrationsAPPROVED

Quant Time: Sep 15 00:16:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

09/15/2023
Supervised By :Mahesh
Dadoda

09/15/2023

