

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
 Data File : VW027113.D
 Acq On : 14 Sep 2023 19:28
 Operator : SY/MD
 Sample : VIBLK511
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK511




Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt
 09/15/2023

Supervised By :Mahesh
 Dadoda

09/15/2023

Quant Time: Sep 15 00:17:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

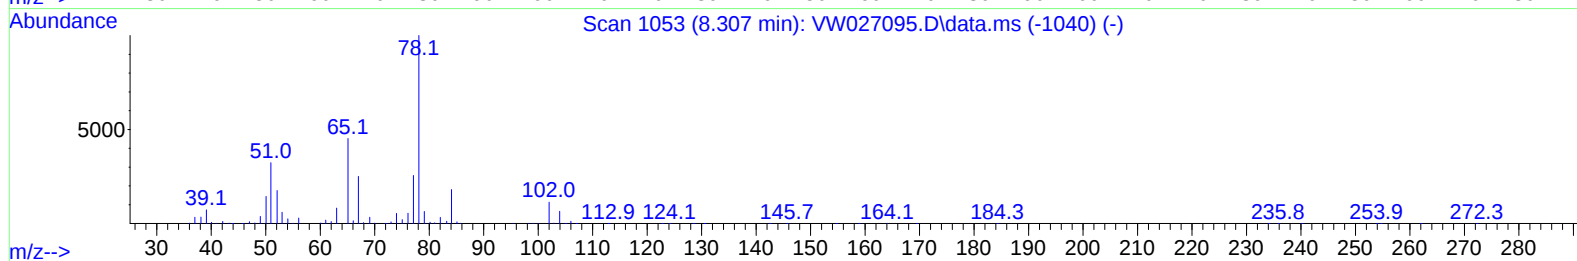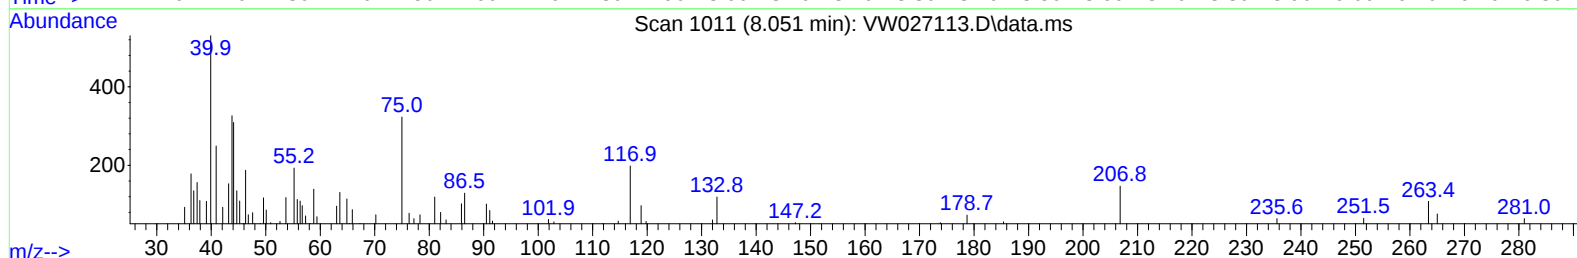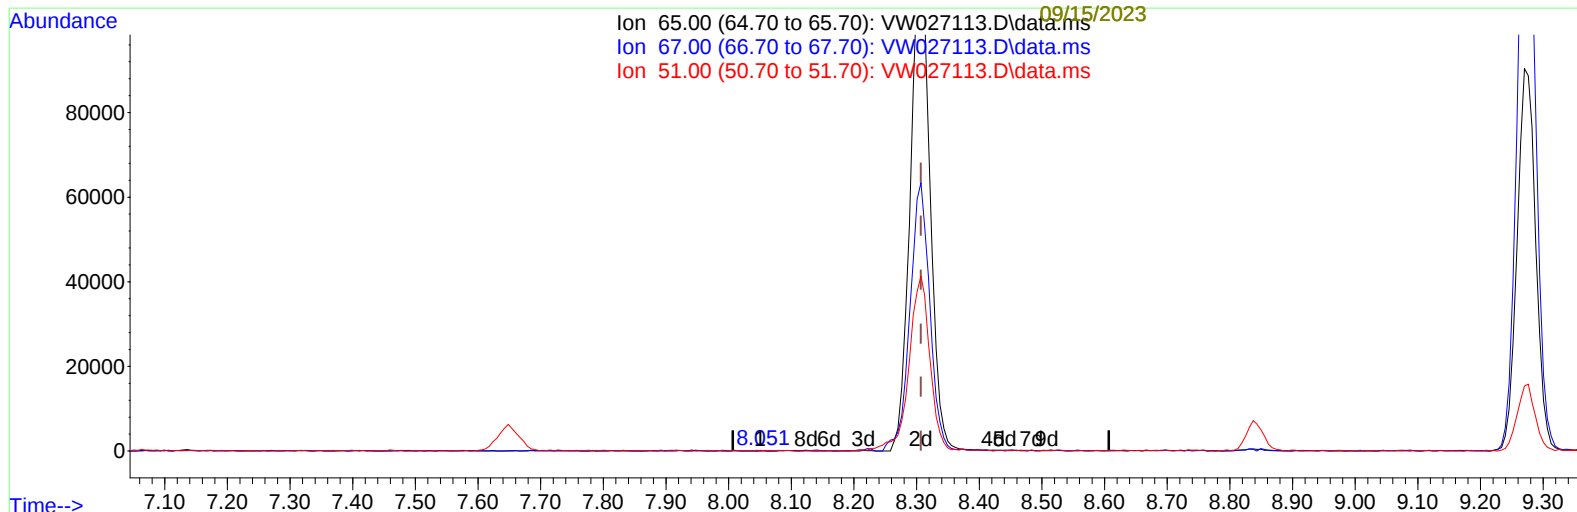

TIC: VW027113.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.051min (-0.256) 0.01 ug/L

response 93

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	56.99
51.00	110.30	94.62
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
 Data File : VW027113.D
 Acq On : 14 Sep 2023 19:28
 Operator : SY/MD
 Sample : VIBLK511
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK511

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt
 09/15/2023
 Supervised By :Mahesh
 Dadoda
 09/15/2023

Quant Time: Sep 15 00:17:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

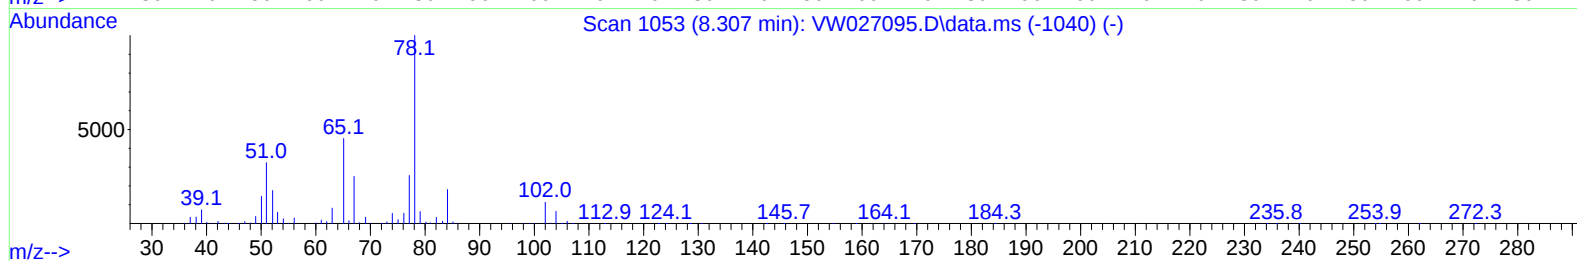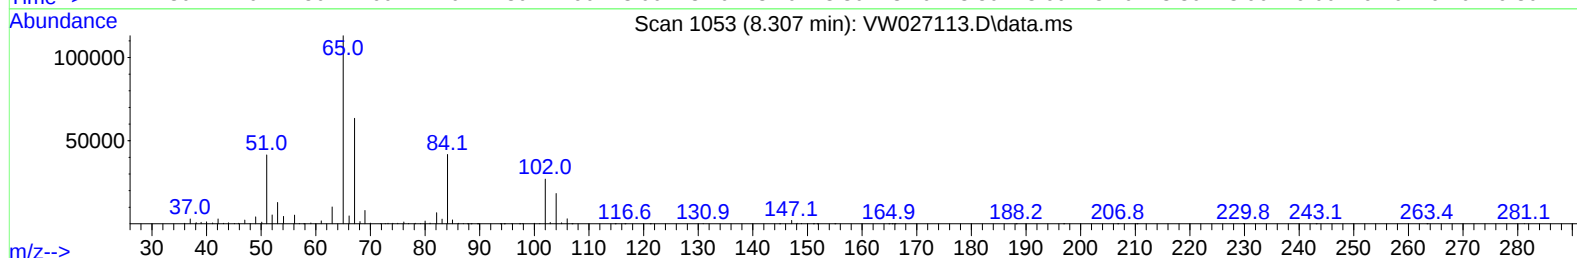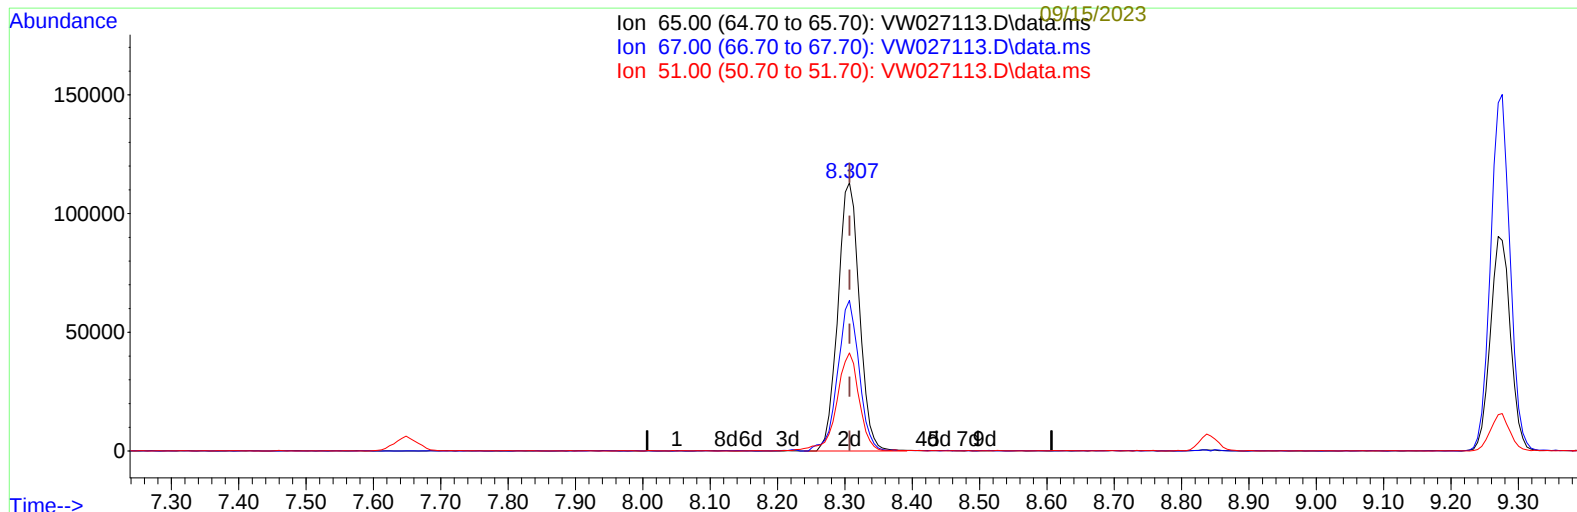

TIC: VW027113.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 18.95 ug/L m

response 250920

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.02#
51.00	110.30	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
 Data File : VW027113.D
 Acq On : 14 Sep 2023 19:28
 Operator : SY/MD
 Sample : VIBLK511
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK511

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt
 09/15/2023
 Supervised By :Mahesh
 Dadoda
 09/15/2023

Quant Time: Sep 15 00:17:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Sep 09 02:59:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	846702	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	828860	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	468027	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	186498	12.329	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	49.320%
7) Chloroethane-d5	2.893	69	173746	14.232	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.920%
11) 1,1-Dichloroethene-d2	4.021	65	90374	16.211	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.840%
21) 2-Butanone-d5	7.075	46	141074	48.401	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.800%
24) Chloroform-d	7.648	84	465622	18.481	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.920%
26) 1,2-Dichloroethane-d4	8.307	65	250920m	18.947	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	75.800%
32) Benzene-d6	8.276	84	1010957	18.595	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.400%
36) 1,2-Dichloropropane-d6	9.276	67	301532	18.892	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.560%
41) Toluene-d8	10.325	98	912453	18.538	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.160%
43) trans-1,3-Dichloroprop...	10.575	79	117627	18.991	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.960%
47) 2-Hexanone-d5	10.922	63	81067	54.405	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.800%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	296052	23.902	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	349597	21.597	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.400%
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	44461	2.710	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091423\
Data File : VW027113.D
Acq On : 14 Sep 2023 19:28
Operator : SY/MD
Sample : VIBLK511
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK511

Manual IntegrationsAPPROVED

Quant Time: Sep 15 00:17:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM090523SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Sep 09 02:59:49 2023
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt
09/15/2023
Supervised By :Mahesh
Dadoda
09/15/2023

