
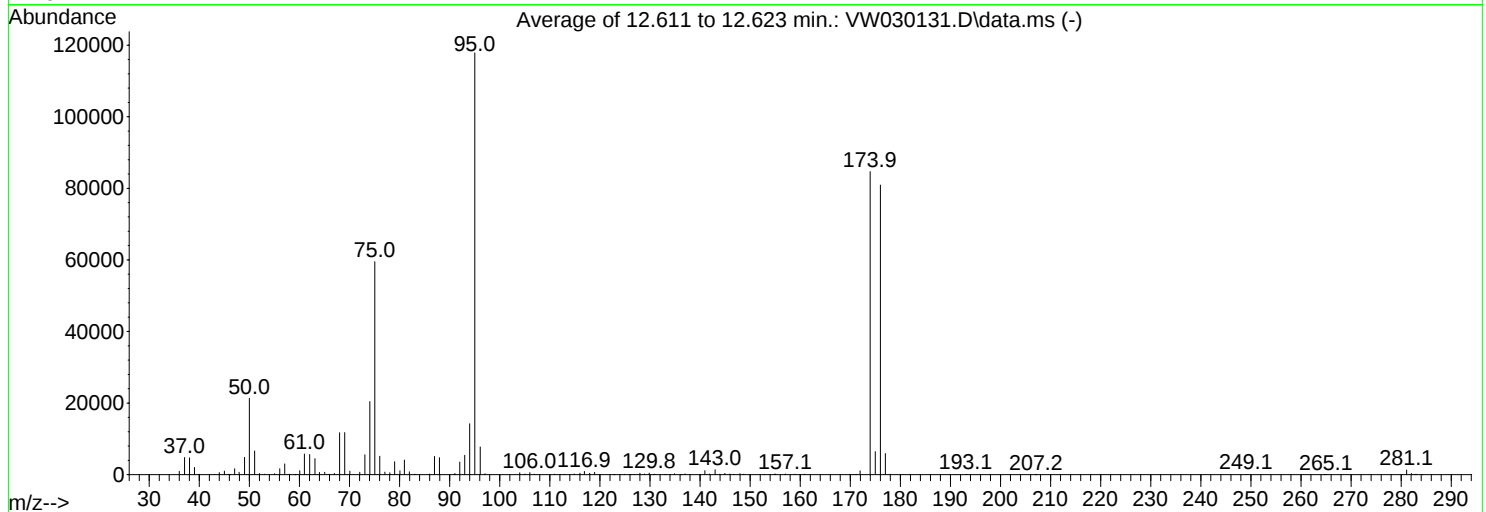


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW091624\
Data File : VW030131.D
Acq On : 16 Sep 2024 13:57
Operator : SY/MD
Sample : BFB557
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB557

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Title : SFAM01.0
Last Update : Tue Sep 17 04:41:19 2024

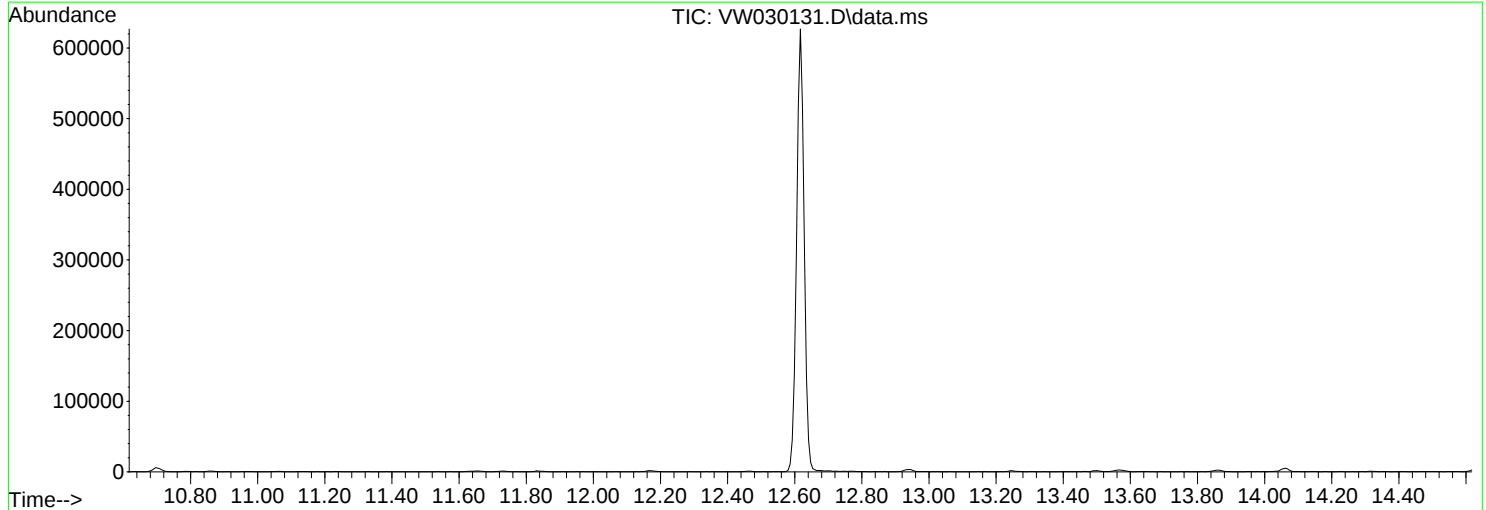

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	21304	PASS
75	95	30	80	50.5	59515	PASS
95	95	100	100	100.0	117853	PASS
96	95	5	9	6.6	7749	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.8	84656	PASS
175	174	5	9	7.6	6431	PASS
176	174	95	101	95.6	80904	PASS
177	176	5	9	7.3	5927	PASS

m/z	Abundance
40.00	119.0
44.00	147.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557

m/z	Abundance
36.00	958.0
37.10	4730.0
38.10	5036.0
39.10	2080.0
40.00	258.0
42.90	87.0
44.00	714.0
45.00	1079.0
46.00	182.0
47.10	1418.0
47.90	770.0
49.00	5025.0
50.00	21528.0
51.10	6805.0
52.00	272.0
53.00	198.0
55.10	298.0
56.00	1689.0
57.00	3088.0
58.10	195.0
60.10	1040.0
61.00	5862.0
62.00	5527.0
63.10	4577.0
64.00	758.0
65.10	840.0
66.00	141.0
67.10	379.0
68.00	11471.0
69.00	11393.0
70.10	1150.0
72.00	625.0
73.00	5206.0
74.00	19920.0
75.00	56672.0
76.00	4978.0
77.10	721.0
78.00	591.0
79.00	3841.0
80.00	1093.0
81.00	3935.0
82.00	788.0
83.00	163.0
86.00	149.0
87.00	4825.0
88.00	4809.0
90.90	375.0
92.00	3421.0
93.00	5315.0
94.00	13125.0
95.00	113232.0
96.10	7383.0
97.10	234.0
104.10	551.0
105.00	158.0
106.00	566.0
106.90	89.0
109.90	72.0
111.00	130.0
112.00	70.0
112.80	116.0
115.00	166.0
116.00	352.0
116.90	728.0
117.90	272.0
119.00	726.0
120.20	54.0
124.90	162.0
128.00	348.0
128.90	120.0
129.90	398.0
131.00	238.0
133.00	263.0
134.90	236.0
136.90	192.0
139.80	68.0
141.00	925.0
141.90	175.0
143.00	1301.0
143.90	120.0
144.90	502.0
146.00	165.0
146.70	127.0
148.00	240.0
148.70	147.0
150.10	89.0
152.80	111.0
153.90	120.0
154.80	250.0
155.10	274.0
156.90	182.0
158.90	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557

160.90	114.0
170.50	98.0
171.00	204.0
172.00	1056.0
174.00	69064.0
175.00	5183.0
176.00	71160.0
177.00	5304.0
177.90	156.0
190.90	81.0
193.10	179.0
207.20	136.0
249.00	222.0
265.00	184.0
281.10	2020.0
282.10	438.0
282.90	263.0
284.10	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557

m/z	Abundance
36.00	1109.0
37.00	5762.0
38.00	4973.0
39.10	2206.0
40.00	250.0
43.00	58.0
44.00	792.0
45.00	1061.0
45.80	122.0
46.20	114.0
47.00	2049.0
48.00	818.0
49.10	5156.0
50.00	23880.0
51.00	7504.0
52.00	326.0
52.90	135.0
55.10	290.0
56.10	1805.0
57.10	3126.0
58.10	120.0
59.10	56.0
60.00	1253.0
61.00	6441.0
62.00	6474.0
63.10	5388.0
64.00	769.0
65.00	704.0
65.90	116.0
66.90	342.0
68.00	13338.0
69.10	13356.0
70.10	982.0
72.10	768.0
73.00	6340.0
74.10	23120.0
75.10	67088.0
76.10	5887.0
77.00	851.0
78.00	618.0
79.00	3962.0
80.10	1197.0
80.90	4547.0
82.00	921.0
83.10	131.0
86.00	238.0
87.00	5921.0
88.00	5208.0
91.10	533.0
92.00	3972.0
93.00	6167.0
94.00	16552.0
95.00	133952.0
96.10	8554.0
97.00	354.0
103.90	619.0
104.90	152.0
106.00	707.0
106.90	181.0
109.90	71.0
110.80	98.0
112.10	117.0
112.80	140.0
114.90	202.0
116.00	477.0
116.90	1041.0
117.90	482.0
118.90	633.0
120.10	75.0
123.90	81.0
124.90	86.0
126.90	59.0
128.00	498.0
128.90	225.0
129.90	494.0
130.90	168.0
133.20	74.0
134.10	72.0
134.90	336.0
137.00	244.0
139.90	121.0
141.00	1433.0
141.90	149.0
143.00	1532.0
143.90	126.0
145.00	339.0
145.80	112.0
146.00	110.0
146.80	86.0
148.00	317.0
148.80	111.0
149.80	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557

152.90	69.0
154.00	81.0
154.90	217.0
157.10	339.0
158.90	166.0
160.90	174.0
169.80	50.0
170.50	114.0
171.20	293.0
171.90	1258.0
173.90	95600.0
175.00	7405.0
176.00	92192.0
177.00	6783.0
178.00	169.0
191.00	68.0
193.10	122.0
207.10	83.0
249.10	103.0
265.10	83.0
281.10	1234.0
282.00	340.0
282.60	133.0
283.10	201.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557

m/z	Abundance
36.00	746.0
37.00	3905.0
38.00	4077.0
39.00	1707.0
39.90	235.0
44.00	681.0
45.00	803.0
46.30	145.0
47.00	1479.0
47.90	490.0
49.00	4250.0
50.00	18504.0
51.00	5588.0
52.10	288.0
53.10	91.0
55.00	252.0
56.10	1419.0
57.00	2765.0
58.00	126.0
60.00	1046.0
61.00	5028.0
62.10	4943.0
63.10	3515.0
63.90	396.0
65.00	530.0
65.90	114.0
66.90	326.0
68.00	10278.0
69.00	10501.0
70.00	792.0
72.10	627.0
73.10	5105.0
74.10	18232.0
75.10	54784.0
76.10	4522.0
77.00	627.0
78.10	403.0
79.00	3090.0
80.00	916.0
81.00	3684.0
81.90	678.0
83.00	97.0
85.90	195.0
86.90	4610.0
87.90	4213.0
91.00	465.0
92.00	3216.0
93.00	4754.0
94.00	13018.0
95.00	106376.0
96.10	7310.0
97.00	217.0
104.00	510.0
105.10	175.0
106.00	423.0
106.90	93.0
111.00	123.0
111.90	97.0
113.00	137.0
114.80	142.0
116.00	352.0
116.90	864.0
118.00	449.0
118.90	589.0
122.80	51.0
124.80	68.0
126.00	62.0
126.90	65.0
128.00	364.0
128.90	244.0
129.80	419.0
130.70	149.0
134.90	190.0
136.10	61.0
137.10	191.0
140.00	53.0
140.90	1057.0
141.90	203.0
143.00	1397.0
144.00	141.0
144.90	195.0
145.90	212.0
146.80	75.0
147.90	258.0
148.80	144.0
150.00	156.0
152.90	116.0
153.90	70.0
155.10	258.0
157.00	204.0
159.00	156.0
160.90	117.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557

169.90	72.0
172.00	848.0
174.00	89304.0
175.00	6704.0
176.00	79360.0
177.00	5693.0
177.90	131.0
193.30	121.0
206.90	54.0
264.60	51.0
281.10	599.0
282.20	218.0
283.20	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB557