

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
 Data File : VW030167.D
 Acq On : 20 Sep 2024 10:27
 Operator : SY/MD
 Sample : VW0920SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 20 23:51:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 20 23:43:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	387669	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	358009	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	170302	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	84427	16.864	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.440%
7) Chloroethane-d5	2.899	69	62701	17.740	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.960%
11) 1,1-Dichloroethene-d2	4.021	65	44747	17.888	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.560%
21) 2-Butanone-d5	7.087	46	45971	37.922	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.840%
24) Chloroform-d	7.648	84	204759	19.210	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.840%
26) 1,2-Dichloroethane-d4	8.307	65	106508	19.898	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.600%
32) Benzene-d6	8.276	84	414265	20.086	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.360%
36) 1,2-Dichloropropane-d6	9.276	67	124914	19.616	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.480%
41) Toluene-d8	10.325	98	374109	20.241	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.960%
43) trans-1,3-Dichloroprop...	10.575	79	47578	18.649	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.600%
47) 2-Hexanone-d5	10.922	63	39574	40.613	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.220%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	94887	20.015	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.040%
66) 1,2-Dichlorobenzene-d4	13.848	152	126710	21.918	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.680%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	3695	0.426	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
Data File : VW030167.D
Acq On : 20 Sep 2024 10:27
Operator : SY/MD
Sample : VW0920SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 20 23:51:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 20 23:43:18 2024
Response via : Initial Calibration

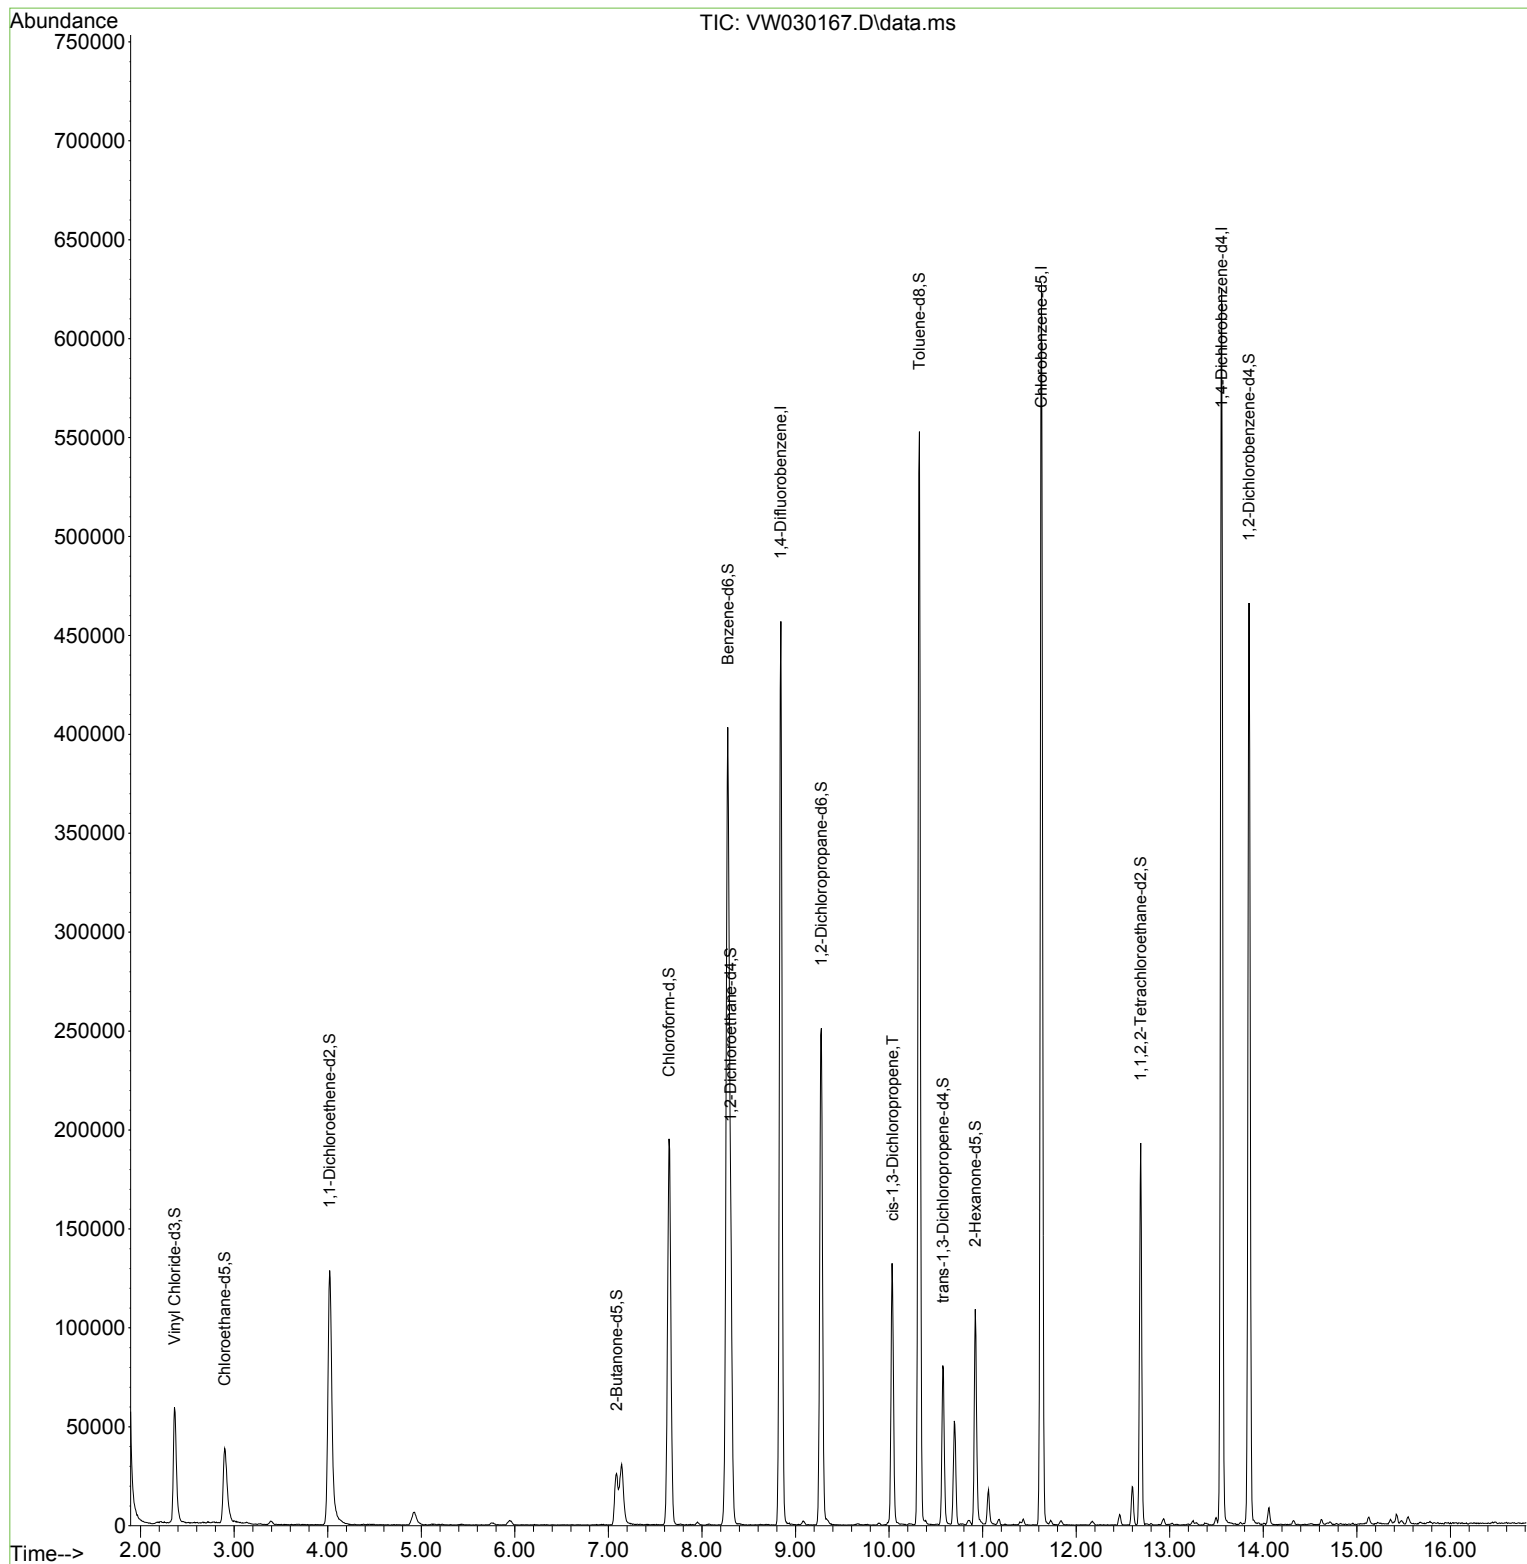

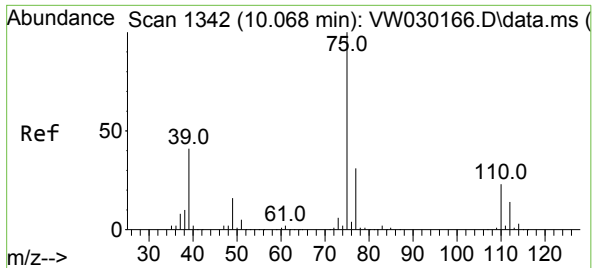

#39
cis-1,3-Dichloropropene
Concen: 0.426 ug/L
RT: 10.038 min Scan# 11
Delta R.T. -0.030 min
Lab File: VW030167.D
Acq: 20 Sep 2024 10:27

Instrument :
MSVOA_W
ClientSampleId :

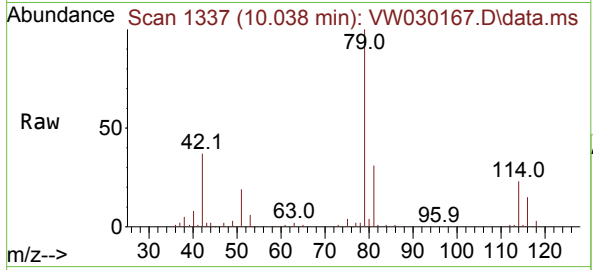

Tgt Ion: 75 Resp: 3695
Ion Ratio Lower Upper
75 100
77 46.5 20.7 38.5#

