

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
 Data File : VW030175.D
 Acq On : 20 Sep 2024 15:14
 Operator : SY/MD
 Sample : P4024-06
 Misc : 14.63g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 20 23:54:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 20 23:43:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	416063	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	159742	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.538	152	104199	25.000	ug/L	#-0.02
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	108907	20.269	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.080%
7) Chloroethane-d5	2.899	69	92277	24.326	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.320%
11) 1,1-Dichloroethene-d2	4.021	65	46191	17.205	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.840%
21) 2-Butanone-d5	7.075	46	68521	52.666	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.340%
24) Chloroform-d	7.648	84	202749	17.723	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	70.880%
26) 1,2-Dichloroethane-d4	8.307	65	110316	19.203	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	76.800%
32) Benzene-d6	8.276	84	389769	42.355	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	169.400%#
36) 1,2-Dichloropropane-d6	9.270	67	119642	42.108	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	168.440%#
41) Toluene-d8	10.319	98	260696	31.612	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	126.440%
43) trans-1,3-Dichloroprop...	10.575	79	41458	36.420	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	145.680%#
47) 2-Hexanone-d5	10.922	63	55410	127.444	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	254.880%#
56) 1,1,2,2-Tetrachloroeth...	12.709	84	129610	61.271	ug/L	0.02
Spiked Amount	25.000	Range	45 - 120	Recovery	=	245.080%#
66) 1,2-Dichlorobenzene-d4	13.861	152	27135	7.671	ug/L	0.01
Spiked Amount	25.000	Range	75 - 120	Recovery	=	30.680%#
Target Compounds						
					Qvalue	
13) Acetone	4.119	43	648890	434.719	ug/L	98
14) Carbon disulfide	4.387	76	42148	2.987	ug/L	97
19) 1,1-Dichloroethane	6.222	63	6058	0.545	ug/L	92
22) 2-Butanone	7.173	43	15292	8.655	ug/L	99
25) Chloroform	7.630	83	4789	0.424	ug/L	# 64
29) Cyclohexane	7.929	56	111313	32.706	ug/L	# 47
30) 1,1,1-Trichloroethane	7.874	97	156631	40.538	ug/L	96
31) Carbon tetrachloride	7.874	117	21018	5.986	ug/L	99
33) Benzene	8.325	78	388428	39.771	ug/L	100
34) Trichloroethene	9.093	95	635643	241.097	ug/L	92
35) Methylcyclohexane	9.337	83	600207	147.669	ug/L	94
37) 1,2-Dichloropropane	9.368	63	47907	18.098	ug/L	# 23
38) Bromodichloromethane	9.618	83	5861	1.758	ug/L	# 77
40) 4-Methyl-2-pentanone	10.209	43	89292	66.015	ug/L	# 88
42) Toluene	10.386	91	9761802	941.958	ug/L	98
45) 1,1,2-Trichloroethane	10.764	97	162133	84.173	ug/L	# 24
46) Tetrachloroethene	10.861	164	752816	386.975	ug/L	96
48) 2-Hexanone	10.934	43	2016814	1938.971	ug/L	# 46
50) 1,2-Dibromoethane	11.239	107	1108	0.624	ug/L	# 1

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
 Data File : VW030175.D
 Acq On : 20 Sep 2024 15:14
 Operator : SY/MD
 Sample : P4024-06
 Misc : 14.63g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 20 23:54:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 20 23:43:18 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
51) Chlorobenzene	11.654	112	84548	12.631	ug/L	96
52) Ethylbenzene	11.727	91	5333575	449.608	ug/L	97
53) m,p-Xylene	11.831	106	6792347	1551.855	ug/L	75
54) o-Xylene	12.166	106	6094803	1479.784	ug/L	78
55) Styrene	12.166	104	316168	44.256	ug/L #	1
57) 1,1,2,2-Tetrachloroethane	12.702	83	35278	15.344	ug/L #	1
60) Isopropylbenzene	12.465	105	3610542	235.341	ug/L	97
61) 1,2,3-Trichloropropane	12.806	75	57580	26.563	ug/L #	1
62) 1,3,5-Trimethylbenzene	13.592	105	14446197	1284.742	ug/L	100
63) 1,2,4-Trimethylbenzene	13.105	105	16816272	1438.553	ug/L	88
64) 1,3-Dichlorobenzene	13.501	146	6547	0.963	ug/L #	1
65) 1,4-Dichlorobenzene	13.580	146	25191	3.586	ug/L #	1
67) 1,2-Dichlorobenzene	13.867	146	38697	6.315	ug/L #	1
68) 1,2-Dibromo-3-chloropr...	14.495	75	18292	38.692	ug/L #	25
70) 1,2,4-trichlorobenzene	15.129	180	9790	2.547	ug/L #	1
71) Naphthalene	15.354	128	2073336	296.990	ug/L	98
72) 1,2,3-Trichlorobenzene	15.556	180	3021	0.896	ug/L #	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
Data File : VW030175.D
Acq On : 20 Sep 2024 15:14
Operator : SY/MD
Sample : P4024-06
Misc : 14.63g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 20 23:54:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 20 23:43:18 2024
Response via : Initial Calibration

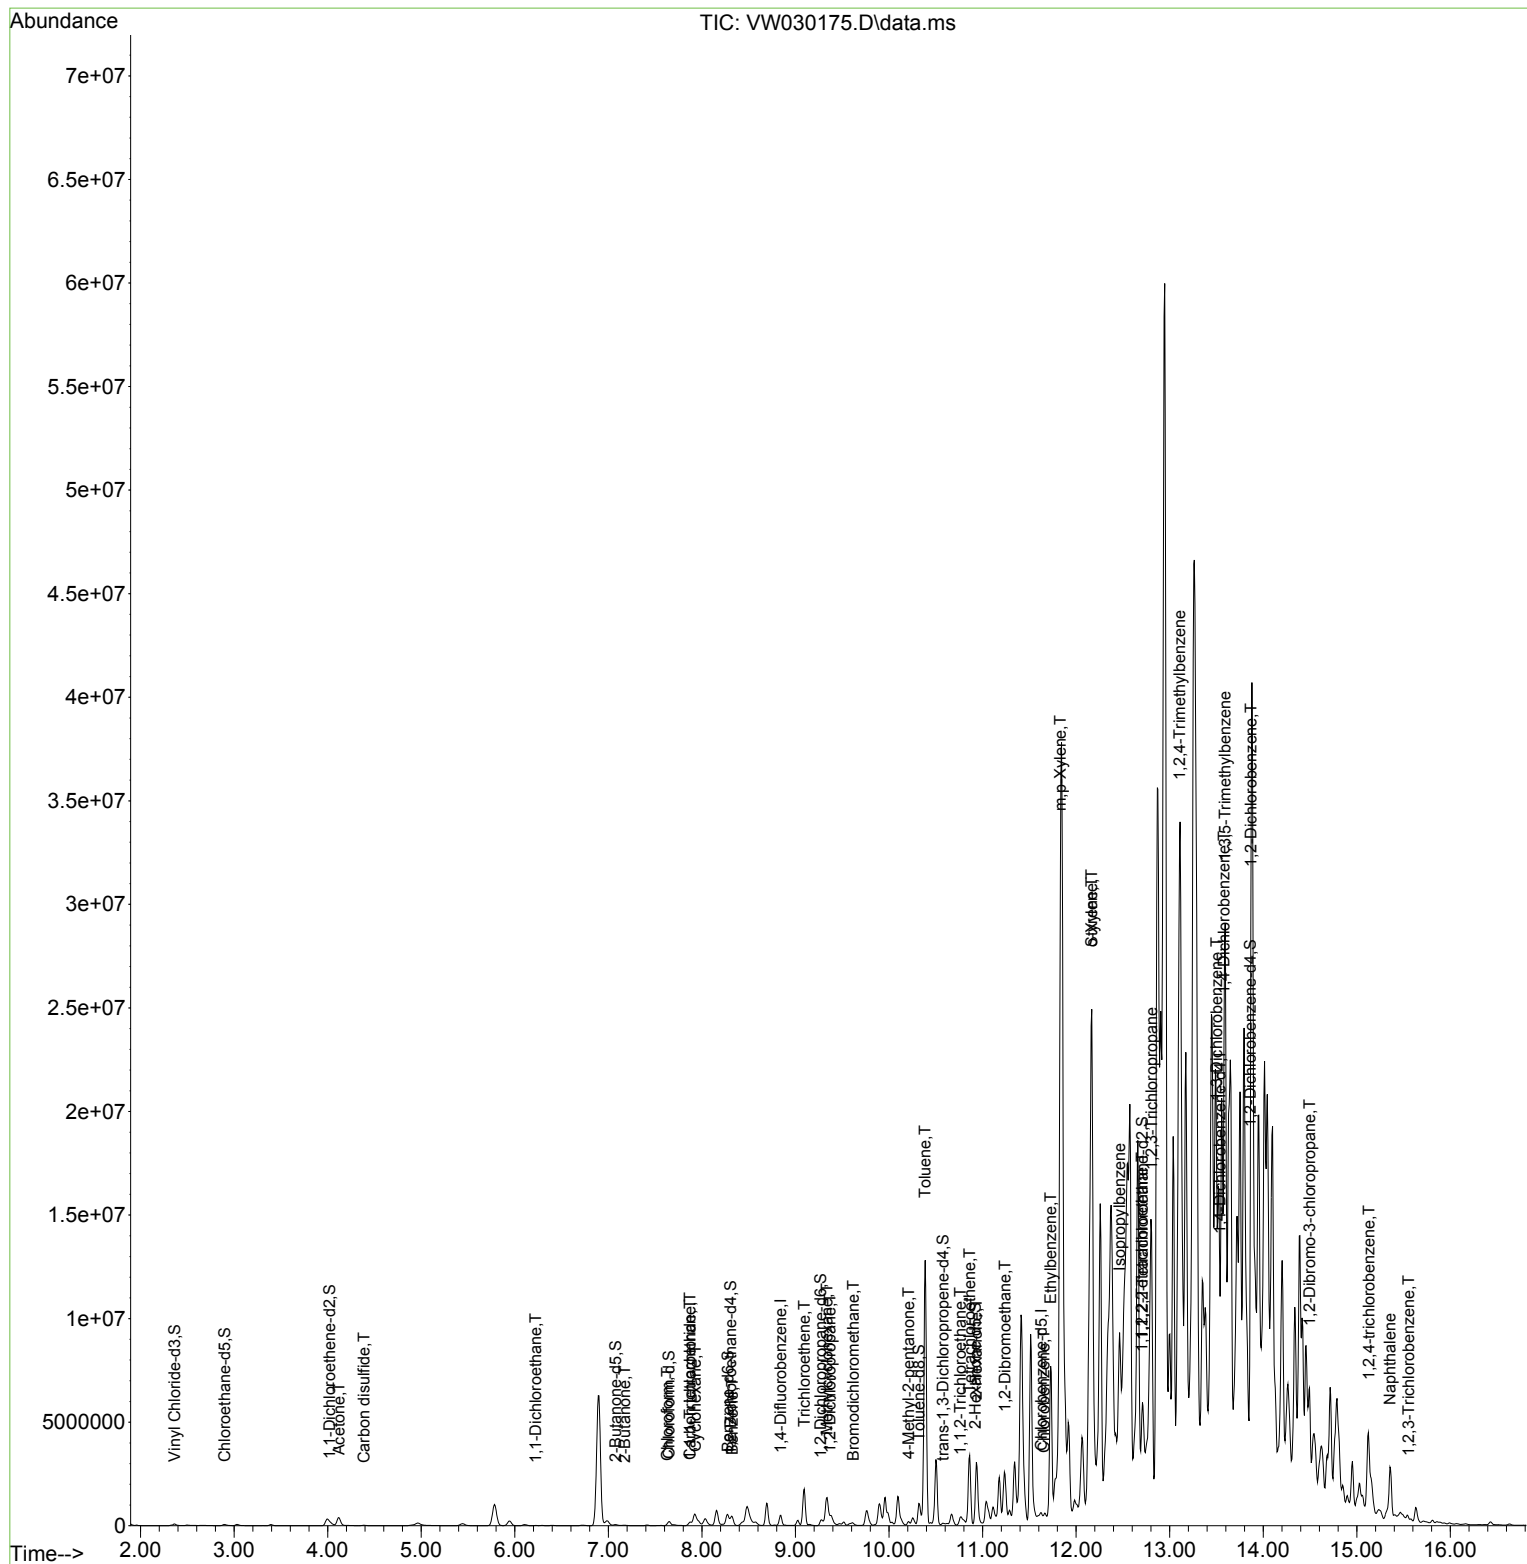



#13

Acetone

Concen: 434.719 ug/L

RT: 4.119 min Scan# 366

Delta R.T. -0.018 min


Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W

ClientSampleId :






Tgt Ion: 43 Resp: 648890

Ion Ratio Lower Upper

43 100

58 33.9 0.0 65.0

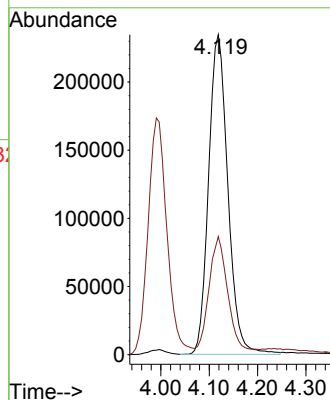

#14

Carbon disulfide

Concen: 2.987 ug/L

RT: 4.387 min Scan# 410

Delta R.T. -0.006 min

Lab File: VW030175.D




Acq: 20 Sep 2024 15:14


Tgt Ion: 76 Resp: 42148

Ion Ratio Lower Upper

76 100


78 8.3 7.6 11.4

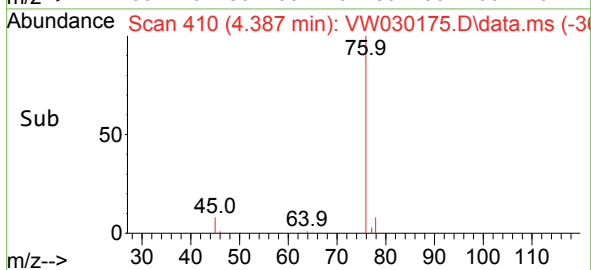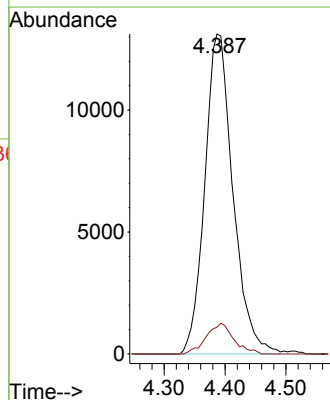






#19
1,1-Dichloroethane
Concen: 0.545 ug/L
RT: 6.222 min Scan# 711
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion: 63 Resp: 6058
Ion Ratio Lower Upper
63 100
65 37.0 21.6 40.0
83 13.3 9.0 16.8

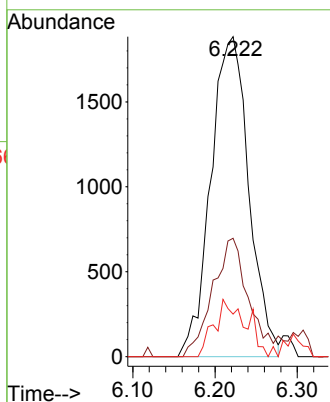

#22
2-Butanone
Concen: 8.655 ug/L
RT: 7.173 min Scan# 867
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion: 43 Resp: 15292
Ion Ratio Lower Upper
43 100
72 27.2 13.9 41.7

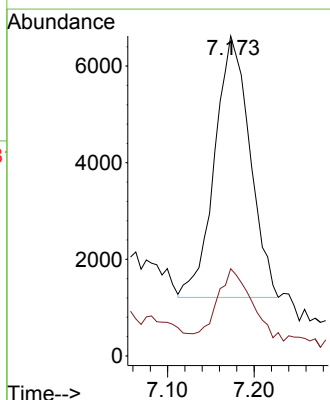



#25

Chloroform

Concen: 0.424 ug/L

RT: 7.630 min Scan# 942

Delta R.T. -0.049 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 83 Resp: 4789

Ion Ratio Lower Upper

83 100

85 36.9 46.1 85.5#

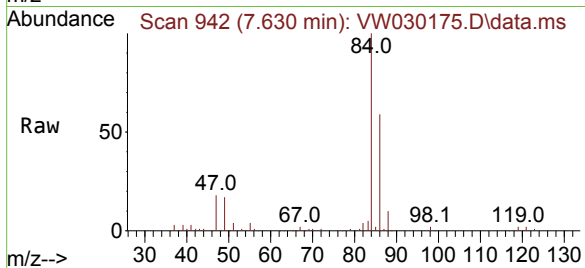

#29

Cyclohexane

Concen: 32.706 ug/L

RT: 7.929 min Scan# 991

Delta R.T. -0.030 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14




Tgt Ion: 56 Resp: 111313


Ion Ratio Lower Upper

56 100

69 49.5 24.6 37.0#

84 140.6 68.9 103.3#


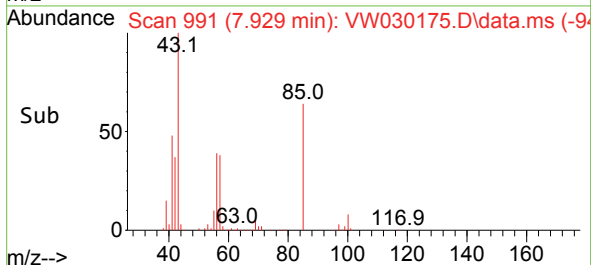
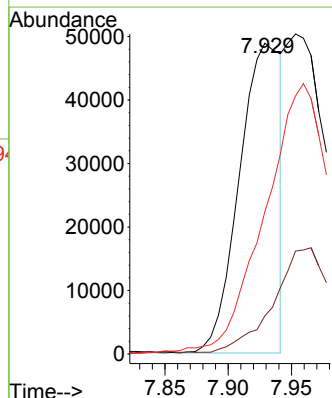
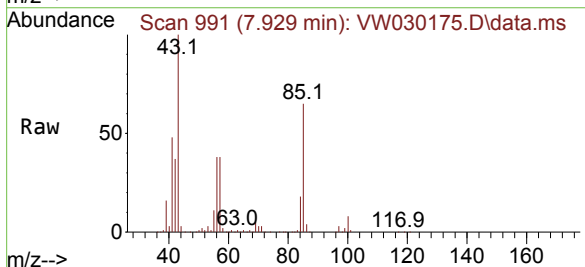


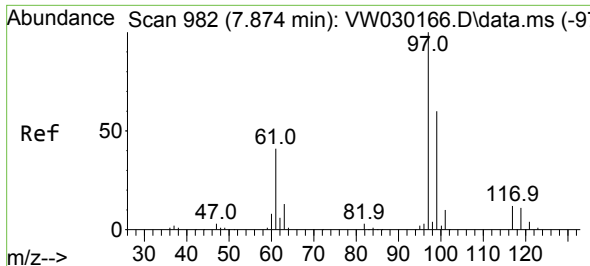

#30
1,1,1-Trichloroethane
Concen: 40.538 ug/L
RT: 7.874 min Scan# 982
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 97 Resp: 156631
Ion Ratio Lower Upper
97 100
99 65.0 51.3 76.9
61 40.5 36.4 54.6

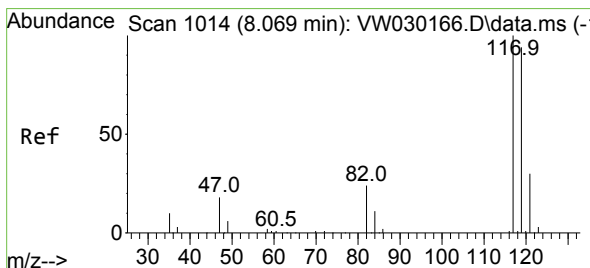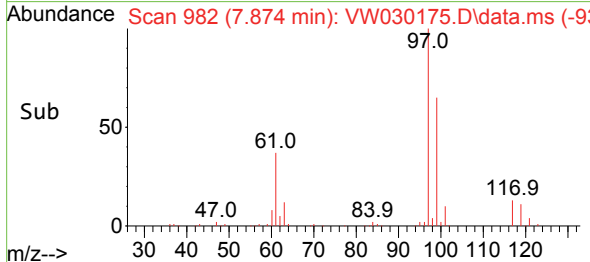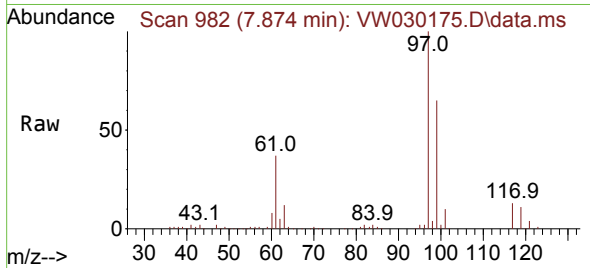

#31
Carbon tetrachloride
Concen: 5.986 ug/L
RT: 7.874 min Scan# 982
Delta R.T. -0.195 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion: 117 Resp: 21018
Ion Ratio Lower Upper
117 100
119 94.8 76.2 114.4

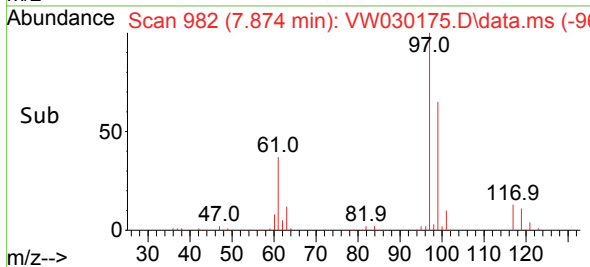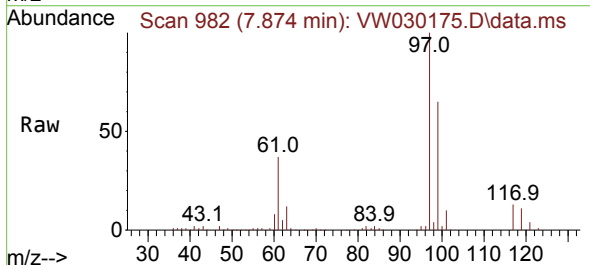

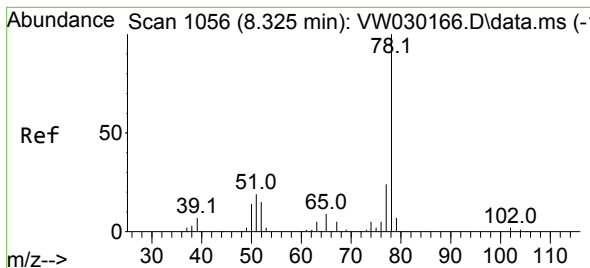

#33

Benzene

Concen: 39.771 ug/L

RT: 8.325 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VW030175.D





Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion: 78 Resp: 388428

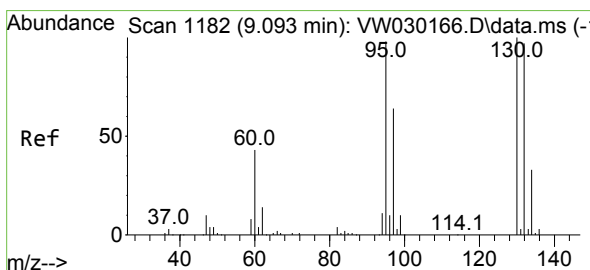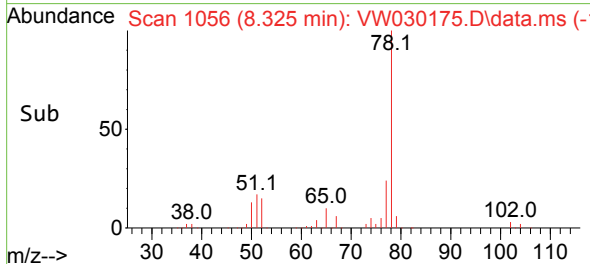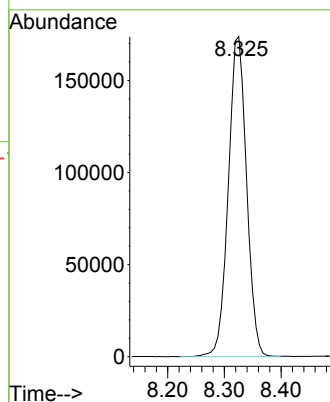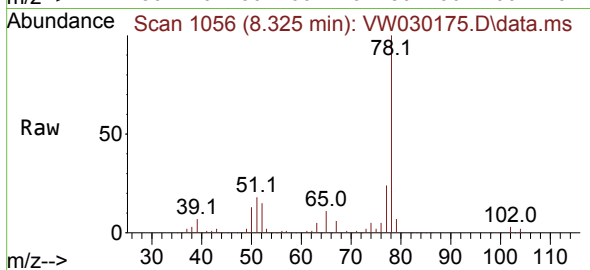

#34

Trichloroethene

Concen: 241.097 ug/L

RT: 9.093 min Scan# 1182

Delta R.T. 0.000 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Tgt Ion: 95 Resp: 635643




Ion Ratio Lower Upper


95 100

97 60.9 45.2 84.0

132 104.1 64.8 120.3

130 105.4 69.8 129.6


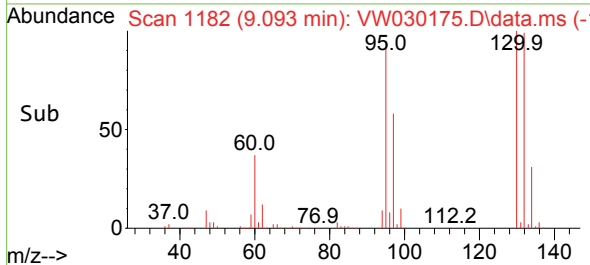
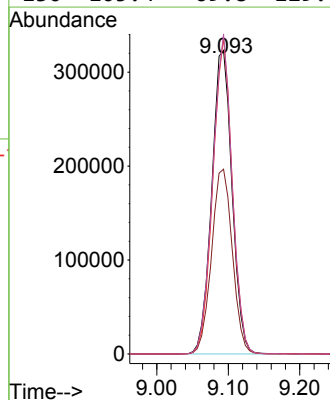
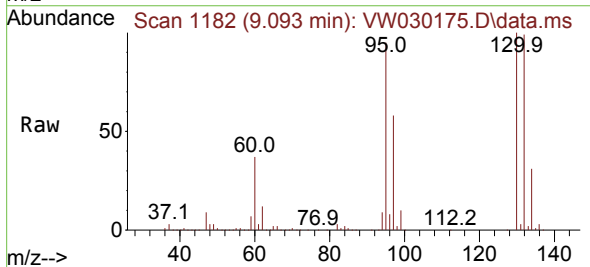


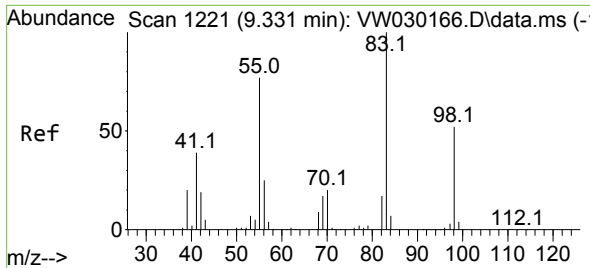

#35
Methylcyclohexane
Concen: 147.669 ug/L
RT: 9.337 min Scan# 11
Delta R.T. 0.006 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 83 Resp: 600207
Ion Ratio Lower Upper
83 100
55 86.4 63.0 94.6
98 48.6 38.7 58.1

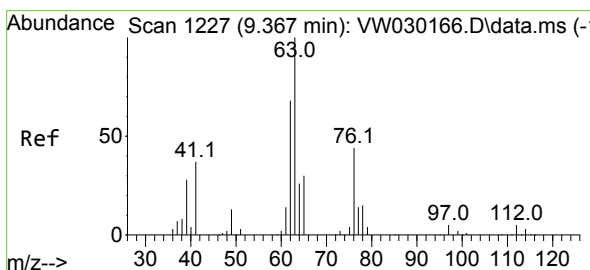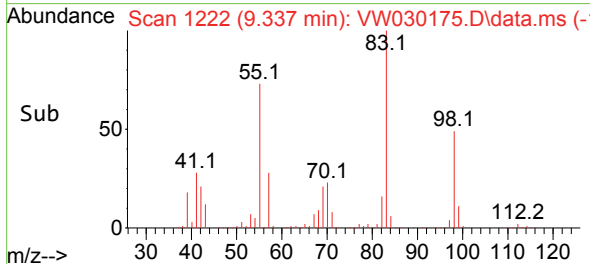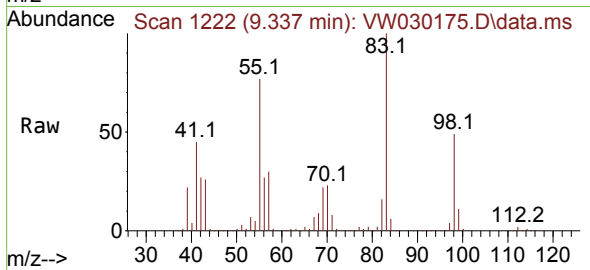

#37
1,2-Dichloropropane
Concen: 18.098 ug/L
RT: 9.368 min Scan# 1227
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14


Tgt Ion: 63 Resp: 47907
Ion Ratio Lower Upper
63 100
112 29.7 3.5 5.3#

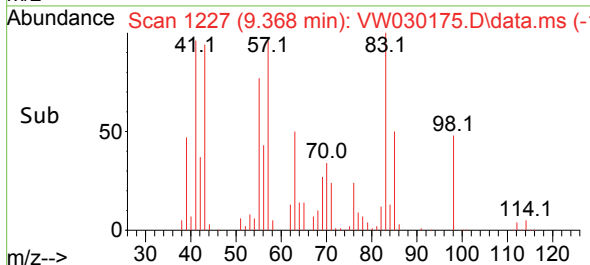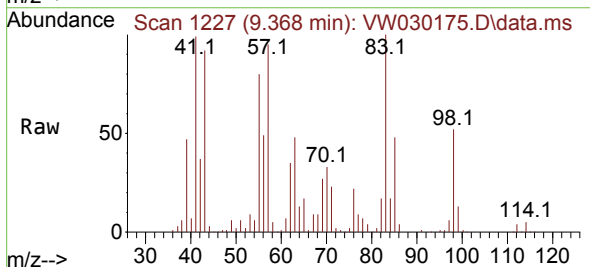



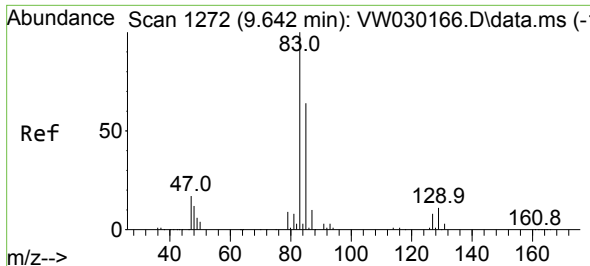


#38
Bromodichloromethane
Concen: 1.758 ug/L
RT: 9.618 min Scan# 1268
Delta R.T. -0.024 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Instrument :
MSVOA_W
ClientSampleId :



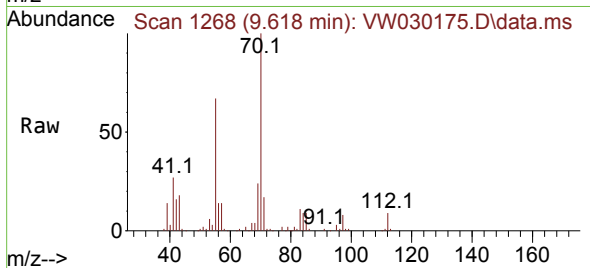



Tgt Ion: 83 Resp: 5861
Ion Ratio Lower Upper
83 100
85 78.4 42.6 79.0
127 0.0 6.3 9.5#

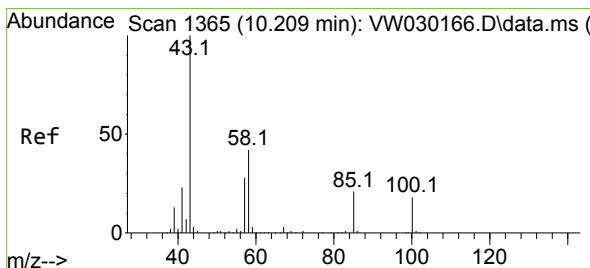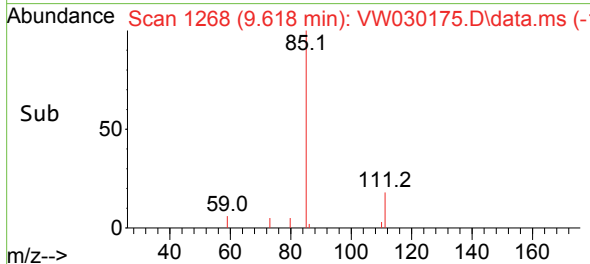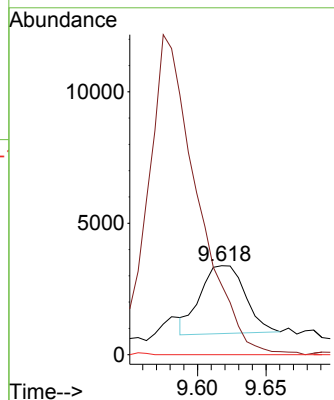

#40
4-Methyl-2-pentanone
Concen: 66.015 ug/L
RT: 10.209 min Scan# 1365
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion: 43 Resp: 89292
Ion Ratio Lower Upper
43 100
58 48.7 32.7 49.1
100 21.2 12.7 19.1#

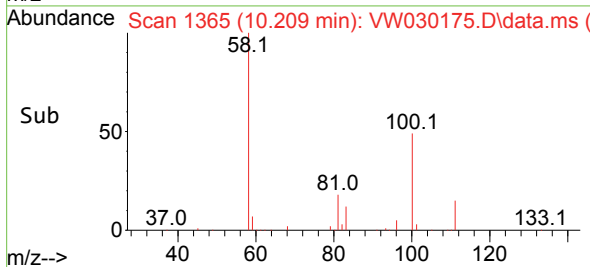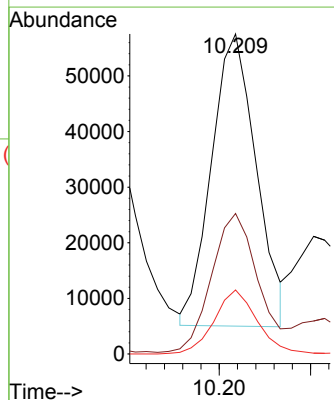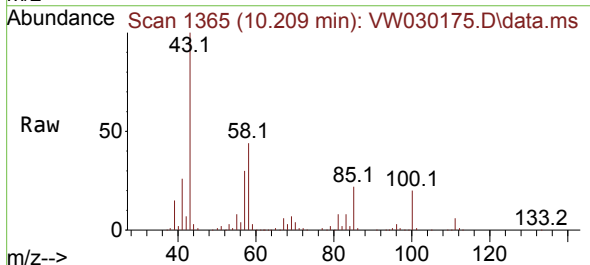



#42

Toluene

Concen: 941.958 ug/L

RT: 10.386 min Scan# 1

Delta R.T. 0.000 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion: 91 Resp: 9761802

Ion Ratio Lower Upper

91 100

92 59.8 40.7 75.5

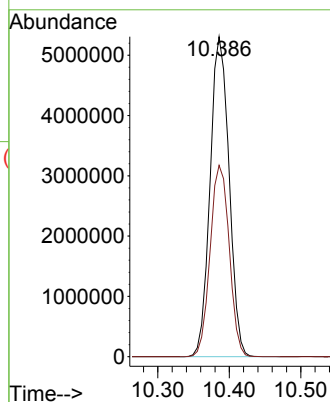

#45

1,1,2-Trichloroethane

Concen: 84.173 ug/L

RT: 10.764 min Scan# 1456

Delta R.T. -0.018 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Tgt Ion: 97 Resp: 162133




Ion Ratio Lower Upper


97 100

99 0.3 45.6 84.8#

83 9.2 64.0 119.0#

85 18.1 38.9 72.3#

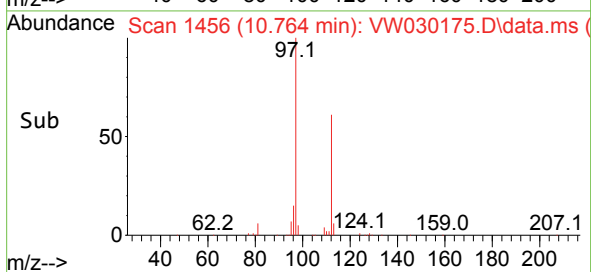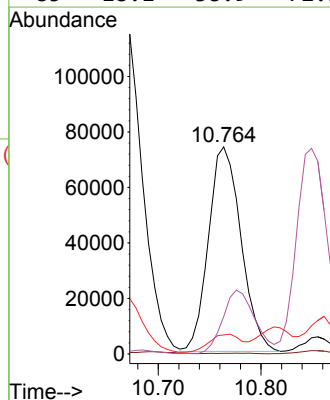



#46

Tetrachloroethene

Concen: 386.975 ug/L

RT: 10.861 min Scan# 1472

Delta R.T. 0.000 min


Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W

ClientSampleId :



Tgt Ion:164 Resp: 752816




Ion Ratio Lower Upper

164 100

129 91.8 66.0 122.6

131 86.5 64.8 120.4

166 119.9 81.6 151.6

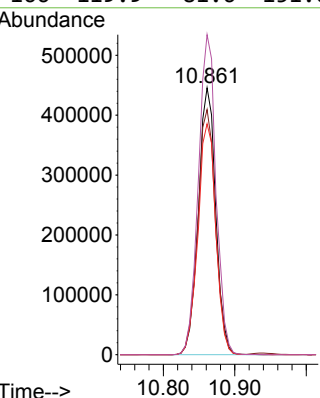

#48

2-Hexanone

Concen: 1938.971 ug/L

RT: 10.934 min Scan# 1484

Delta R.T. -0.030 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Tgt Ion: 43 Resp: 2016814




Ion Ratio Lower Upper


43 100

58 0.9 44.8 67.2#

57 22.4 15.4 23.2


100 0.0 9.6 14.4#

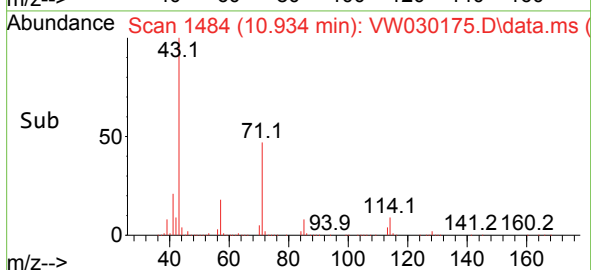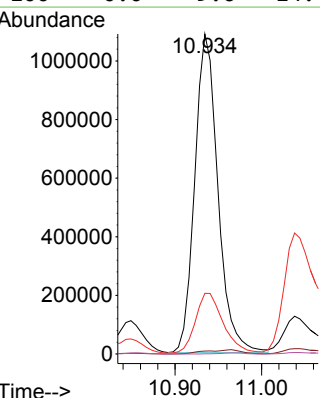






#50
1,2-Dibromoethane
Concen: 0.624 ug/L
RT: 11.239 min Scan# 1533
Delta R.T. 0.006 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:107 Resp: 1108
Ion Ratio Lower Upper
107 100
109 559.8 68.7 127.7#
188 0.0 2.6 4.0#

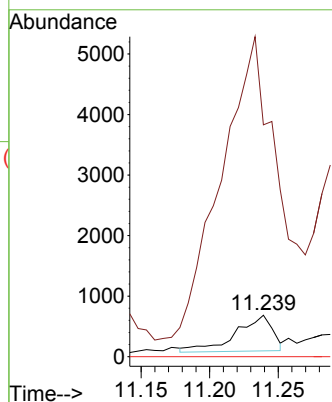

#51
Chlorobenzene
Concen: 12.631 ug/L
RT: 11.654 min Scan# 1602
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion:112 Resp: 84548
Ion Ratio Lower Upper
112 100
114 33.0 23.8 44.2
77 62.4 52.9 79.3



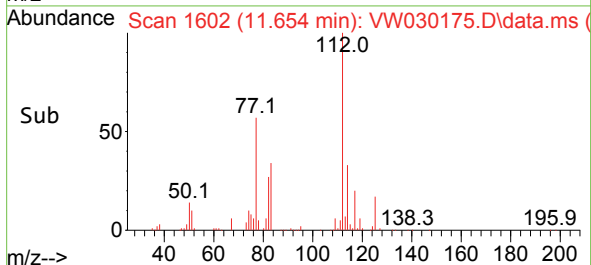
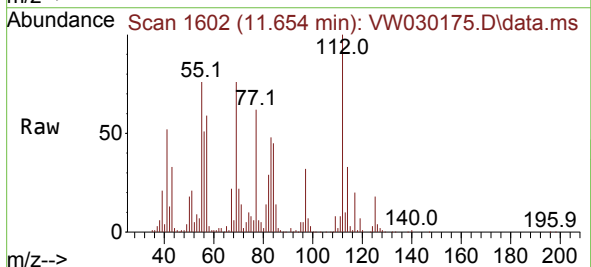




#52
Ethylbenzene
Concen: 449.608 ug/L
RT: 11.727 min Scan# 1
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 91 Resp: 5333575
Ion Ratio Lower Upper
91 100
106 29.5 21.9 40.7

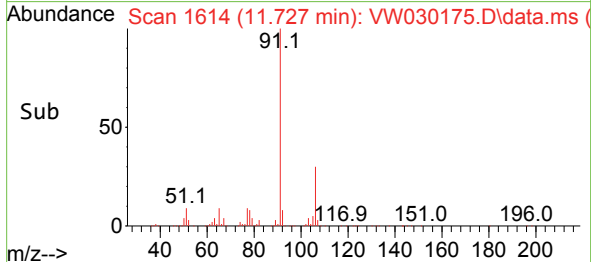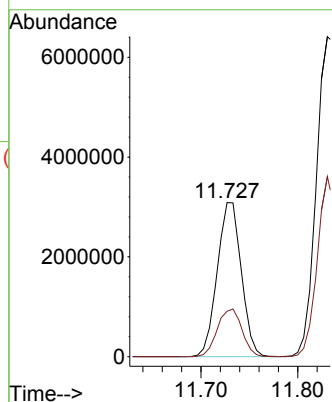

#53
m,p-Xylene
Concen: 1551.855 ug/L
RT: 11.831 min Scan# 1631
Delta R.T. -0.006 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion:106 Resp: 6792347
Ion Ratio Lower Upper
106 100
91 177.6 152.9 283.9





#54

o-Xylene

Concen: 1479.784 ug/L

RT: 12.166 min Scan# 1

Delta R.T. 0.006 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W





ClientSampleId :

Tgt Ion:106 Resp: 6094803

Ion Ratio Lower Upper

106 100

91 189.5 158.1 293.7



#55

Styrene

Concen: 44.256 ug/L

RT: 12.166 min Scan# 1686

Delta R.T. -0.012 min

Lab File: VW030175.D




Acq: 20 Sep 2024 15:14


Tgt Ion:104 Resp: 316168

Ion Ratio Lower Upper

104 100

78 301.8 31.4 58.2#

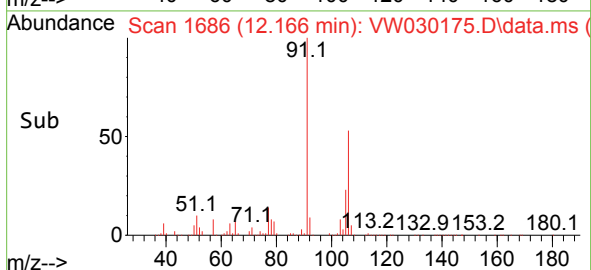



#57

1,1,2-Tetrachloroethane

Concen: 15.344 ug/L

RT: 12.702 min Scan# 1

Delta R.T. -0.006 min

Lab File: VW030175.D





Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W

ClientSampleId :

Tgt Ion:	83	Resp:	35278
Ion	Ratio	Lower	Upper
83	100		
85	209.3	44.5	82.7#
131	0.4	7.4	11.2#



#60

Isopropylbenzene

Concen: 235.341 ug/L




RT: 12.465 min Scan# 1735


Delta R.T. 0.006 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Tgt Ion:	105	Resp:	3610542
Ion	Ratio	Lower	Upper
105	100		
120	26.7	20.2	30.2
77	15.4	13.0	19.4



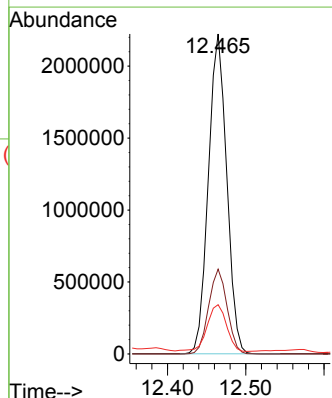





#61
1,2,3-Trichloropropane
Concen: 26.563 ug/L
RT: 12.806 min Scan# 1
Delta R.T. 0.037 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 75 Resp: 57580
Ion Ratio Lower Upper
75 100
77 735.9 26.2 39.2#
110 335.1 29.7 44.5#

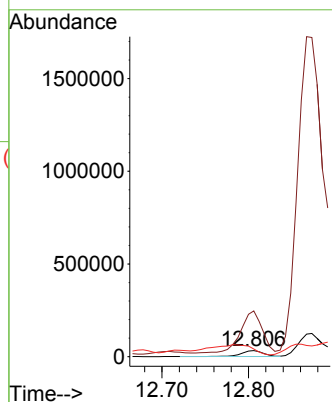

#62
1,3,5-Trimethylbenzene
Concen: 1284.742 ug/L
RT: 13.592 min Scan# 1920
Delta R.T. 0.653 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14


Tgt Ion:105 Resp:14446197
Ion Ratio Lower Upper
105 100
120 46.6 37.3 55.9

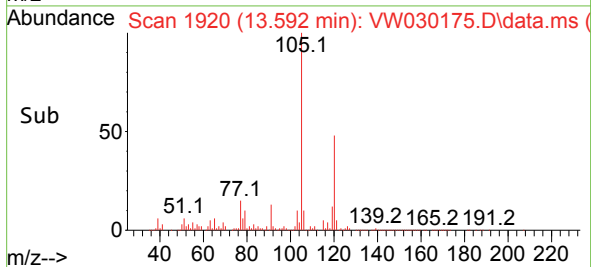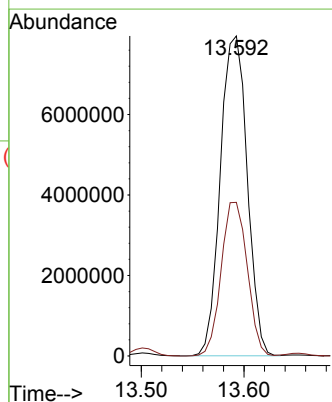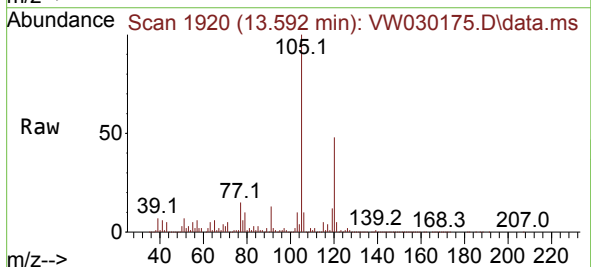






#63
1,2,4-Trimethylbenzene
Concen: 1438.553 ug/L
RT: 13.105 min Scan# 11
Delta R.T. -0.140 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Instrument :
MSVOA_W
ClientSampleId :







Tgt Ion:105 Resp:16816272
Ion Ratio Lower Upper
105 100
120 36.0 34.8 52.2

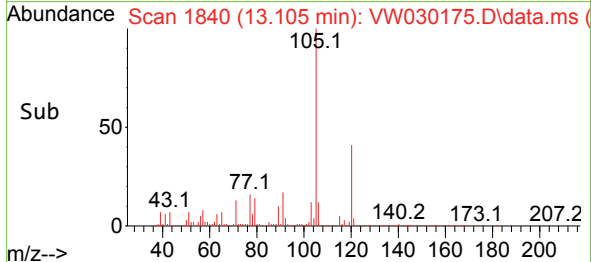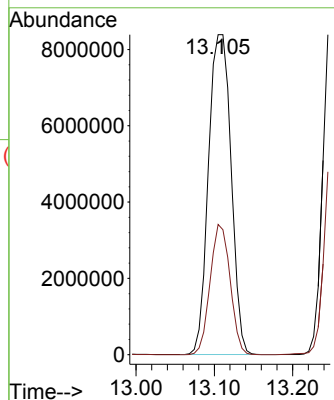

#64
1,3-Dichlorobenzene
Concen: 0.963 ug/L
RT: 13.501 min Scan# 1905
Delta R.T. 0.006 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion:146 Resp: 6547
Ion Ratio Lower Upper
146 100
111 4220.4 31.9 59.3#
148 59.3 47.7 88.5


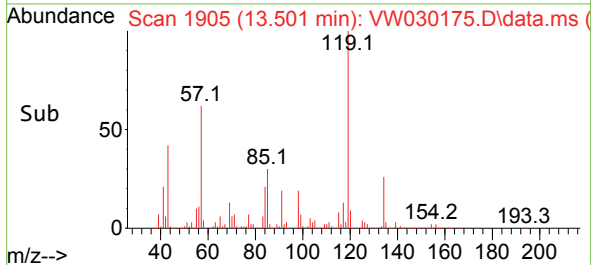
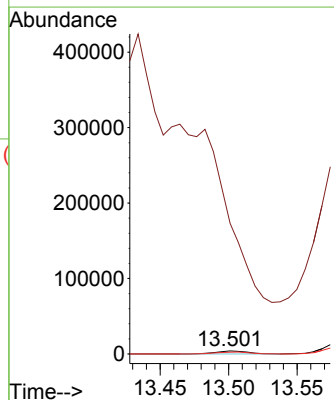
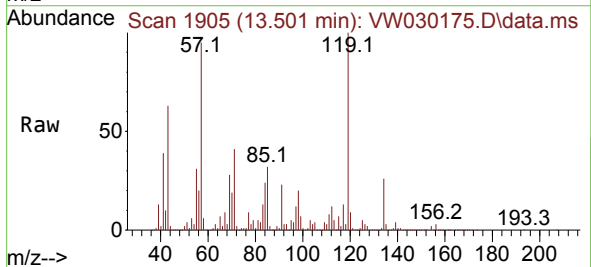


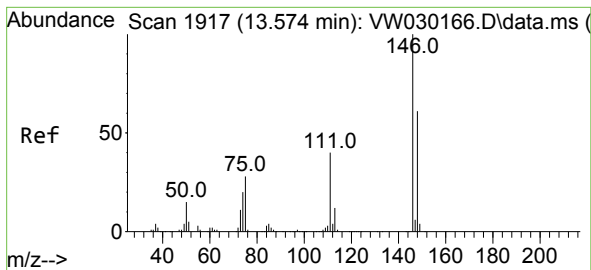

#65
1,4-Dichlorobenzene
Concen: 3.586 ug/L
RT: 13.580 min Scan# 1918
Delta R.T. 0.006 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion:146 Resp: 25191
Ion Ratio Lower Upper
146 100
111 1724.9 29.5 54.7#
148 65.1 44.4 82.5

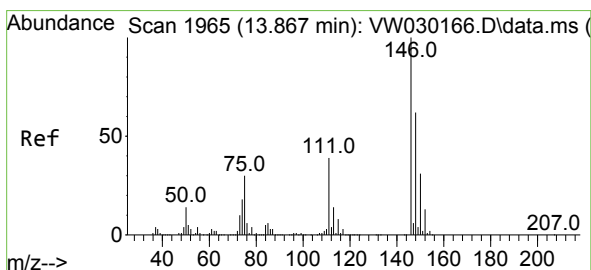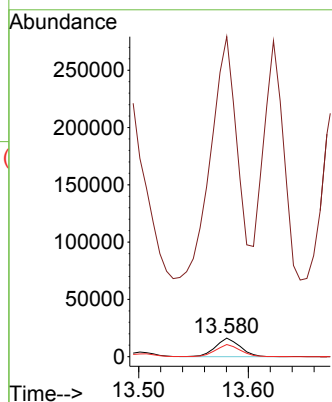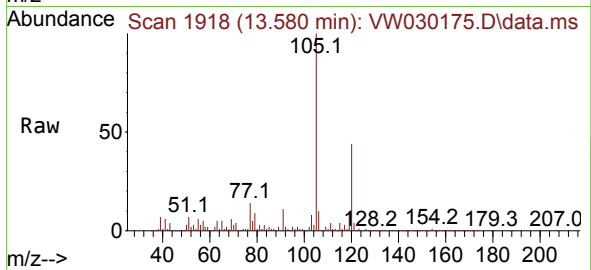

#67
1,2-Dichlorobenzene
Concen: 6.315 ug/L
RT: 13.867 min Scan# 1965
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion:146 Resp: 38697
Ion Ratio Lower Upper
146 100
111 602.5 32.7 49.1#
148 66.2 49.8 74.6


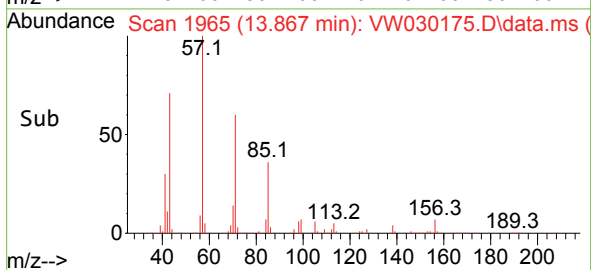
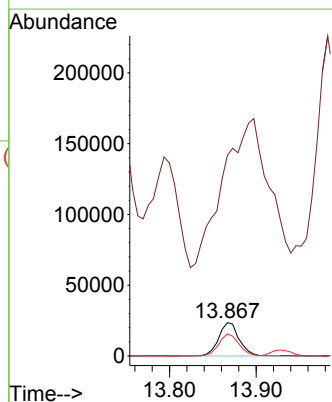
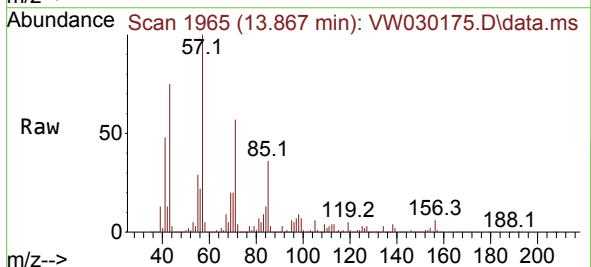




#68
1,2-Dibromo-3-chloropropane
Concen: 38.692 ug/L
RT: 14.495 min Scan# 2068
Delta R.T. 0.019 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14




Instrument :
MSVOA_W
ClientSampleId :


Tgt Ion: 75 Resp: 18292
Ion Ratio Lower Upper
75 100
155 22.7 60.5 90.7#
157 4.2 66.9 100.3#

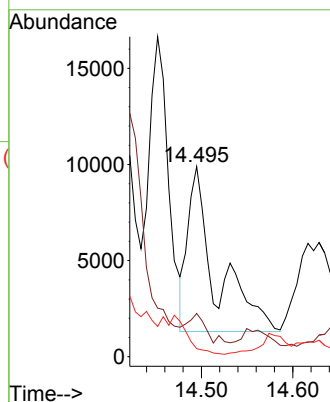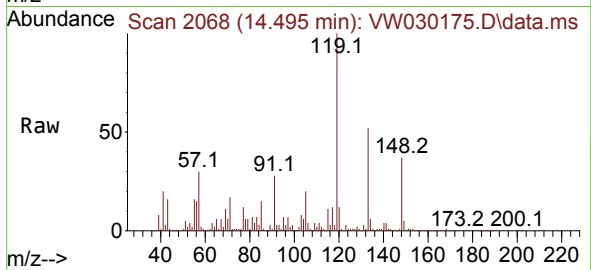

#70
1,2,4-trichlorobenzene
Concen: 2.547 ug/L
RT: 15.129 min Scan# 2172
Delta R.T. 0.000 min
Lab File: VW030175.D
Acq: 20 Sep 2024 15:14

Tgt Ion:180 Resp: 9790
Ion Ratio Lower Upper
180 100
182 95.8 73.4 110.2
145 2625.3 24.0 36.0#

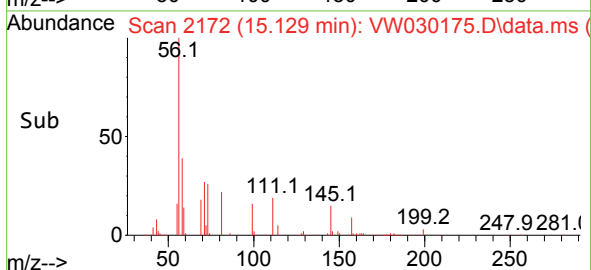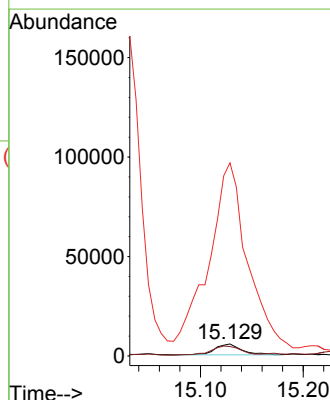



#71

Naphthalene

Concen: 296.990 ug/L

RT: 15.354 min Scan# 2210

Delta R.T. -0.006 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Instrument :

MSVOA_W

ClientSampleId :





Tgt Ion:128 Resp: 2073336

Ion Ratio Lower Upper

128 100

127 13.7 10.1 15.1

129 11.0 8.4 12.6

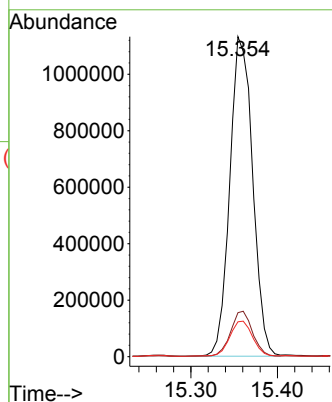

#72

1,2,3-Trichlorobenzene

Concen: 0.896 ug/L

RT: 15.556 min Scan# 2242

Delta R.T. 0.006 min

Lab File: VW030175.D

Acq: 20 Sep 2024 15:14

Tgt Ion:180 Resp: 3021

Ion Ratio Lower Upper

180 100

182 32.1 76.4 114.6#

145 0.0 26.2 39.4#

