

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
 Data File : VW030186.D
 Acq On : 20 Sep 2024 19:38
 Operator : SY/MD
 Sample : P4109-22
 Misc : 5.42g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EW7

Quant Time: Sep 20 23:57:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 20 23:43:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	840315	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	780177	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	373531	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	150372	13.857	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.440%
7) Chloroethane-d5	2.899	69	124775	16.286	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.160%
11) 1,1-Dichloroethene-d2	4.021	65	80276	14.805	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.240%
21) 2-Butanone-d5	7.075	46	93864	35.721	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.440%
24) Chloroform-d	7.648	84	388586	16.818	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	67.280%
26) 1,2-Dichloroethane-d4	8.306	65	197148	16.992	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	67.960%#
32) Benzene-d6	8.270	84	799745	17.794	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	71.160%
36) 1,2-Dichloropropane-d6	9.270	67	235646	16.981	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	67.920%#
41) Toluene-d8	10.324	98	753825	18.716	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.880%
43) trans-1,3-Dichloroprop...	10.574	79	95326	17.146	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.600%
47) 2-Hexanone-d5	10.922	63	87766	41.332	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	82.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	180821	17.502	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	70.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	245384	19.352	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.400%
Target Compounds					Qvalue	
13) Acetone	4.124	43	12811	4.249	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092024\
Data File : VW030186.D
Acq On : 20 Sep 2024 19:38
Operator : SY/MD
Sample : P4109-22
Misc : 5.42g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EW7

Quant Time: Sep 20 23:57:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 20 23:43:18 2024
Response via : Initial Calibration

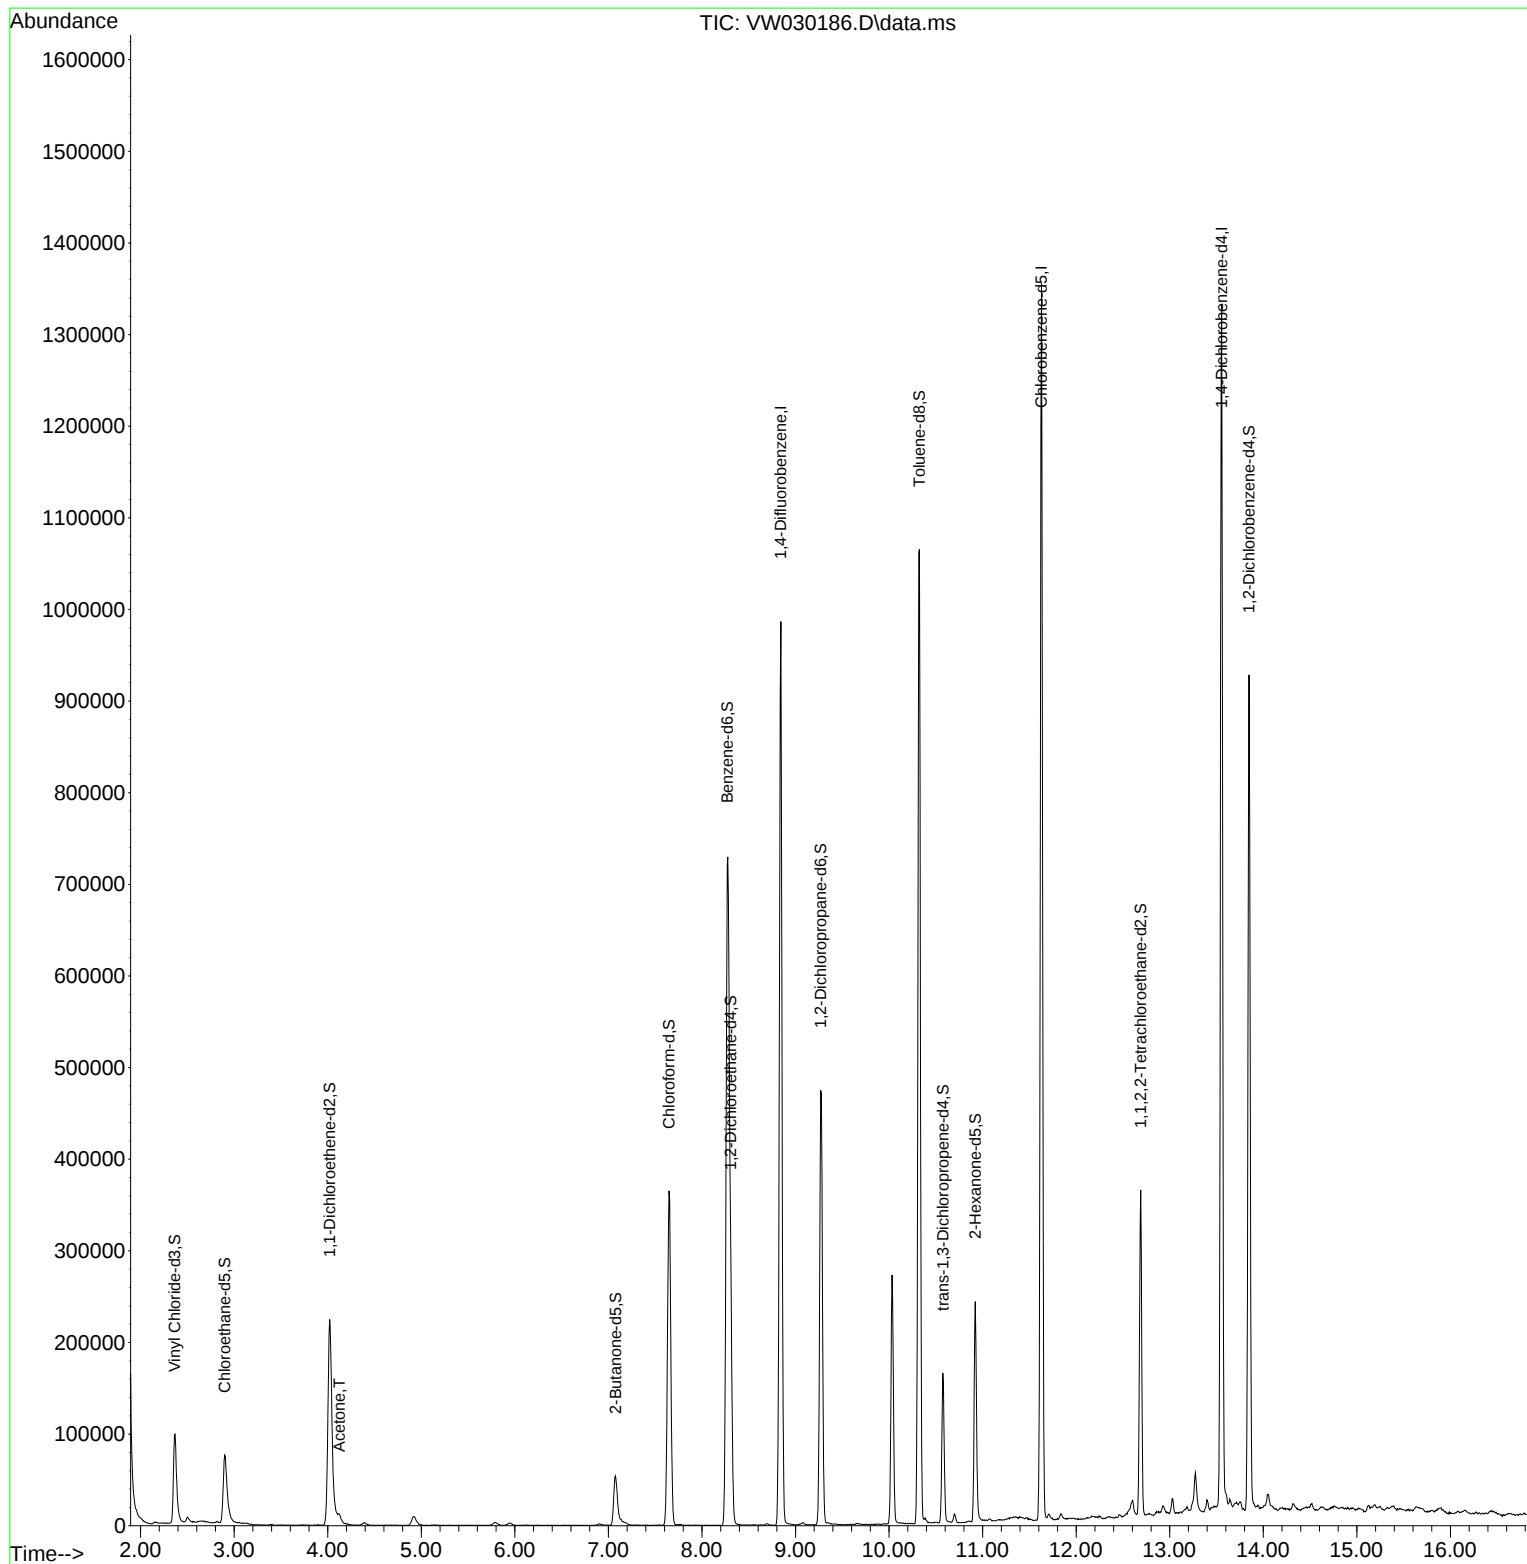

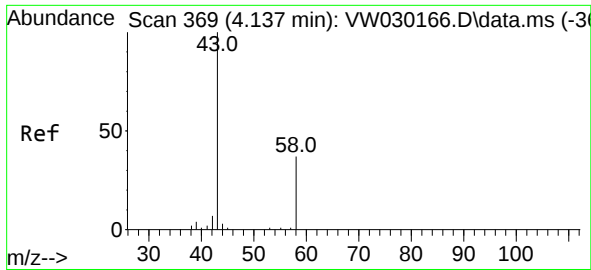

#13
 Acetone
 Concen: 4.249 ug/L
 RT: 4.124 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW030186.D
 Acq: 20 Sep 2024 19:38

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EW7

Tgt Ion: 43 Resp: 12811
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 65.0

