

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092222\
 Data File : VW024627.D
 Acq On : 22 Sep 2022 11:00
 Operator : SY/VA
 Sample : VW0922SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK407

Quant Time: Sep 23 00:43:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 23 00:42:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	335481	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	333526	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	150925	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	203590	26.600	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.400%
7) Chloroethane-d5	2.879	69	162307	25.100	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.400%
11) 1,1-Dichloroethene-d2	4.013	63	153984	18.138	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.560%
21) 2-Butanone-d5	7.086	46	44288	42.241	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.480%
24) Chloroform-d	7.647	84	214810	22.515	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.080%
26) 1,2-Dichloroethane-d4	8.305	65	129614	25.111	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.440%
32) Benzene-d6	8.275	84	447684	23.940	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.760%
36) 1,2-Dichloropropane-d6	9.274	67	121405	22.630	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.520%
41) Toluene-d8	10.323	98	428265	23.540	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.160%
43) trans-1,3-Dichloroprop...	10.579	79	53414	22.298	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.200%
47) 2-Hexanone-d5	10.927	63	36163	42.207	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.420%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	98374	21.026	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.120%
66) 1,2-Dichlorobenzene-d4	13.847	152	127257	23.552	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.200%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4821	0.662	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092222\
Data File : VW024627.D
Acq On : 22 Sep 2022 11:00
Operator : SY/VA
Sample : VW0922SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK407

Quant Time: Sep 23 00:43:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092122SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 23 00:42:09 2022
Response via : Initial Calibration

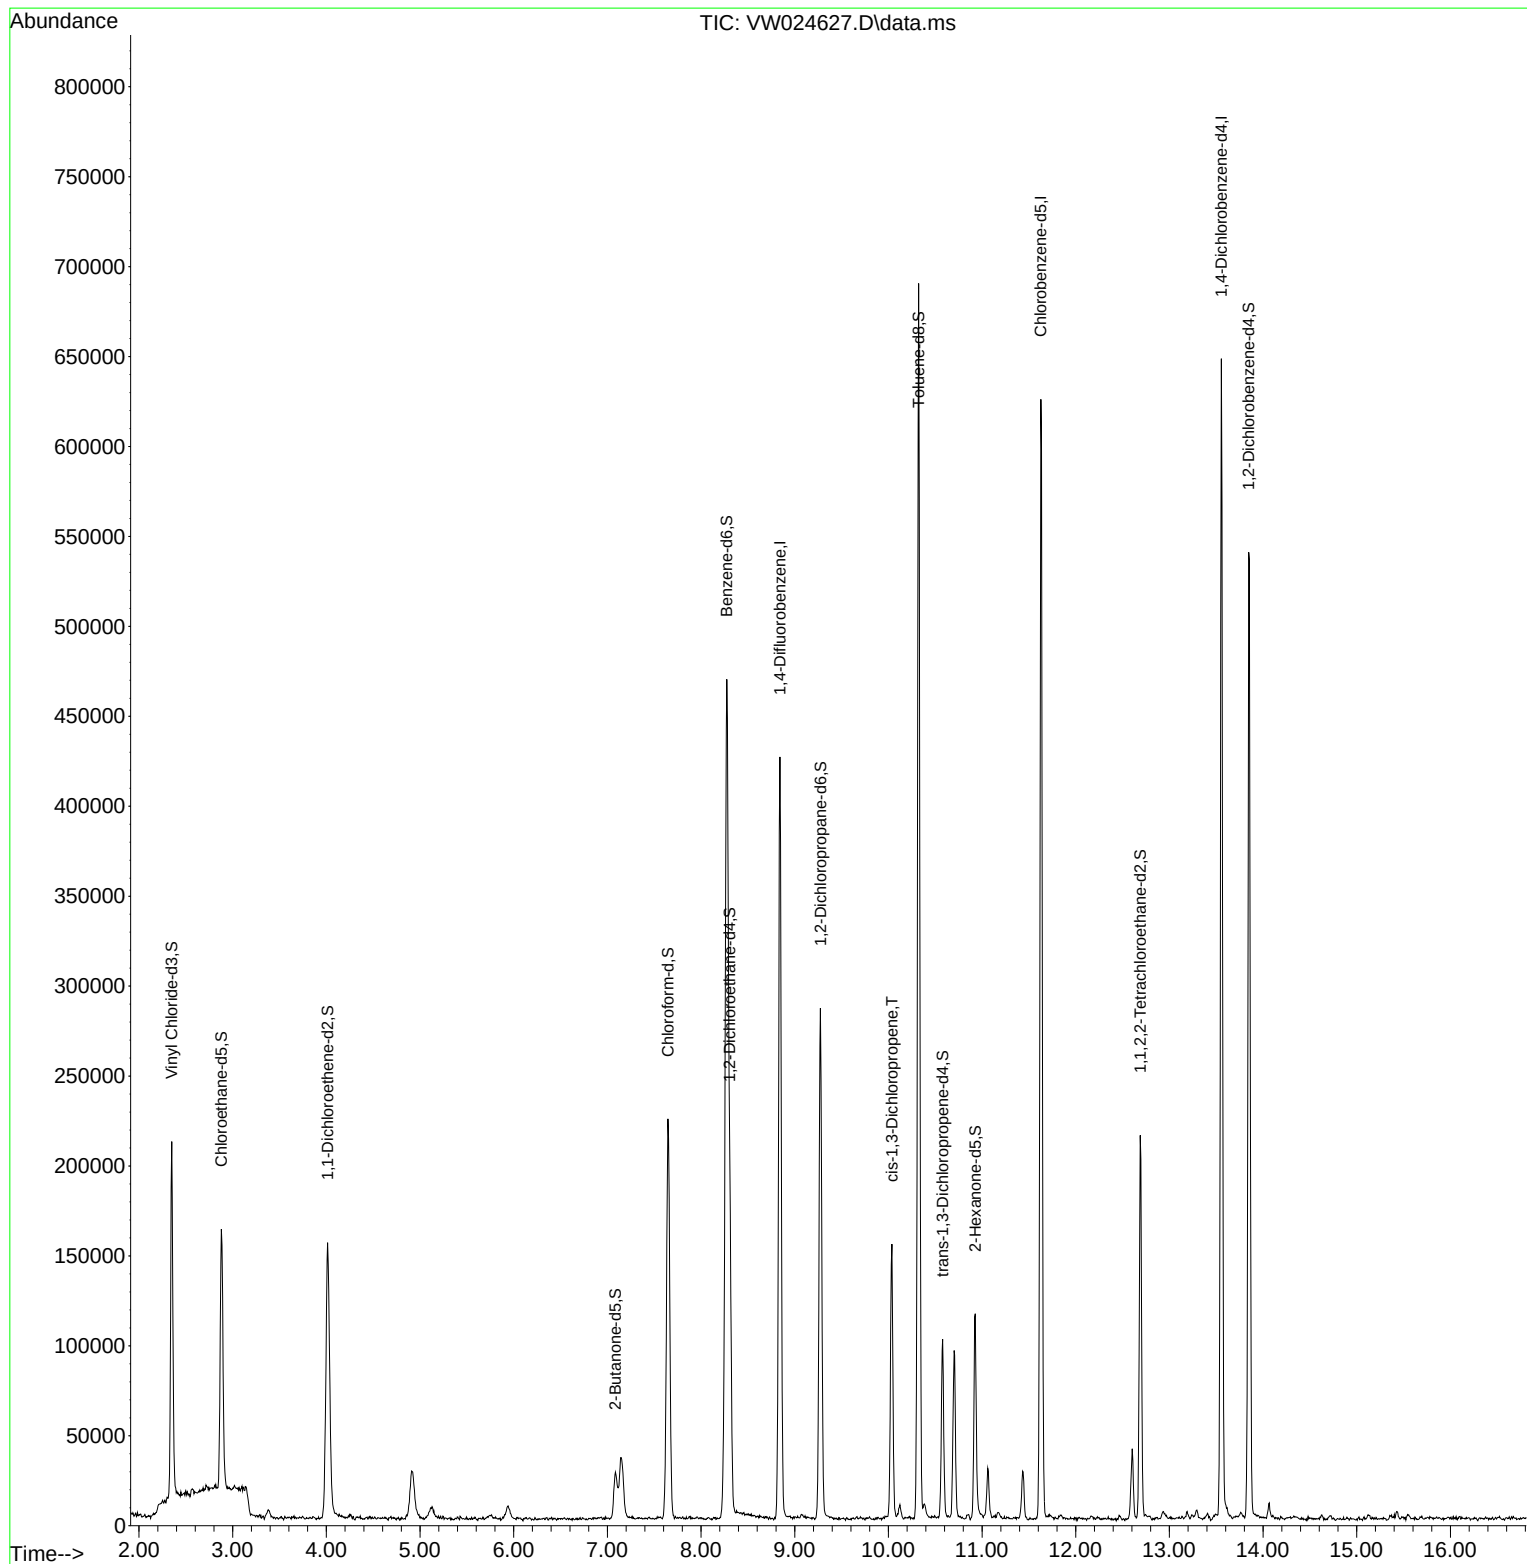

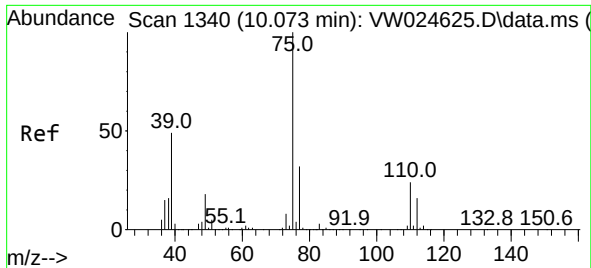

#39
 cis-1,3-Dichloropropene
 Concen: 0.662 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024627.D
 Acq: 22 Sep 2022 11:00

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK407

Tgt Ion: 75 Resp: 4821
 Ion Ratio Lower Upper
 75 100
 77 35.3 22.5 41.7

