

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
 Data File : VW030198.D
 Acq On : 23 Sep 2024 14:30
 Operator : SY/MD
 Sample : P4109-20
 Misc : 4.88g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 24 01:18:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 24 01:15:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	364735	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	334757	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	159863	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	103772	22.031	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.120%
7) Chloroethane-d5	2.905	69	84906	25.533	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.120%
11) 1,1-Dichloroethene-d2	4.027	65	45788	19.456	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	77.840%
21) 2-Butanone-d5	7.081	46	44170	38.728	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.460%
24) Chloroform-d	7.654	84	215493	21.488	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.960%
26) 1,2-Dichloroethane-d4	8.307	65	108903	21.625	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.480%
32) Benzene-d6	8.276	84	427767	22.182	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	88.720%
36) 1,2-Dichloropropane-d6	9.270	67	124922	20.980	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	83.920%
41) Toluene-d8	10.325	98	386809	22.382	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.520%
43) trans-1,3-Dichloroprop...	10.575	79	47072	19.732	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.920%
47) 2-Hexanone-d5	10.922	63	36972	40.578	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.160%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	87420	19.721	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.880%
66) 1,2-Dichlorobenzene-d4	13.849	152	127345	23.466	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.880%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3907	0.481	ug/L	Qvalue # 59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
Data File : VW030198.D
Acq On : 23 Sep 2024 14:30
Operator : SY/MD
Sample : P4109-20
Misc : 4.88g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 24 01:18:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 24 01:15:59 2024
Response via : Initial Calibration

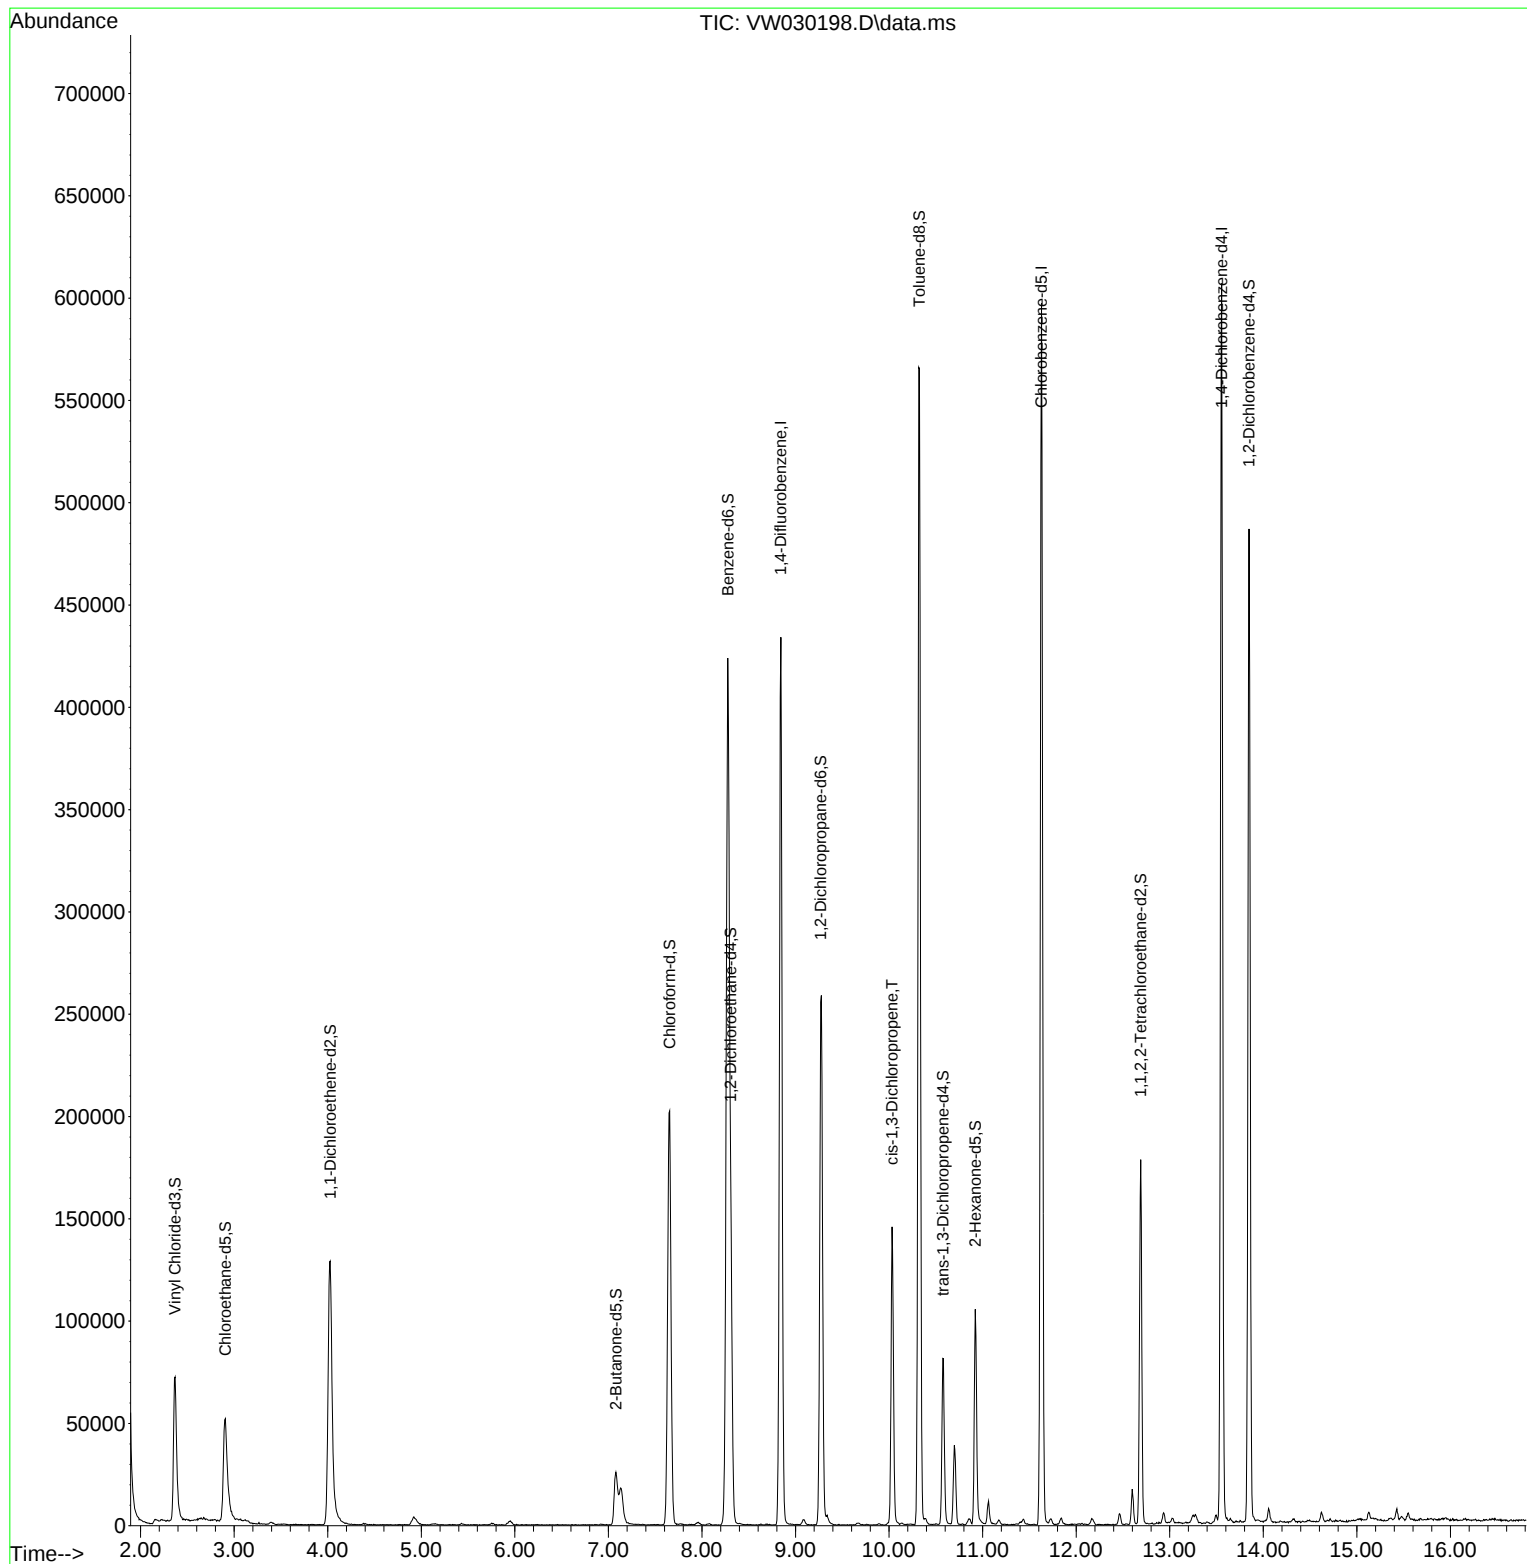

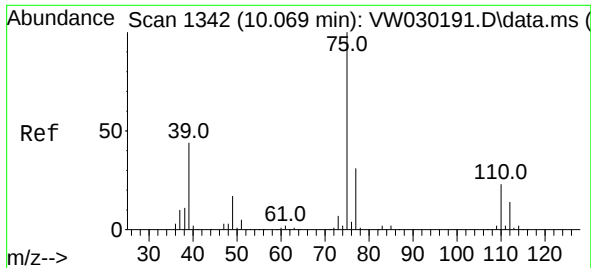

#39
 cis-1,3-Dichloropropene
 Concen: 0.481 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW030198.D
 Acq: 23 Sep 2024 14:30

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 3907
 Ion Ratio Lower Upper
 75 100
 77 51.8 20.7 38.5#

