

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
 Data File : VW030202.D
 Acq On : 23 Sep 2024 16:06
 Operator : SY/MD
 Sample : P4109-23
 Misc : 5.11g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 24 01:19:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 24 01:15:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	395160	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	353436	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	166678	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	105720	20.717	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.880%
7) Chloroethane-d5	2.899	69	87377	24.253	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.000%
11) 1,1-Dichloroethene-d2	4.021	65	46086	18.074	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.280%
21) 2-Butanone-d5	7.075	46	55602	44.997	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.000%
24) Chloroform-d	7.648	84	220806	20.322	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.280%
26) 1,2-Dichloroethane-d4	8.307	65	122199	22.397	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.600%
32) Benzene-d6	8.276	84	439525	21.587	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.360%
36) 1,2-Dichloropropane-d6	9.276	67	133929	21.304	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.200%
41) Toluene-d8	10.325	98	397932	21.809	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.240%
43) trans-1,3-Dichloroprop...	10.575	79	54025	21.450	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.800%
47) 2-Hexanone-d5	10.922	63	46977	48.834	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.660%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	106359	22.725	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.880%
66) 1,2-Dichlorobenzene-d4	13.849	152	136846	24.186	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.760%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4209	0.491	ug/L	# 54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
Data File : VW030202.D
Acq On : 23 Sep 2024 16:06
Operator : SY/MD
Sample : P4109-23
Misc : 5.11g/10mL/MSVOA_W/SOIL/B
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 24 01:19:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 24 01:15:59 2024
Response via : Initial Calibration

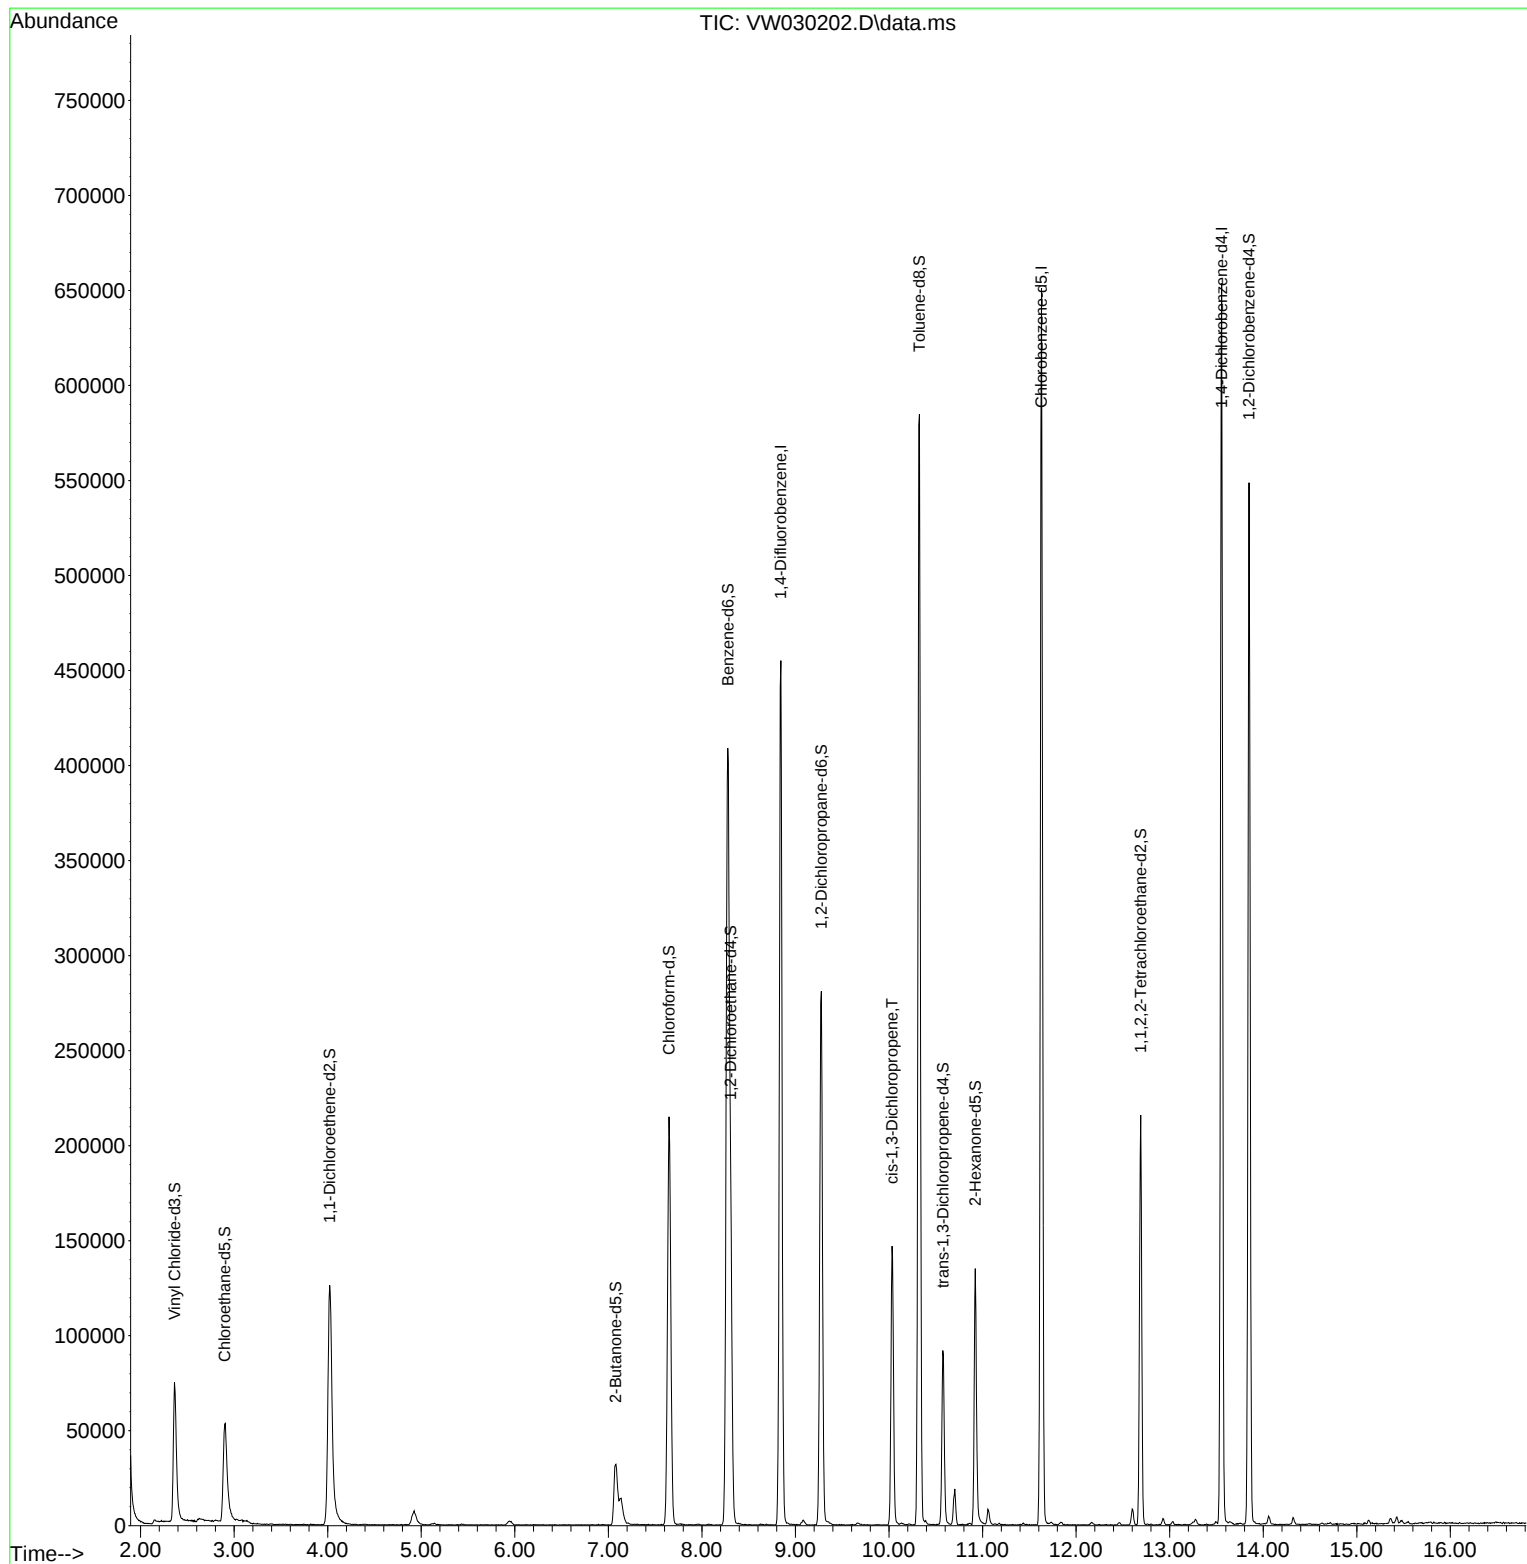

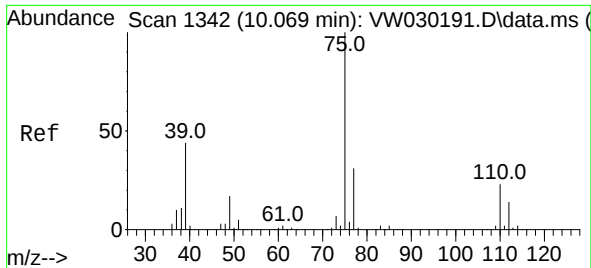

#39
cis-1,3-Dichloropropene
Concen: 0.491 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.036 min
Lab File: VW030202.D
Acq: 23 Sep 2024 16:06

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 4209
Ion Ratio Lower Upper
75 100
77 54.2 20.7 38.5#

