




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
Data File : VW030193.D
Acq On : 23 Sep 2024 11:29
Operator : SY/MD
Sample : P4109-14 RE
Misc : 4.95g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4ET6RE

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:31:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 24 01:15:59 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 09/25/2024
Supervised By :Mahesh Dadoda 09/25/2024

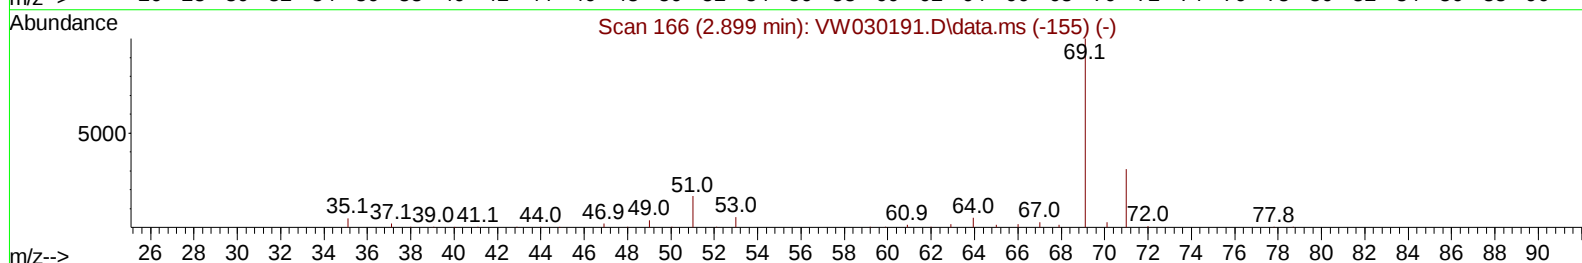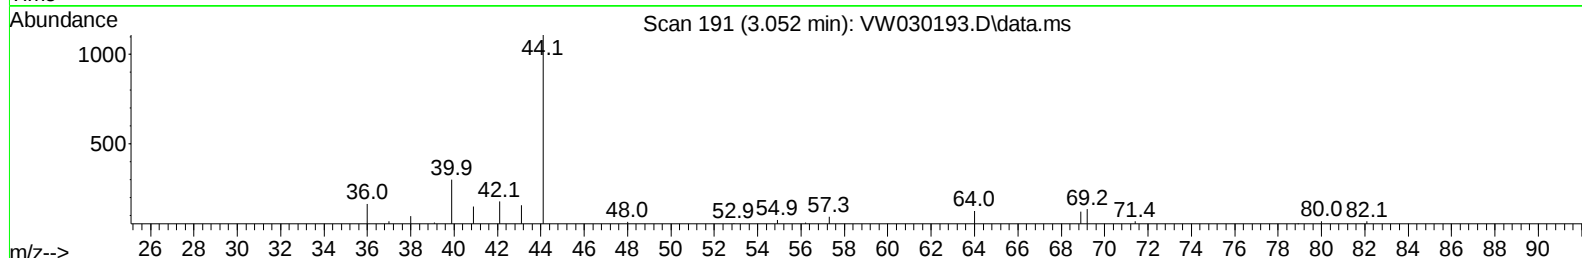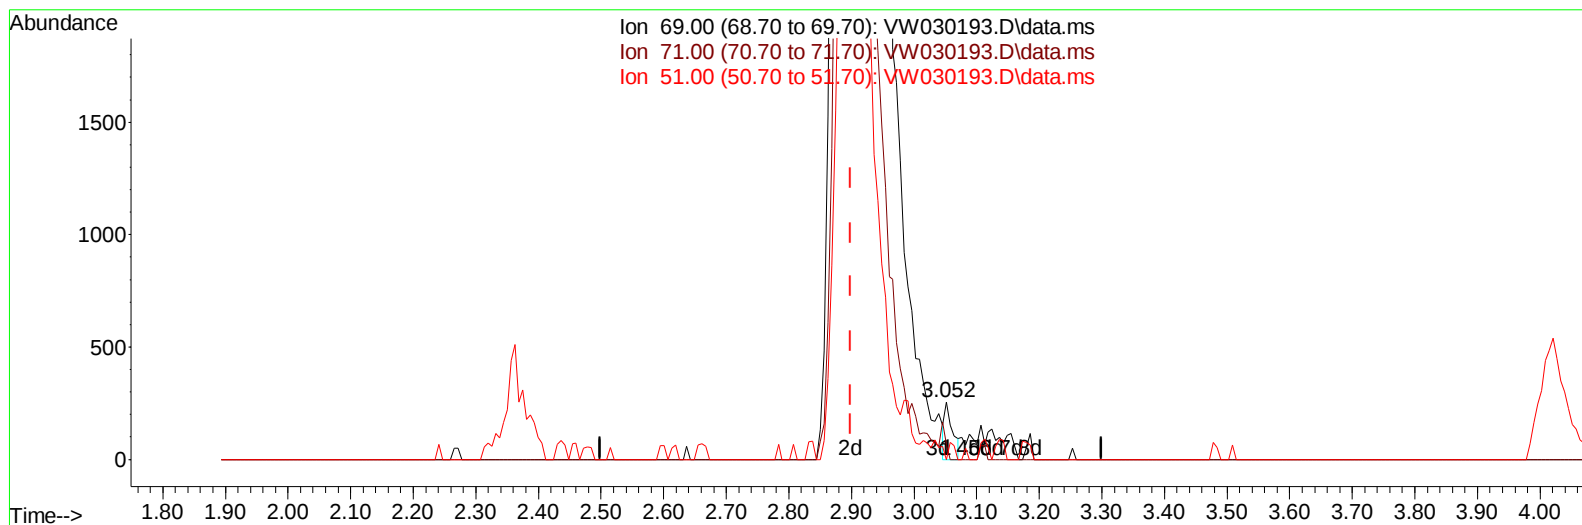

TIC: VW030193.D\data.ms

(7) Chloroethane-d5 (S)

3.052min (+ 0.152) 0.06 ug/L

response 222

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.50	38.29
51.00	25.80	22.52
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
 Data File : VW030193.D
 Acq On : 23 Sep 2024 11:29
 Operator : SY/MD
 Sample : P4109-14 RE
 Misc : 4.95g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4ET6RE

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:31:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 24 01:15:59 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 09/25/2024
 Supervised By :Mahesh Dadoda 09/25/2024

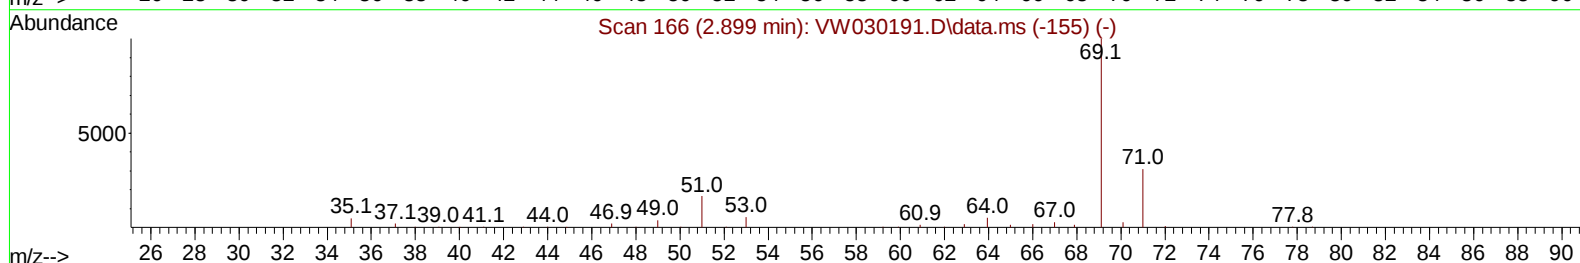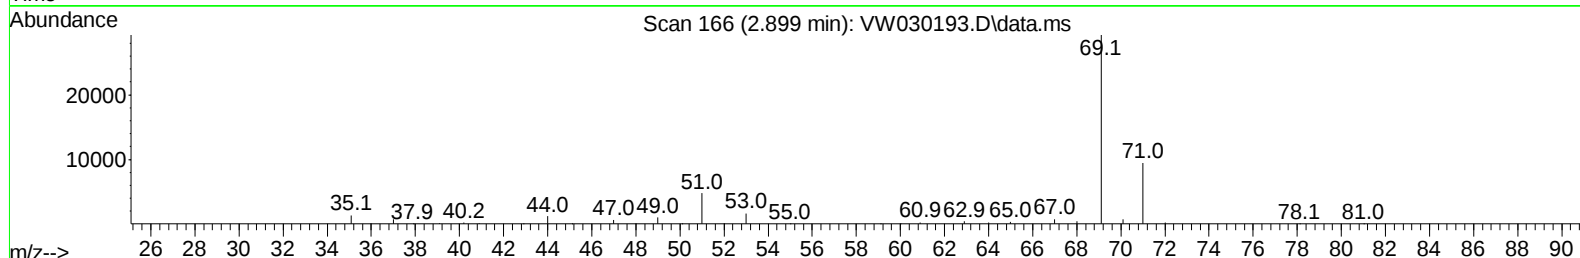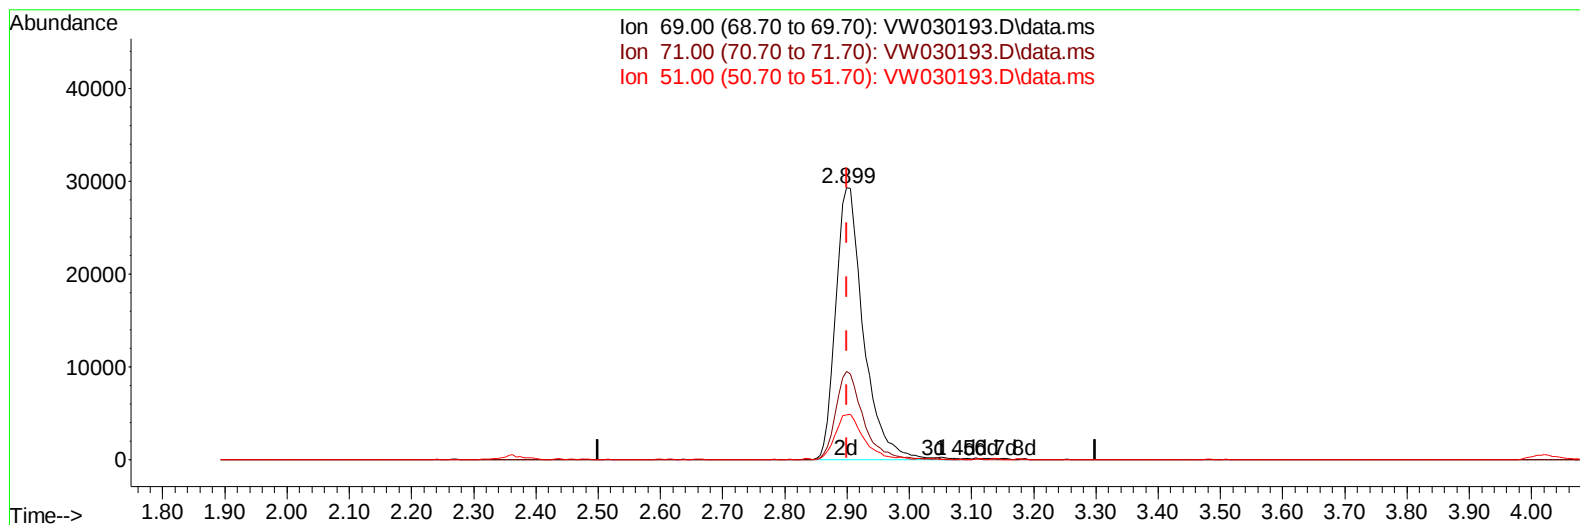

TIC: VW030193.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.000) 23.73 ug/L m

response 90188

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.50	0.09#
51.00	25.80	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
 Data File : VW030193.D
 Acq On : 23 Sep 2024 11:29
 Operator : SY/MD
 Sample : P4109-14 RE
 Misc : 4.95g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4ET6RE

Manual IntegrationsAPPROVED

Quant Time: Sep 24 01:31:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Sep 24 01:15:59 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 09/25/2024
 Supervised By :Mahesh Dadoda 09/25/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	416799	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	229754	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	50670	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	110731	20.572	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	82.280%	
7) Chloroethane-d5	2.899	69	90188m	23.734	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.920%	
11) 1,1-Dichloroethene-d2	4.021	65	46601	17.328	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	69.320%	
21) 2-Butanone-d5	7.075	46	24298	18.643	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	37.280%	
24) Chloroform-d	7.648	84	198975	17.362	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	69.440%	
26) 1,2-Dichloroethane-d4	8.307	65	111334	19.346	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	77.400%	
32) Benzene-d6	8.276	84	380592	28.755	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	115.000%	
36) 1,2-Dichloropropane-d6	9.270	67	114878	28.111	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	112.440%	
41) Toluene-d8	10.325	98	253965	21.411	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	85.640%	
43) trans-1,3-Dichloroprop...	10.575	79	21526	13.148	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	52.600%	
47) 2-Hexanone-d5	10.922	63	15954	25.513	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	51.020%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	54839	18.025	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	72.080%	
66) 1,2-Dichlorobenzene-d4	13.848	152	29490	17.145	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	68.560%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
Data File : VW030193.D
Acq On : 23 Sep 2024 11:29
Operator : SY/MD
Sample : P4109-14 RE
Misc : 4.95g/10mL/MSVOA_W/SOIL/B
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4ET6RE

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 09/25/2024
Supervised By :Mahesh Dadoda 09/25/2024

Quant Time: Sep 24 01:31:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Sep 24 01:15:59 2024
Response via : Initial Calibration

