
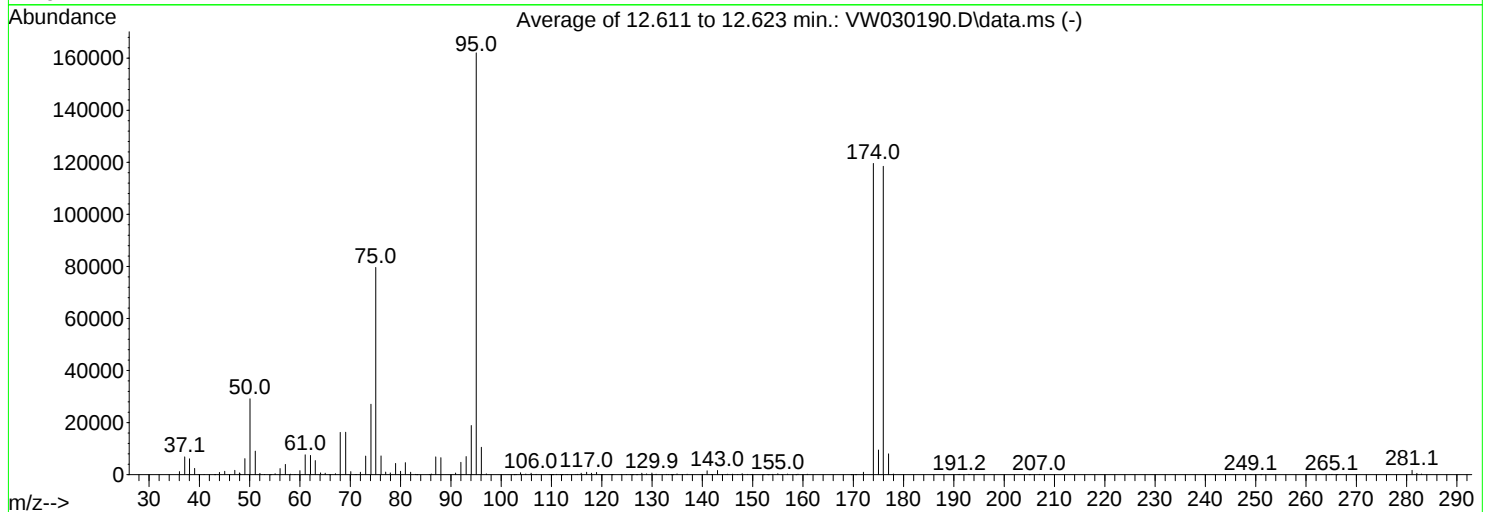


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092324\
Data File : VW030190.D
Acq On : 23 Sep 2024 09:15
Operator : SY/MD
Sample : BFB560
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB560

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Title : SFAM01.0
Last Update : Wed Sep 25 01:17:29 2024

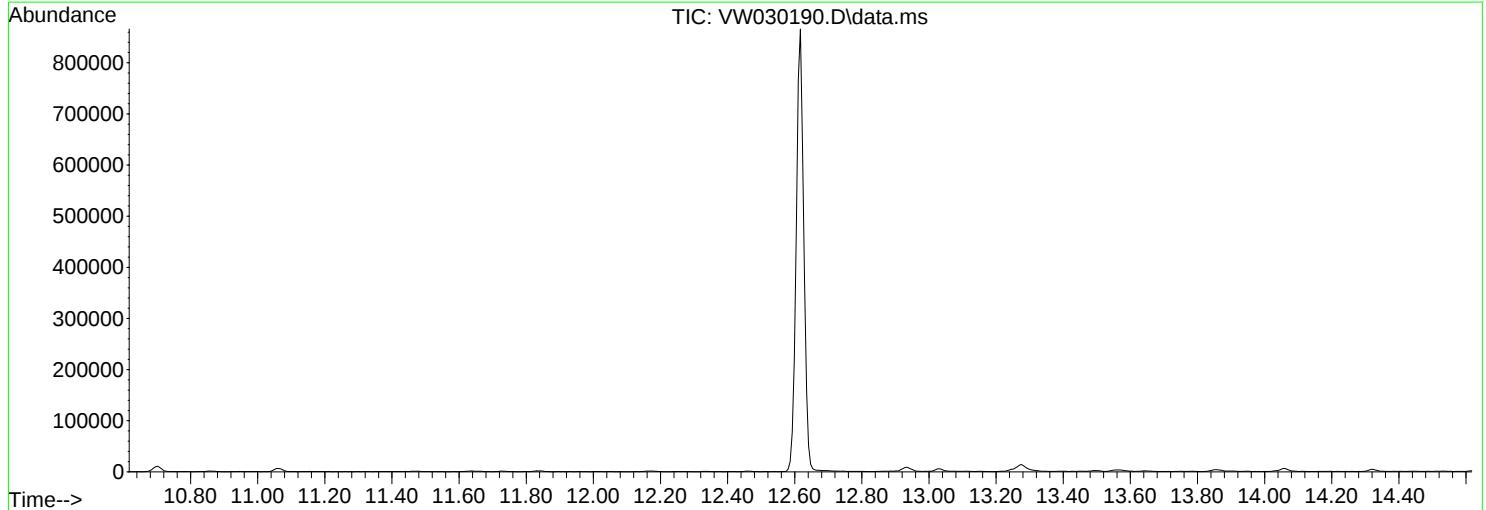

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	29120	PASS
75	95	30	80	49.1	79592	PASS
95	95	100	100	100.0	162069	PASS
96	95	5	9	6.5	10545	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	119568	PASS
175	174	5	9	7.9	9501	PASS
176	174	95	101	99.1	118496	PASS
177	176	5	9	6.7	7997	PASS

m/z	Abundance
38.80	103.0
39.90	247.0
43.00	86.0
43.90	166.0
57.10	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560

m/z	Abundance
36.10	1352.0
37.10	7158.0
38.10	6862.0
39.00	2896.0
40.00	330.0
41.00	73.0
43.10	113.0
44.10	1104.0
45.10	1484.0
46.00	155.0
47.10	1703.0
48.00	1140.0
49.10	6545.0
50.00	30672.0
51.10	9627.0
52.10	455.0
53.00	118.0
54.10	66.0
55.00	475.0
56.10	2671.0
57.10	4327.0
58.10	185.0
59.10	74.0
60.00	1707.0
61.00	7879.0
62.10	8028.0
63.00	5700.0
64.00	772.0
65.00	753.0
65.90	67.0
67.10	372.0
68.00	16848.0
69.10	17136.0
70.10	1287.0
70.90	58.0
72.00	939.0
73.00	7475.0
74.10	28624.0
75.00	84704.0
76.10	7709.0
77.10	1111.0
78.00	662.0
79.00	4547.0
80.00	1355.0
81.00	5021.0
82.00	982.0
83.00	111.0
85.80	227.0
86.20	270.0
87.00	7088.0
88.00	6741.0
90.90	614.0
92.00	4811.0
93.10	7060.0
94.10	18936.0
95.00	165504.0
96.00	10746.0
97.00	315.0
103.00	104.0
103.90	750.0
104.90	329.0
106.00	537.0
106.90	112.0
109.70	119.0
110.20	85.0
111.00	127.0
111.90	126.0
112.90	135.0
114.90	116.0
115.20	117.0
115.90	629.0
117.00	1040.0
117.90	505.0
118.90	891.0
123.80	52.0
125.00	152.0
125.80	66.0
126.90	66.0
127.90	524.0
128.90	394.0
130.00	611.0
130.90	267.0
132.90	326.0
133.80	94.0
134.90	345.0
136.00	71.0
136.90	186.0
139.90	112.0
140.90	1393.0
141.80	134.0
143.00	1553.0
145.10	283.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560

146.00	244.0
147.10	72.0
147.90	351.0
149.00	134.0
149.70	127.0
152.90	125.0
153.90	135.0
155.00	273.0
157.00	223.0
159.00	176.0
160.90	193.0
172.00	1073.0
174.00	114528.0
175.00	8747.0
176.00	109816.0
177.00	8219.0
178.00	272.0
190.80	173.0
191.20	242.0
192.90	219.0
205.00	57.0
207.10	143.0
249.00	141.0
251.00	62.0
264.60	111.0
265.20	218.0
281.10	2636.0
282.10	630.0
283.00	327.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560

m/z	Abundance
36.10	1115.0
37.10	7743.0
38.00	6949.0
39.10	2546.0
40.10	271.0
40.90	79.0
43.10	129.0
44.10	1070.0
45.00	1432.0
46.10	114.0
47.00	1887.0
47.90	956.0
49.00	6969.0
50.00	32496.0
51.10	10314.0
52.00	540.0
53.00	52.0
55.10	353.0
56.00	2518.0
57.10	4240.0
58.10	211.0
58.90	59.0
60.00	1710.0
61.10	8830.0
62.10	8149.0
63.10	6018.0
64.10	826.0
65.00	516.0
67.00	453.0
68.00	18368.0
69.10	18672.0
70.10	1229.0
71.20	140.0
72.00	1091.0
73.00	7951.0
74.10	29928.0
75.10	88840.0
76.10	7995.0
77.00	969.0
78.00	636.0
79.00	4571.0
80.00	1354.0
80.90	4880.0
82.00	1098.0
82.90	97.0
83.10	99.0
86.10	265.0
87.00	7296.0
88.00	7346.0
90.90	761.0
92.00	5242.0
93.00	7793.0
94.00	21160.0
95.00	187264.0
96.10	12441.0
97.00	329.0
102.60	78.0
103.90	880.0
104.90	277.0
105.90	694.0
107.00	176.0
109.90	74.0
111.00	155.0
111.80	87.0
113.10	156.0
114.80	145.0
115.20	129.0
115.90	631.0
117.00	1007.0
117.90	700.0
119.00	1028.0
119.90	53.0
123.80	88.0
124.80	102.0
125.70	67.0
128.00	691.0
128.90	306.0
129.90	793.0
130.70	206.0
132.80	96.0
133.30	80.0
134.10	64.0
135.00	315.0
136.10	51.0
136.90	267.0
140.00	86.0
141.00	1684.0
142.00	212.0
143.00	1913.0
143.90	103.0
144.90	291.0
146.00	242.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560

147.00	76.0
147.90	484.0
149.00	150.0
149.90	200.0
152.10	51.0
152.90	135.0
153.90	139.0
155.00	472.0
155.80	87.0
157.00	345.0
158.60	96.0
159.10	163.0
160.80	167.0
169.60	58.0
170.40	55.0
172.00	1098.0
174.00	134080.0
175.00	10633.0
175.90	144128.0
177.00	9465.0
177.90	280.0
191.00	113.0
193.10	208.0
206.90	146.0
249.10	104.0
264.70	75.0
265.10	101.0
266.10	92.0
281.10	1720.0
282.00	539.0
282.90	280.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560

m/z	Abundance
36.00	1017.0
37.10	5640.0
38.00	4496.0
39.10	1719.0
40.00	277.0
43.10	130.0
44.00	865.0
45.00	1065.0
47.10	1375.0
48.20	785.0
49.10	5008.0
50.10	24192.0
51.10	7106.0
52.10	424.0
52.90	62.0
55.10	282.0
56.00	1805.0
57.10	3431.0
58.00	111.0
60.00	1174.0
61.10	6095.0
62.10	6013.0
63.10	4602.0
64.20	453.0
65.00	484.0
67.10	256.0
68.00	13516.0
69.10	13030.0
70.10	964.0
71.00	65.0
72.00	666.0
73.10	5944.0
74.10	22632.0
75.10	65232.0
76.10	5984.0
77.00	892.0
77.90	690.0
79.00	3859.0
80.00	1104.0
81.00	3876.0
82.00	697.0
83.20	109.0
86.00	183.0
87.00	6058.0
88.00	5459.0
91.00	485.0
92.00	4197.0
93.00	5911.0
94.00	16520.0
95.10	133440.0
96.10	8447.0
97.10	254.0
103.10	70.0
103.80	594.0
104.80	158.0
106.00	509.0
106.90	141.0
109.90	76.0
111.00	111.0
112.10	82.0
113.20	74.0
115.10	144.0
115.90	355.0
117.00	757.0
118.00	406.0
119.00	756.0
122.00	58.0
123.90	63.0
126.10	70.0
127.90	522.0
128.90	227.0
130.00	480.0
130.80	190.0
133.20	73.0
134.90	212.0
137.00	184.0
140.10	124.0
141.00	1394.0
143.00	1402.0
144.00	95.0
144.70	131.0
145.90	150.0
146.90	92.0
147.90	323.0
149.00	102.0
150.00	182.0
152.10	62.0
153.10	89.0
153.90	129.0
155.00	342.0
155.80	82.0
156.90	247.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560

158.90	192.0
160.80	177.0
170.50	56.0
172.00	619.0
174.00	110096.0
175.00	9123.0
176.00	101544.0
177.00	6308.0
177.90	222.0
190.90	72.0
192.90	75.0
207.10	70.0
281.00	710.0
282.20	228.0
283.00	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB560