

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
 Data File : VW030218.D
 Acq On : 24 Sep 2024 12:28
 Operator : SY/MD
 Sample : P4131-07
 Misc : 5.34g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 25 01:19:45 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 25 01:17:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	290303	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	266132	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	126347	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	99352	26.501	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	106.000%
7) Chloroethane-d5	2.905	69	82805	31.286	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	125.160%
11) 1,1-Dichloroethene-d2	4.027	65	39541	21.109	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	84.440%
21) 2-Butanone-d5	7.088	46	41585	45.809	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.620%
24) Chloroform-d	7.648	84	191453	23.985	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.960%
26) 1,2-Dichloroethane-d4	8.392	65	134	0.033	ug/L	0.09
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.276	84	369801	24.120	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.480%
36) 1,2-Dichloropropane-d6	9.276	67	110934	23.435	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.760%
41) Toluene-d8	10.319	98	339865	24.737	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.960%
43) trans-1,3-Dichloroprop...	10.575	79	43126	22.740	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.960%
47) 2-Hexanone-d5	10.922	63	34250	47.284	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.560%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	82951	23.538	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.160%
66) 1,2-Dichlorobenzene-d4	13.849	152	110844	25.844	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	3679	0.570	ug/L #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
Data File : VW030218.D
Acq On : 24 Sep 2024 12:28
Operator : SY/MD
Sample : P4131-07
Misc : 5.34g/10mL/MSVOA_W/SOIL/B
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 25 01:19:45 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 25 01:17:29 2024
Response via : Initial Calibration

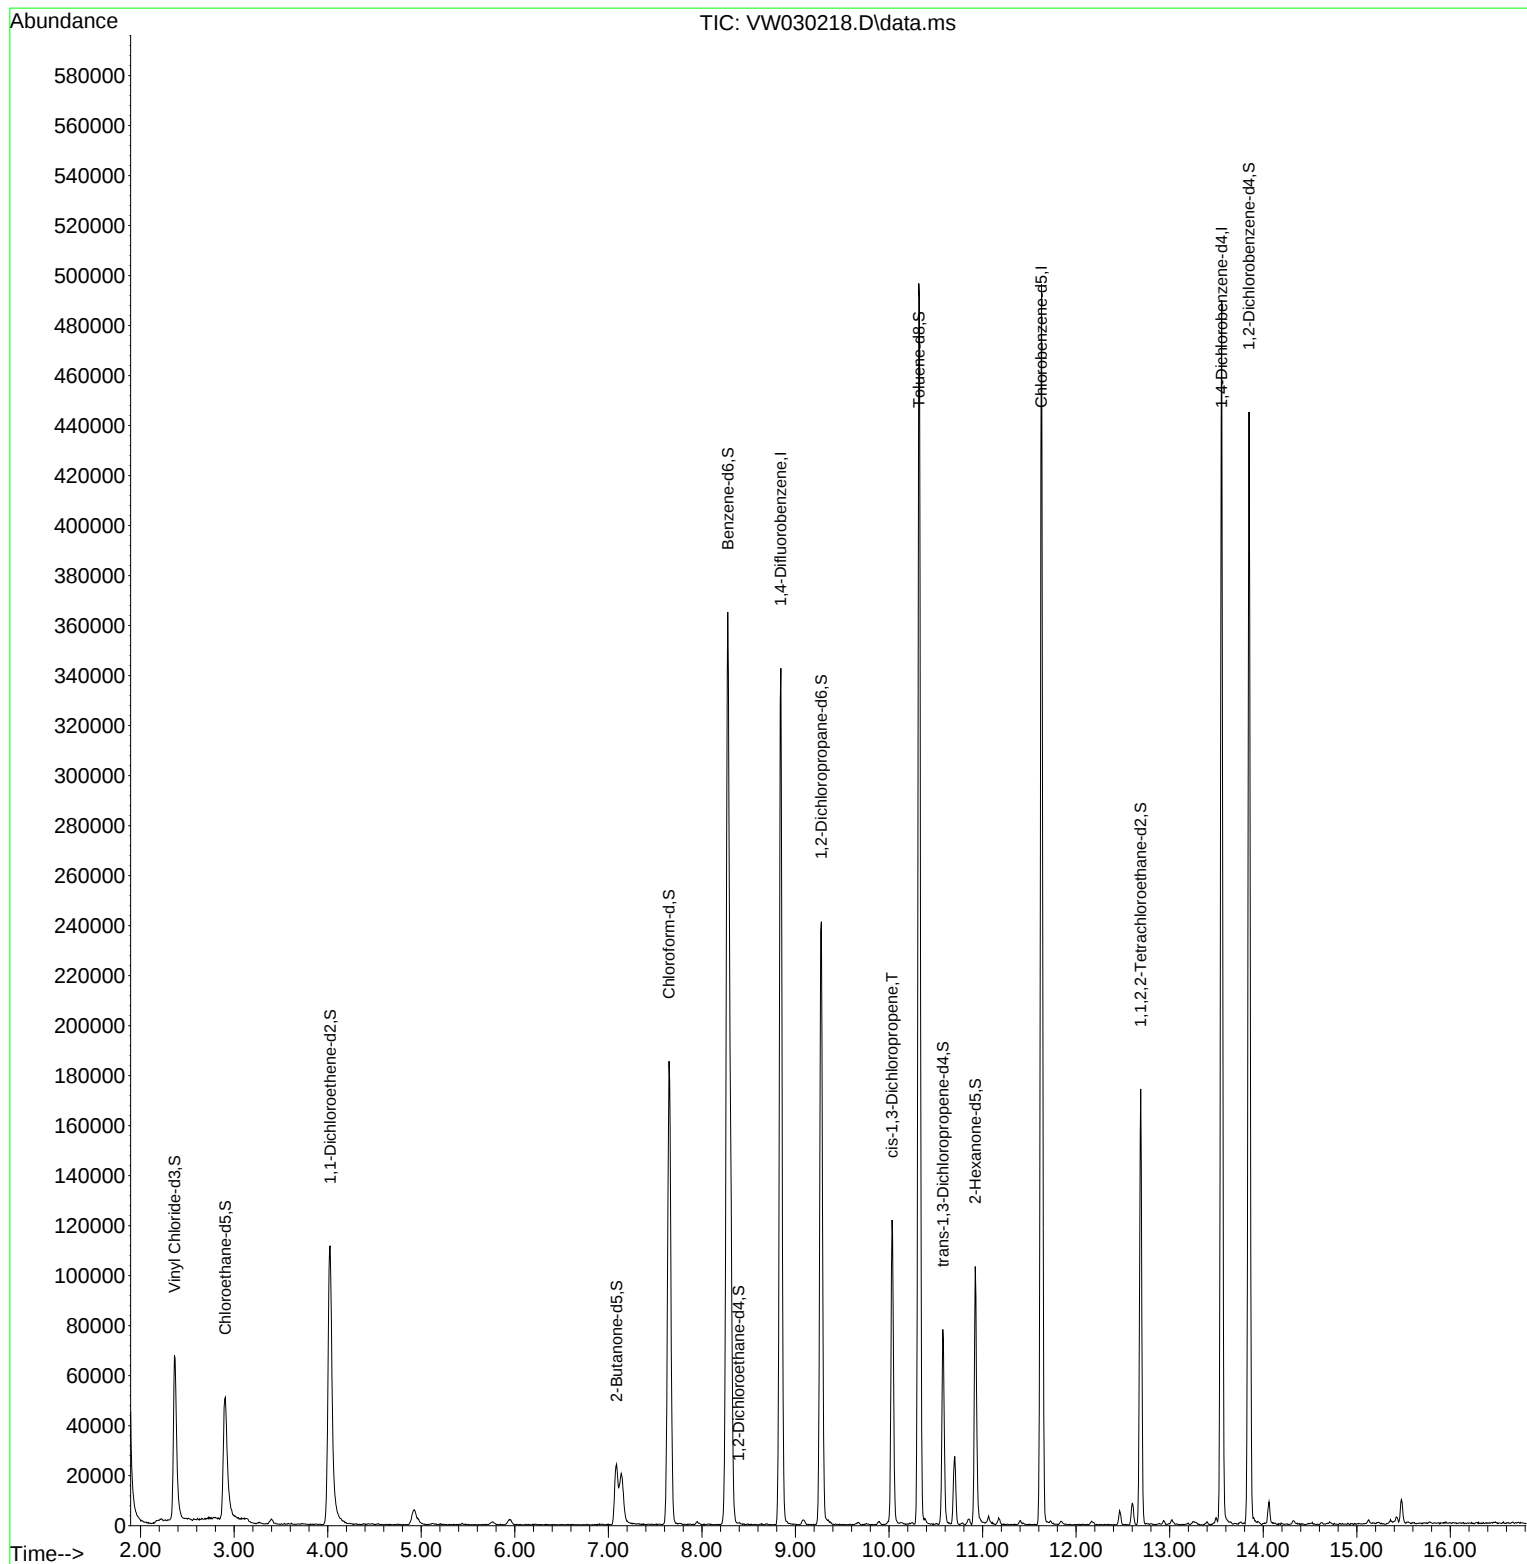

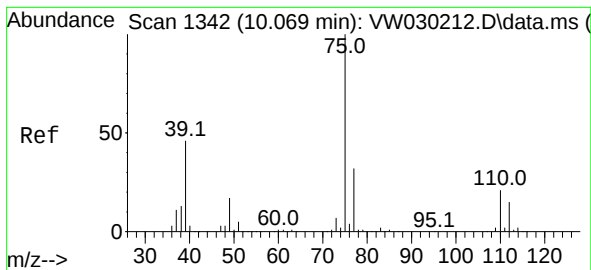

#39

cis-1,3-Dichloropropene

Concen: 0.570 ug/L

RT: 10.032 min Scan# 14

Delta R.T. -0.036 min


Lab File: VW030218.D

Acq: 24 Sep 2024 12:28

Instrument :

MSVOA_W

ClientSampleId :

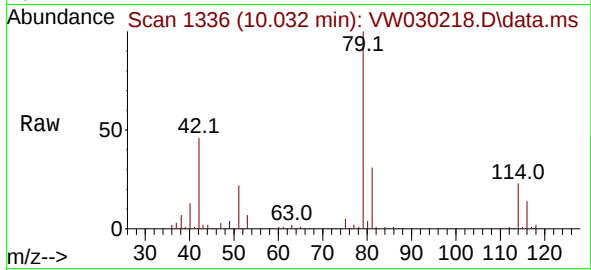

Tgt Ion: 75 Resp: 3679

Ion Ratio Lower Upper

75 100

77 46.8 20.7 38.5#

