

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
 Data File : VW030219.D
 Acq On : 24 Sep 2024 12:51
 Operator : SY/MD
 Sample : P4131-08
 Misc : 4.49g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 25 01:20:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 25 01:17:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	316768	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	292722	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	135811	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	90216	22.054	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.200%
7) Chloroethane-d5	2.899	69	75875	26.272	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.080%
11) 1,1-Dichloroethene-d2	4.021	65	35636	17.435	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.720%
21) 2-Butanone-d5	7.081	46	38652	39.021	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.040%
24) Chloroform-d	7.648	84	177312	20.358	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.440%
26) 1,2-Dichloroethane-d4	8.307	65	94546	21.617	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	86.480%
32) Benzene-d6	8.276	84	340186	20.173	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.680%
36) 1,2-Dichloropropane-d6	9.270	67	103909	19.957	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.840%
41) Toluene-d8	10.325	98	316517	20.945	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	83.760%
43) trans-1,3-Dichloroprop...	10.575	79	40961	19.637	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.560%
47) 2-Hexanone-d5	10.922	63	31490	39.525	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	79.040%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	78542	20.262	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.040%
66) 1,2-Dichlorobenzene-d4	13.848	152	104425	22.650	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.600%
Target Compounds						
39) cis-1,3-Dichloropropene	10.038	75	2942	0.415	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
Data File : VW030219.D
Acq On : 24 Sep 2024 12:51
Operator : SY/MD
Sample : P4131-08
Misc : 4.49g/10mL/MSVOA_W/SOIL/B
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 25 01:20:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 25 01:17:29 2024
Response via : Initial Calibration

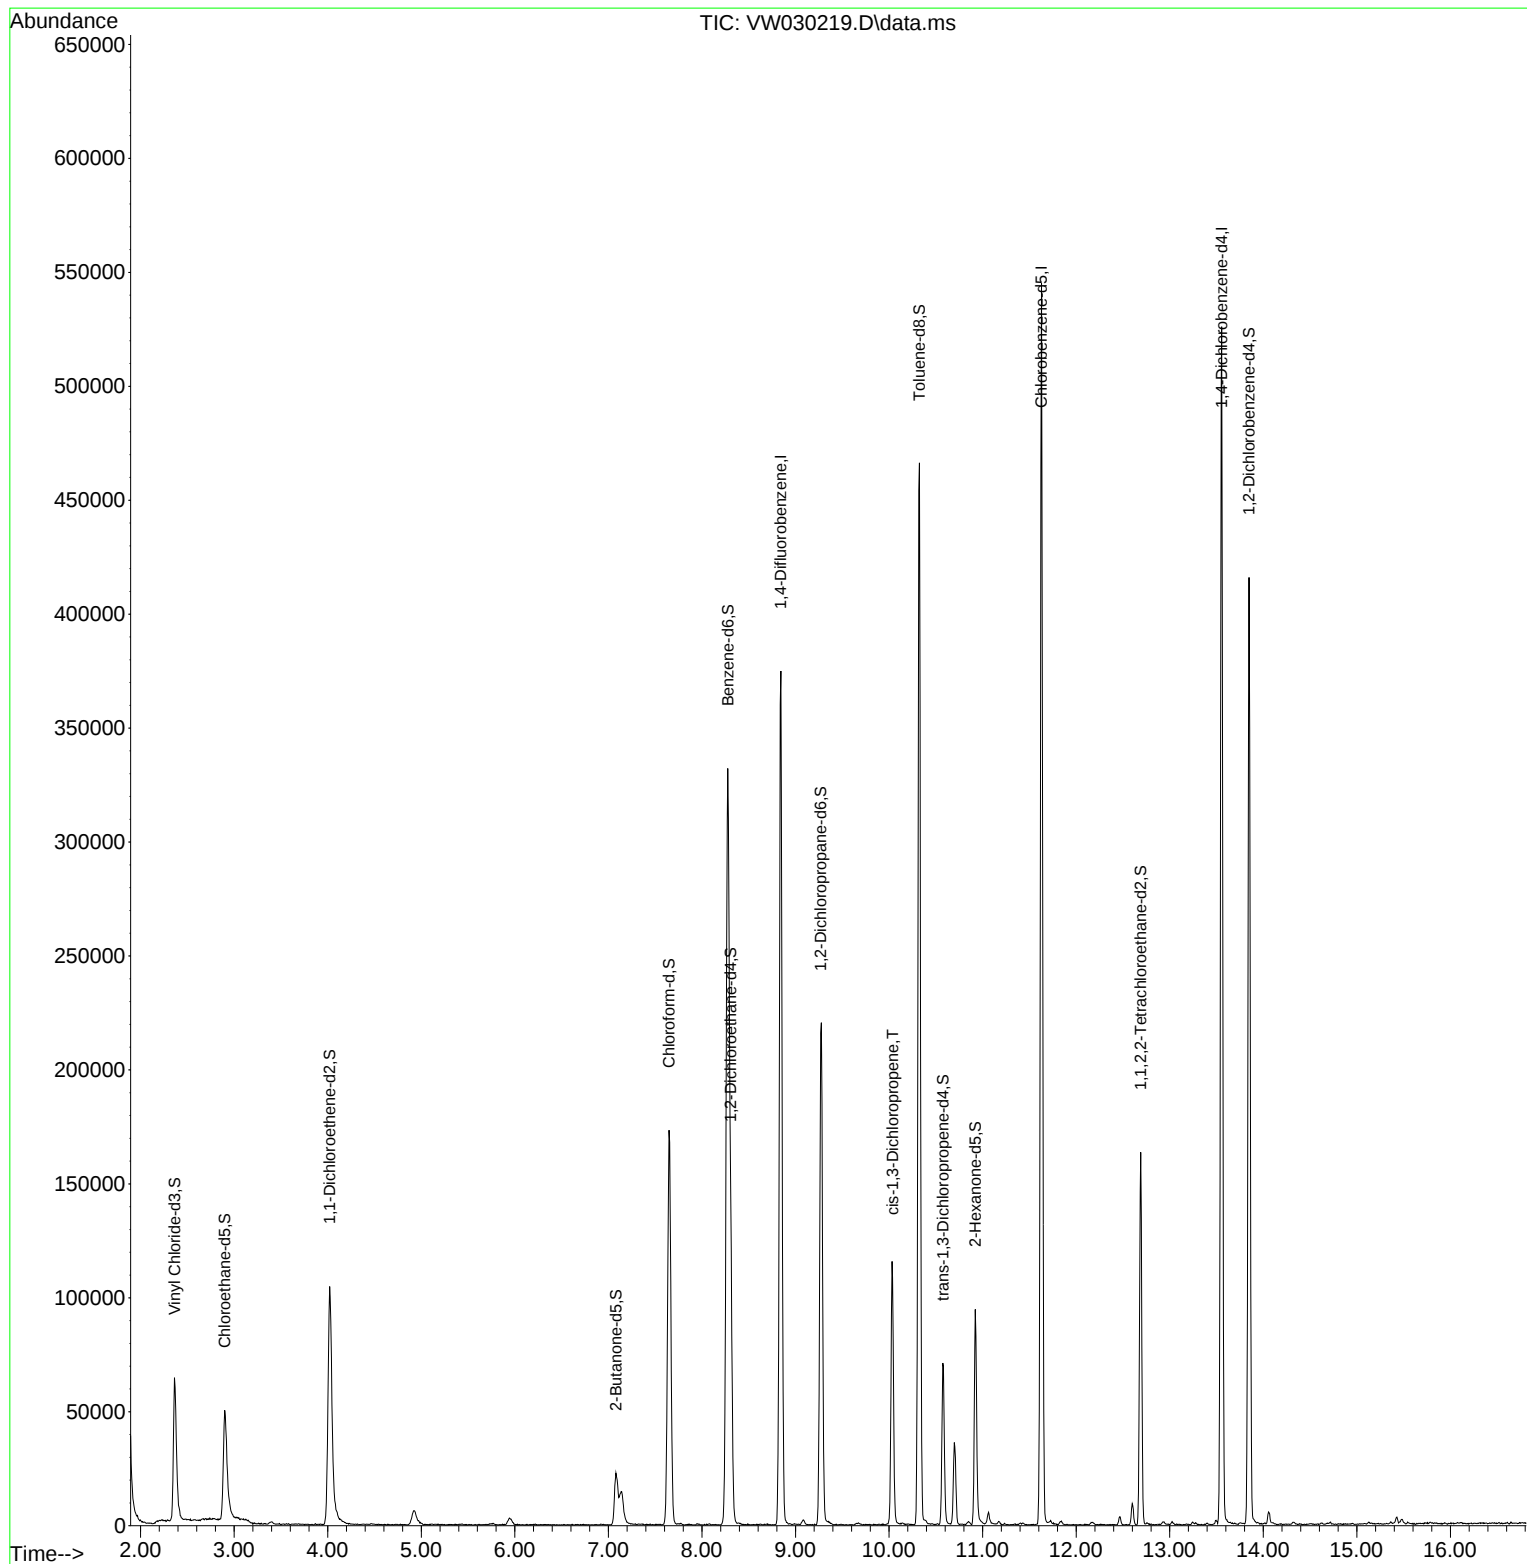

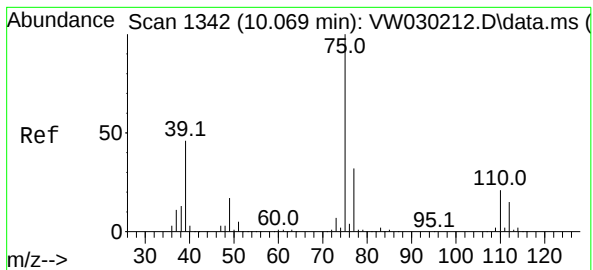

#39
 cis-1,3-Dichloropropene
 Concen: 0.415 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.030 min
 Lab File: VW030219.D
 Acq: 24 Sep 2024 12:51

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2942
 Ion Ratio Lower Upper
 75 100
 77 38.0 20.7 38.5

