

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
 Data File : VW030221.D
 Acq On : 24 Sep 2024 13:39
 Operator : SY/MD
 Sample : P4131-11
 Misc : 5.13g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 25 01:20:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 25 01:17:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	298061	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	281727	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	129587	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	87138	22.638	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.560%
7) Chloroethane-d5	2.905	69	73736	27.134	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.520%
11) 1,1-Dichloroethene-d2	4.027	65	36279	18.863	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.440%
21) 2-Butanone-d5	7.081	46	39528	42.410	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.820%
24) Chloroform-d	7.654	84	173146	21.127	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.520%
26) 1,2-Dichloroethane-d4	8.307	65	94023	22.846	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.400%
32) Benzene-d6	8.276	84	334536	20.612	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.440%
36) 1,2-Dichloropropane-d6	9.276	67	103494	20.653	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.600%
41) Toluene-d8	10.325	98	310047	21.317	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.280%
43) trans-1,3-Dichloroprop...	10.575	79	39669	19.759	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.040%
47) 2-Hexanone-d5	10.922	63	32615	42.534	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.060%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	78984	21.171	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.680%
66) 1,2-Dichlorobenzene-d4	13.848	152	103393	23.504	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.000%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	3137	0.459	ug/L	Qvalue # 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
Data File : VW030221.D
Acq On : 24 Sep 2024 13:39
Operator : SY/MD
Sample : P4131-11
Misc : 5.13g/10mL/MSVOA_W/SOIL/B
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 25 01:20:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 25 01:17:29 2024
Response via : Initial Calibration

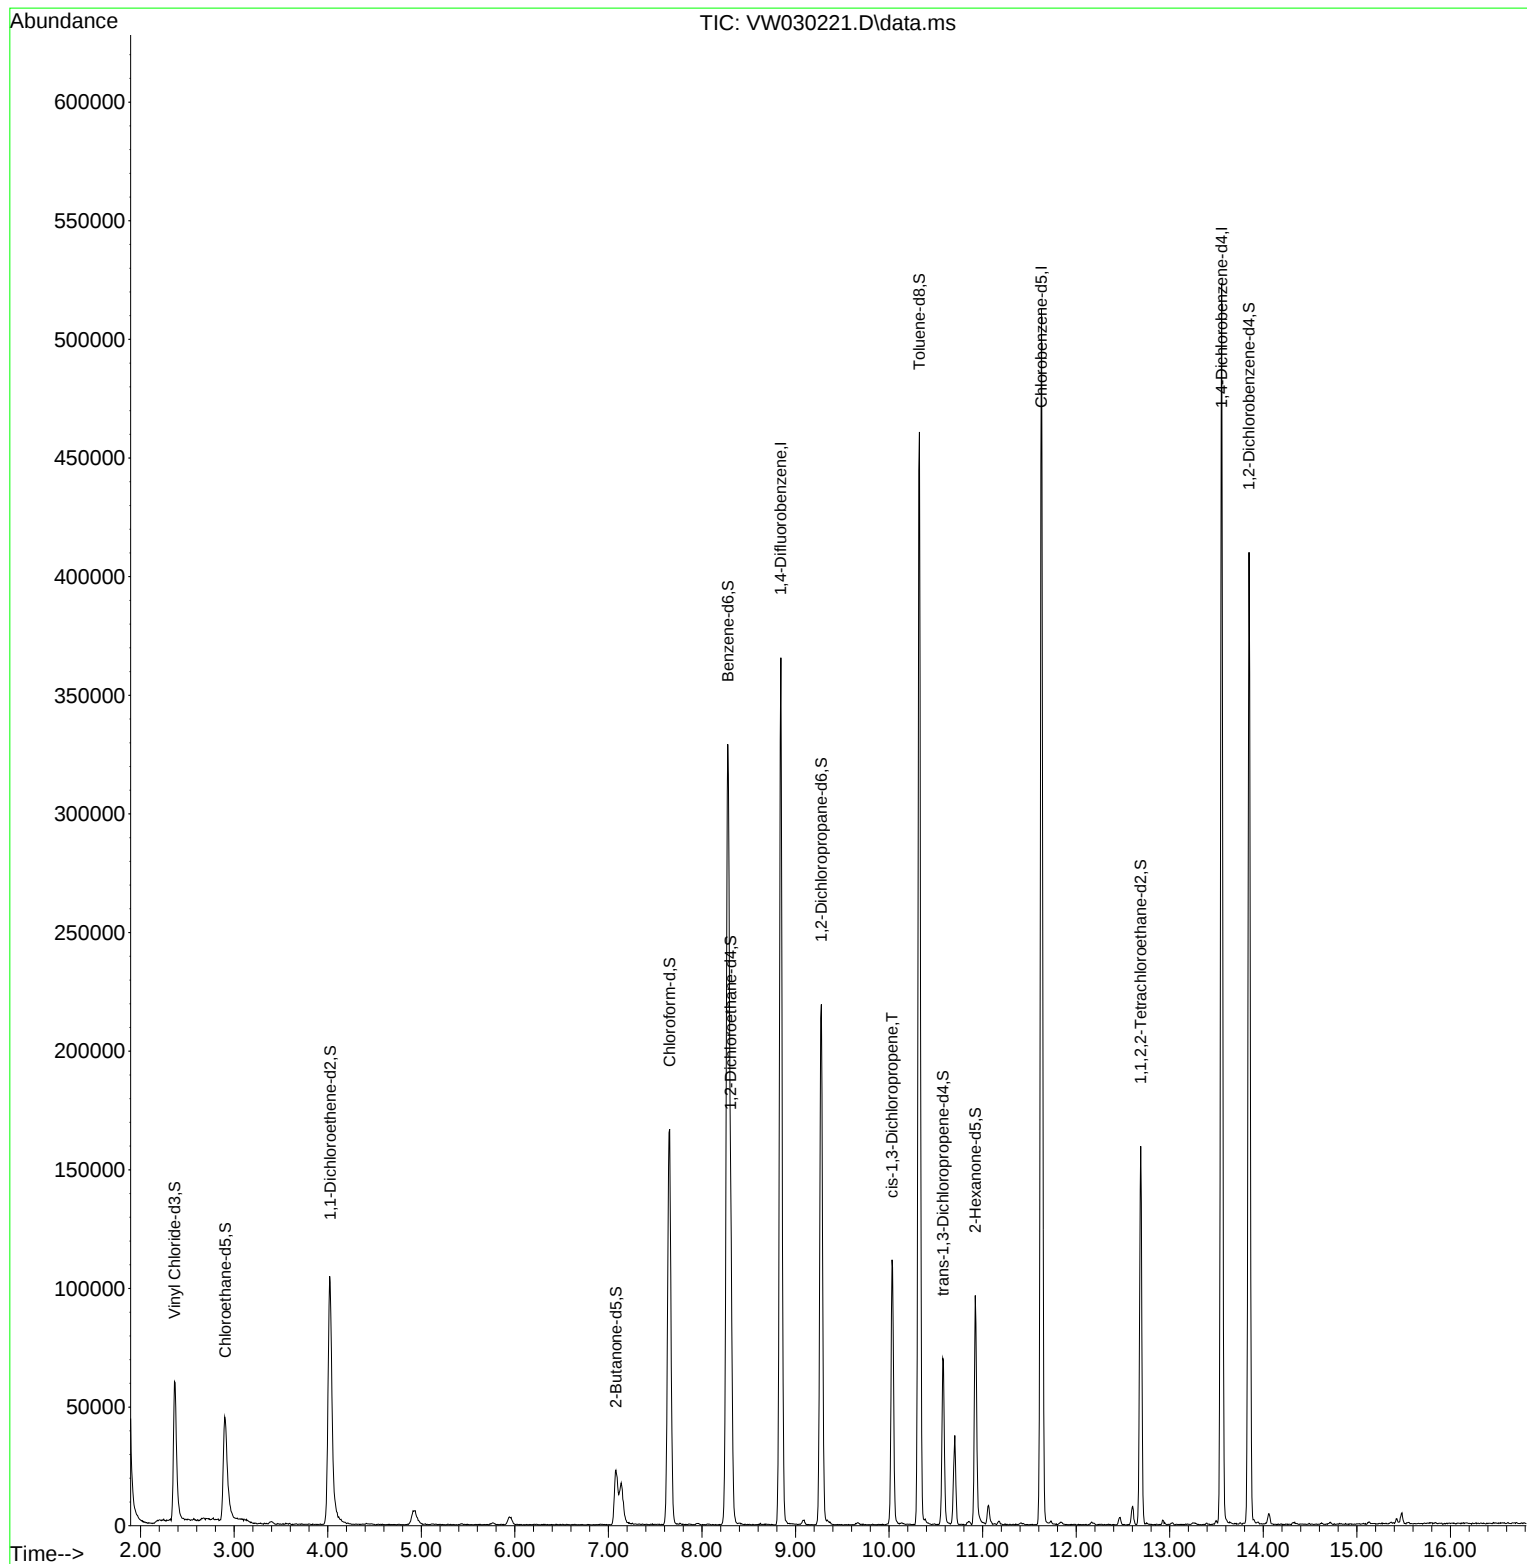

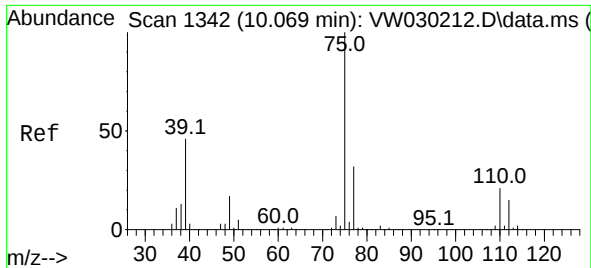

#39
cis-1,3-Dichloropropene
Concen: 0.459 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.037 min
Lab File: VW030221.D
Acq: 24 Sep 2024 13:39

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 3137
Ion Ratio Lower Upper
75 100
77 48.7 20.7 38.5#

