

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
 Data File : VW030222.D
 Acq On : 24 Sep 2024 14:27
 Operator : SY/MD
 Sample : P4131-10
 Misc : 6.61g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 25 01:20:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 25 01:17:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	268528	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	251568	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114812	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	82670	23.839	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.360%
7) Chloroethane-d5	2.905	69	71361	29.148	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.600%
11) 1,1-Dichloroethene-d2	4.027	65	34732	20.045	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.200%
21) 2-Butanone-d5	7.075	46	42961	51.163	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.320%
24) Chloroform-d	7.654	84	167970	22.750	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.000%
26) 1,2-Dichloroethane-d4	8.307	65	91569	24.697	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.800%
32) Benzene-d6	8.276	84	328748	22.684	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.720%
36) 1,2-Dichloropropane-d6	9.276	67	98394	21.990	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.960%
41) Toluene-d8	10.325	98	294585	22.682	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.720%
43) trans-1,3-Dichloroprop...	10.575	79	37906	21.145	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.560%
47) 2-Hexanone-d5	10.922	63	33324	48.669	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.340%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	79366	23.824	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	99890	25.629	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.520%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	2943	0.483	ug/L	Qvalue # 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092424\
Data File : VW030222.D
Acq On : 24 Sep 2024 14:27
Operator : SY/MD
Sample : P4131-10
Misc : 6.61g/10mL/MSVOA_W/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Sep 25 01:20:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 25 01:17:29 2024
Response via : Initial Calibration

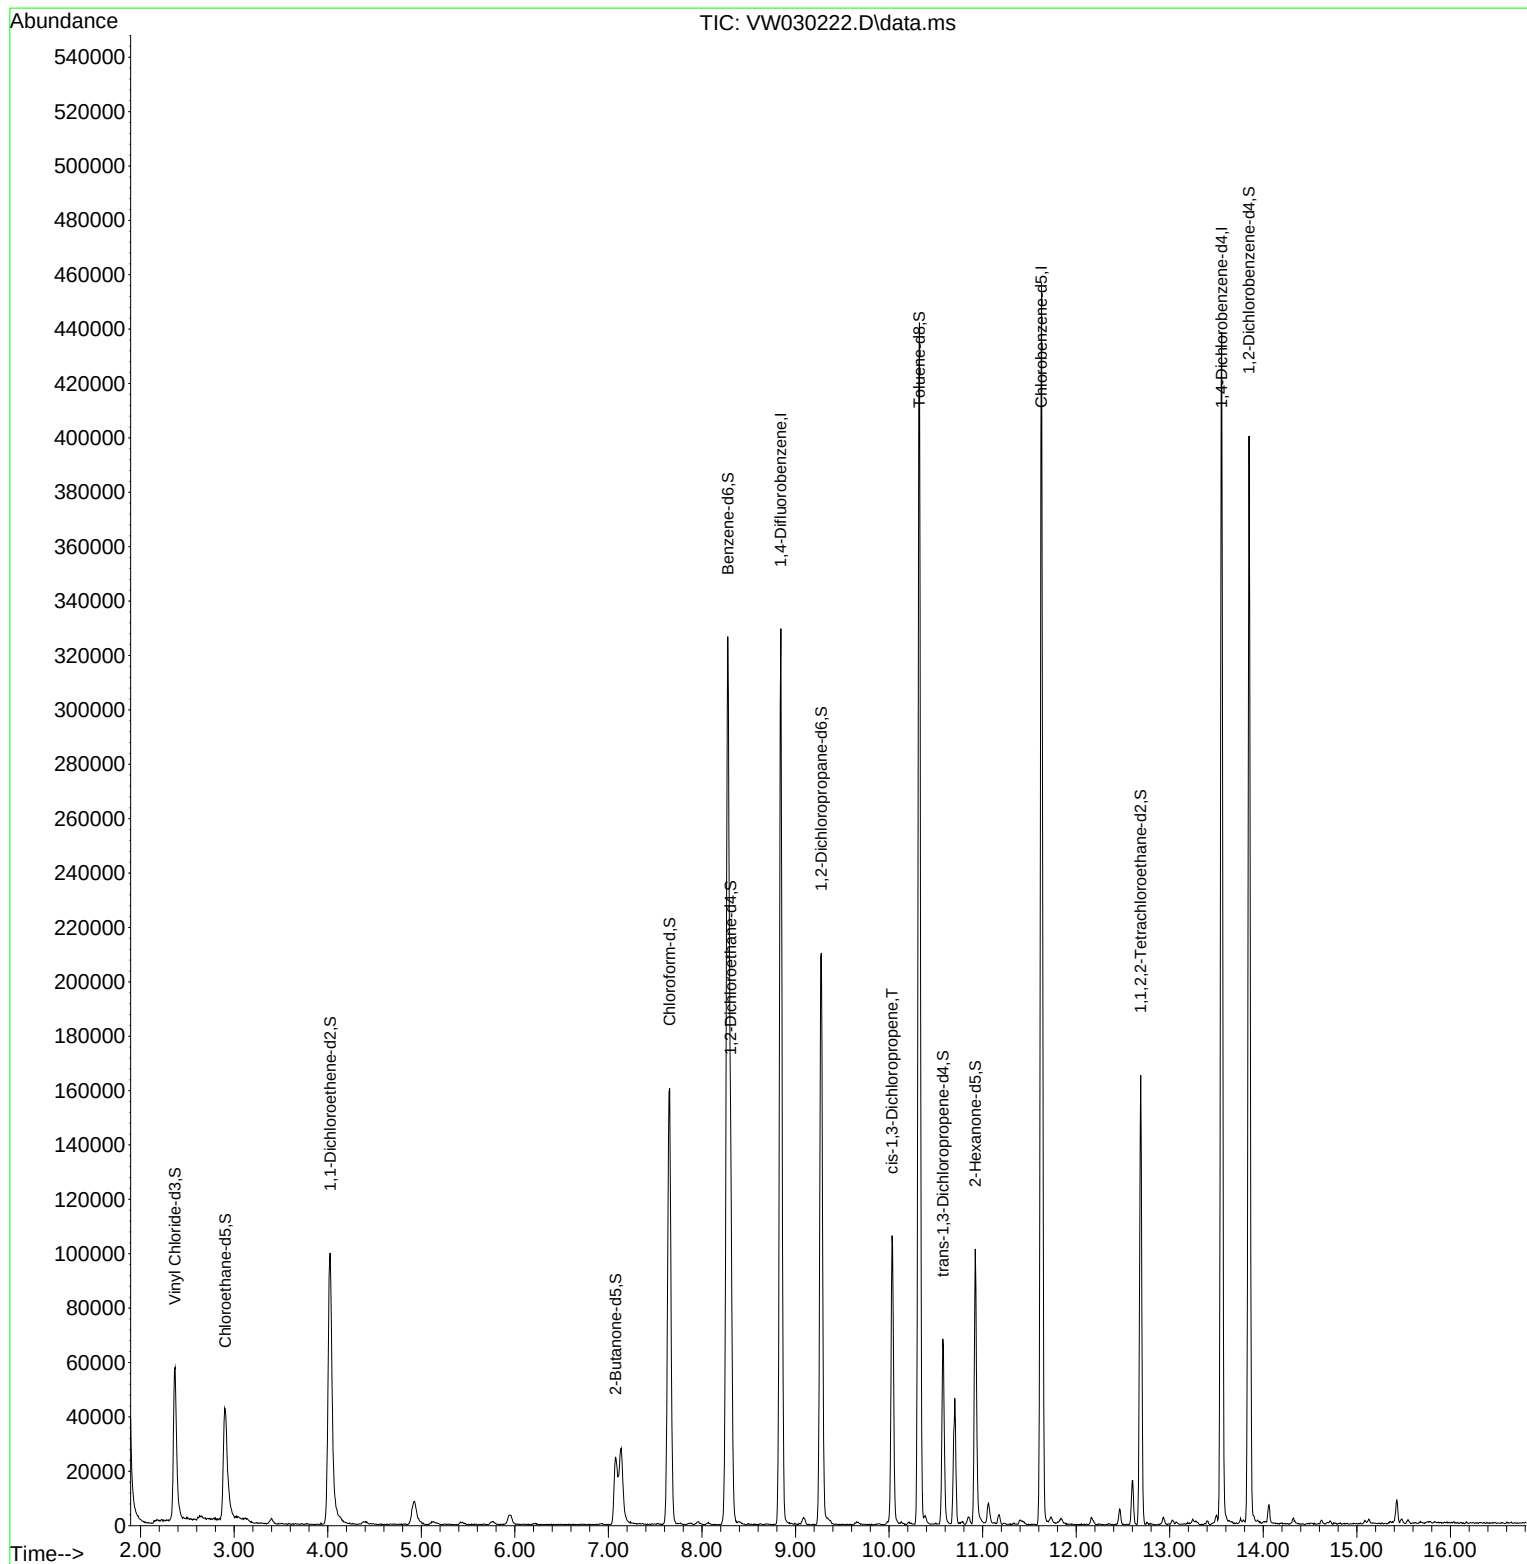

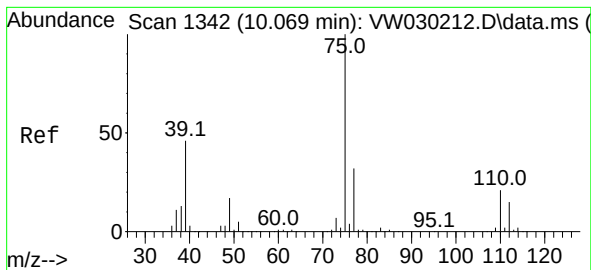

#39
cis-1,3-Dichloropropene
Concen: 0.483 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.036 min
Lab File: VW030222.D
Acq: 24 Sep 2024 14:27

Instrument :
MSVOA_W
ClientSampleId :

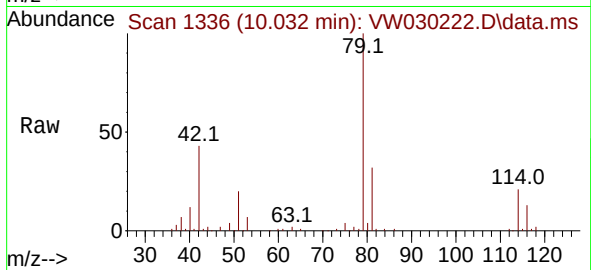

Tgt Ion: 75 Resp: 2943
Ion Ratio Lower Upper
75 100
77 44.7 20.7 38.5#

