
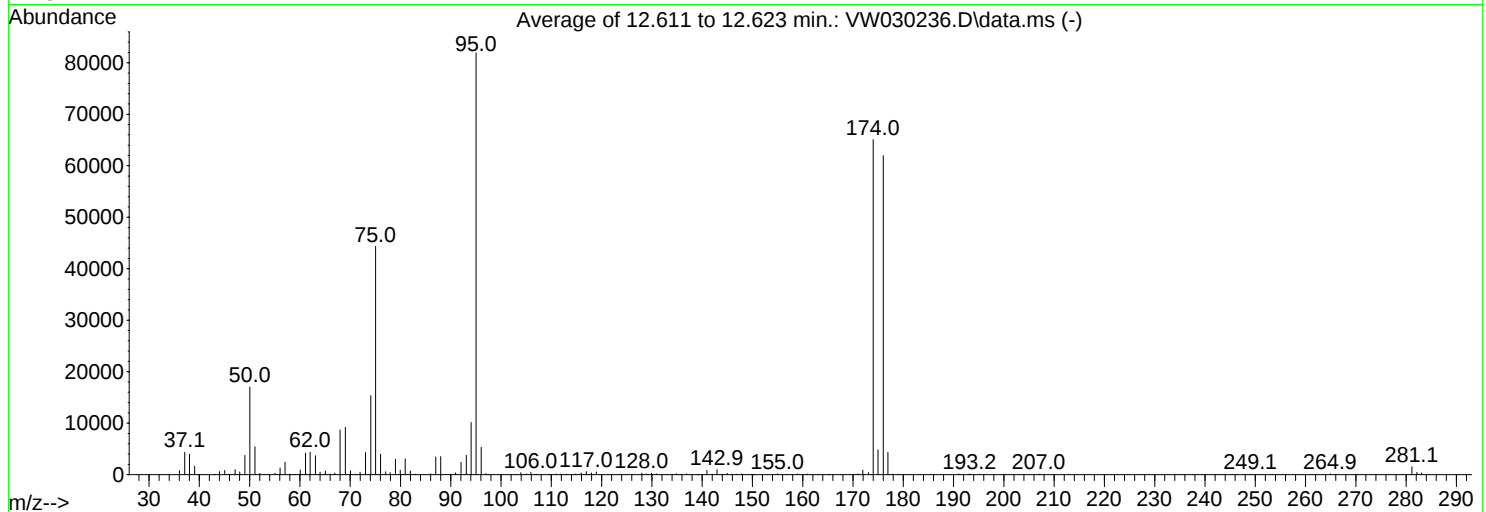


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092524\
Data File : VW030236.D
Acq On : 25 Sep 2024 09:13
Operator : SY/MD
Sample : BFB562
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB562

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM091624SMA.M
Title : SFAM01.0
Last Update : Thu Sep 26 01:18:41 2024

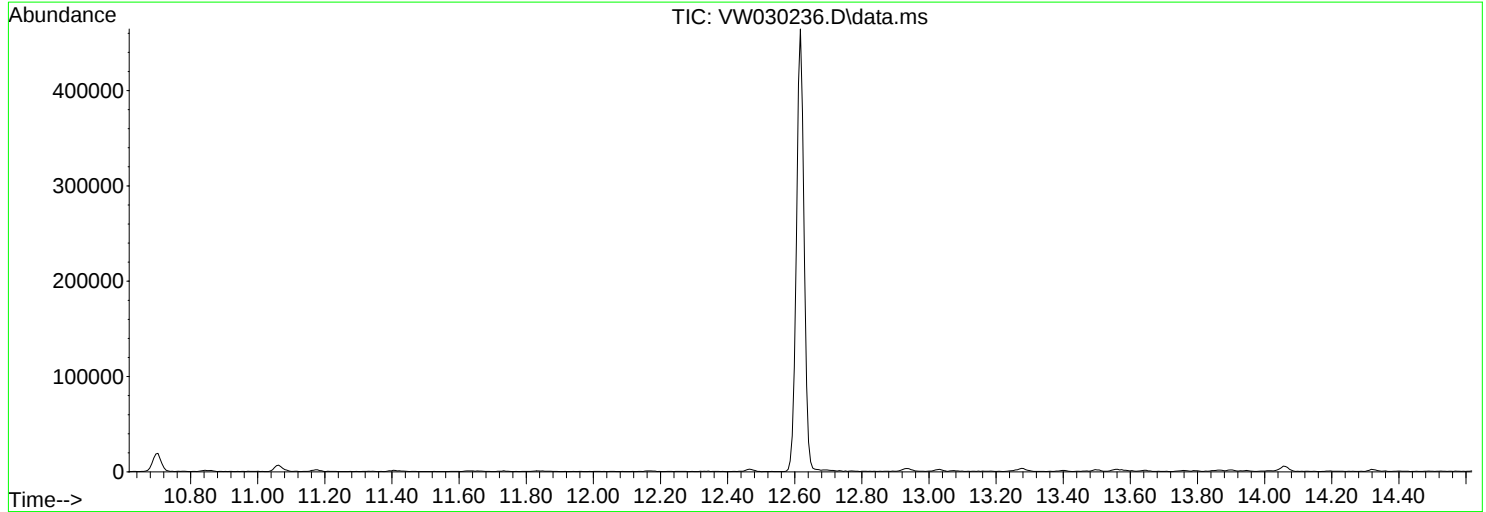

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	16997	PASS
75	95	30	80	54.1	44344	PASS
95	95	100	100	100.0	81933	PASS
96	95	5	9	6.5	5310	PASS
173	174	0.00	2	0.6	414	PASS
174	95	50	120	79.4	65088	PASS
175	174	5	9	7.4	4834	PASS
176	174	95	101	95.2	61987	PASS
177	176	5	9	7.0	4319	PASS

m/z	Abundance
39.90	193.0
43.90	170.0
55.30	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562

m/z	Abundance
36.10	798.0
37.10	4517.0
38.00	4124.0
39.10	1912.0
40.20	244.0
41.10	62.0
44.00	710.0
45.10	851.0
45.90	135.0
47.00	1048.0
48.00	454.0
49.00	3724.0
50.00	17424.0
51.00	5407.0
52.10	304.0
53.10	125.0
55.00	215.0
56.10	1342.0
57.10	2492.0
58.00	225.0
58.90	80.0
59.10	79.0
60.00	891.0
61.10	4152.0
62.00	4612.0
63.10	3936.0
64.00	700.0
65.10	861.0
66.10	112.0
67.00	373.0
68.00	8845.0
69.10	9048.0
70.00	873.0
71.00	63.0
71.90	519.0
73.00	4388.0
74.10	15888.0
75.10	43144.0
76.10	4036.0
77.10	597.0
77.90	386.0
79.00	2987.0
80.00	923.0
81.00	3243.0
81.90	721.0
83.10	105.0
86.00	223.0
87.00	3307.0
88.00	3564.0
91.00	298.0
92.10	2426.0
93.10	3615.0
94.10	10436.0
95.00	82584.0
96.00	5163.0
97.00	227.0
102.90	96.0
104.00	373.0
105.00	169.0
105.90	381.0
106.70	117.0
110.90	92.0
111.80	59.0
113.00	80.0
115.00	115.0
116.00	368.0
116.90	590.0
117.90	338.0
118.90	520.0
125.00	75.0
126.10	75.0
128.00	311.0
129.00	146.0
130.00	298.0
130.90	228.0
133.10	208.0
133.90	62.0
134.90	162.0
136.90	147.0
140.00	67.0
140.90	791.0
141.90	100.0
143.00	929.0
144.00	61.0
145.00	303.0
146.00	138.0
146.80	95.0
147.80	191.0
149.00	83.0
150.00	51.0
152.90	55.0
155.10	149.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562

156.80	109.0
158.90	119.0
161.00	156.0
163.00	57.0
170.30	89.0
170.90	177.0
172.00	922.0
174.00	59536.0
174.90	4292.0
176.00	54576.0
177.00	3942.0
177.90	130.0
178.90	90.0
191.10	207.0
193.20	283.0
193.90	82.0
207.00	126.0
249.10	173.0
251.20	124.0
265.00	302.0
279.10	78.0
281.20	2533.0
282.20	779.0
283.00	458.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562

m/z	Abundance
36.10	825.0
37.10	5033.0
38.10	4378.0
39.00	1791.0
40.00	285.0
43.00	57.0
44.00	864.0
45.00	885.0
45.90	174.0
47.10	1129.0
48.00	681.0
49.10	4329.0
50.10	19064.0
51.10	5758.0
52.00	243.0
53.00	112.0
53.90	79.0
55.00	391.0
56.10	1394.0
57.00	2681.0
58.00	110.0
60.10	1124.0
61.10	4602.0
62.10	4881.0
63.10	4109.0
64.00	491.0
65.00	795.0
66.00	147.0
66.90	285.0
68.00	9690.0
69.00	10321.0
70.10	874.0
71.00	72.0
72.00	640.0
73.00	5097.0
74.10	17328.0
75.10	49816.0
76.10	4571.0
77.00	645.0
78.00	474.0
79.00	3428.0
80.00	966.0
81.00	3422.0
81.90	760.0
83.00	75.0
85.90	175.0
87.00	3831.0
88.00	3919.0
90.90	444.0
92.00	2576.0
93.10	4205.0
94.00	11165.0
95.00	90384.0
96.10	6237.0
97.00	215.0
102.80	54.0
103.90	411.0
105.10	159.0
106.00	474.0
106.70	120.0
107.00	104.0
109.70	60.0
111.00	149.0
111.90	119.0
113.10	98.0
114.80	125.0
116.00	360.0
117.00	698.0
117.90	364.0
118.90	598.0
123.90	79.0
124.80	50.0
125.90	66.0
127.90	377.0
128.90	192.0
129.90	310.0
130.90	158.0
132.80	82.0
134.90	184.0
135.80	62.0
137.00	183.0
141.00	931.0
142.00	120.0
143.00	1024.0
143.90	124.0
145.00	286.0
145.90	172.0
146.90	103.0
147.90	247.0
149.00	75.0
149.90	102.0
152.90	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562

155.00	228.0
156.80	111.0
158.90	127.0
160.80	69.0
165.10	51.0
171.00	125.0
171.90	1042.0
173.10	1242.0
174.00	72392.0
175.00	5222.0
176.00	69248.0
176.90	4964.0
191.00	93.0
192.90	76.0
193.20	101.0
207.00	126.0
249.10	53.0
264.90	138.0
281.10	1559.0
282.10	432.0
283.10	266.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562

m/z	Abundance
36.00	672.0
37.10	3455.0
38.00	3310.0
39.00	1217.0
40.10	175.0
44.10	709.0
45.10	661.0
46.10	92.0
47.20	686.0
48.10	440.0
49.00	3121.0
50.10	14504.0
51.10	5032.0
52.00	214.0
52.80	96.0
53.80	67.0
55.10	247.0
56.00	1160.0
57.00	2105.0
58.00	85.0
58.90	55.0
60.00	680.0
61.10	3864.0
62.00	3541.0
63.10	2956.0
64.10	348.0
65.10	512.0
66.00	134.0
67.00	261.0
68.00	7449.0
69.10	8124.0
70.00	538.0
71.00	60.0
72.00	373.0
73.10	3380.0
74.10	12815.0
75.00	40072.0
76.00	3291.0
77.00	470.0
77.90	398.0
79.00	2508.0
79.90	726.0
80.90	2492.0
82.00	689.0
83.00	67.0
86.10	88.0
87.00	3168.0
88.00	3046.0
91.00	263.0
92.10	2228.0
93.10	3345.0
94.00	8834.0
95.10	72832.0
96.10	4531.0
97.00	193.0
102.80	53.0
104.00	371.0
105.00	183.0
106.00	422.0
107.10	107.0
111.10	94.0
111.90	97.0
113.00	80.0
114.80	103.0
115.90	284.0
116.90	474.0
118.00	338.0
119.00	472.0
123.80	118.0
128.10	233.0
128.80	123.0
129.80	290.0
131.00	82.0
134.80	177.0
135.80	53.0
137.00	129.0
139.10	57.0
140.00	134.0
141.00	743.0
142.10	91.0
142.90	983.0
143.90	89.0
145.00	205.0
146.00	105.0
147.00	82.0
147.80	157.0
149.80	60.0
150.20	50.0
153.10	82.0
154.90	173.0
157.00	123.0
159.00	159.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562

161.00	154.0
170.90	159.0
171.90	775.0
174.00	63336.0
175.00	4989.0
176.00	62136.0
177.00	4052.0
177.90	135.0
191.00	65.0
207.20	59.0
264.90	65.0
281.00	581.0
282.00	223.0
283.10	211.0

Instrument :
MSVOA_W
ClientSampleId :
BFB562