

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092624\
 Data File : VW030267.D
 Acq On : 26 Sep 2024 18:32
 Operator : SY/MD
 Sample : P4183-12
 Misc : 4.79g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Sep 27 04:41:43 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092624SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 27 04:39:02 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	490046	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	426543	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	175415	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	49782	7.529	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	30.120%
7) Chloroethane-d5	2.899	69	40804	8.372	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	33.480%
11) 1,1-Dichloroethene-d2	4.021	65	30001	9.160	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	36.640%#
21) 2-Butanone-d5	7.075	46	38534	24.338	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	48.680%
24) Chloroform-d	7.648	84	158385	10.915	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	43.680%
26) 1,2-Dichloroethane-d4	8.307	65	84958	11.479	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	45.920%#
32) Benzene-d6	8.276	84	300472	11.152	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	44.600%
36) 1,2-Dichloropropane-d6	9.276	67	97151	11.646	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	46.600%#
41) Toluene-d8	10.325	98	262730	10.972	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	43.880%
43) trans-1,3-Dichloroprop...	10.575	79	35655	11.277	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	45.120%
47) 2-Hexanone-d5	10.922	63	32581	27.902	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	55.800%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	69007	12.111	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	48.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	71570	11.724	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	46.880%#
Target Compounds						Qvalue
37) 1,2-Dichloropropane	9.276	63	11130	1.437	ug/L #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092624\
Data File : VW030267.D
Acq On : 26 Sep 2024 18:32
Operator : SY/MD
Sample : P4183-12
Misc : 4.79g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Sep 27 04:41:43 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092624SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 04:39:02 2024
Response via : Initial Calibration

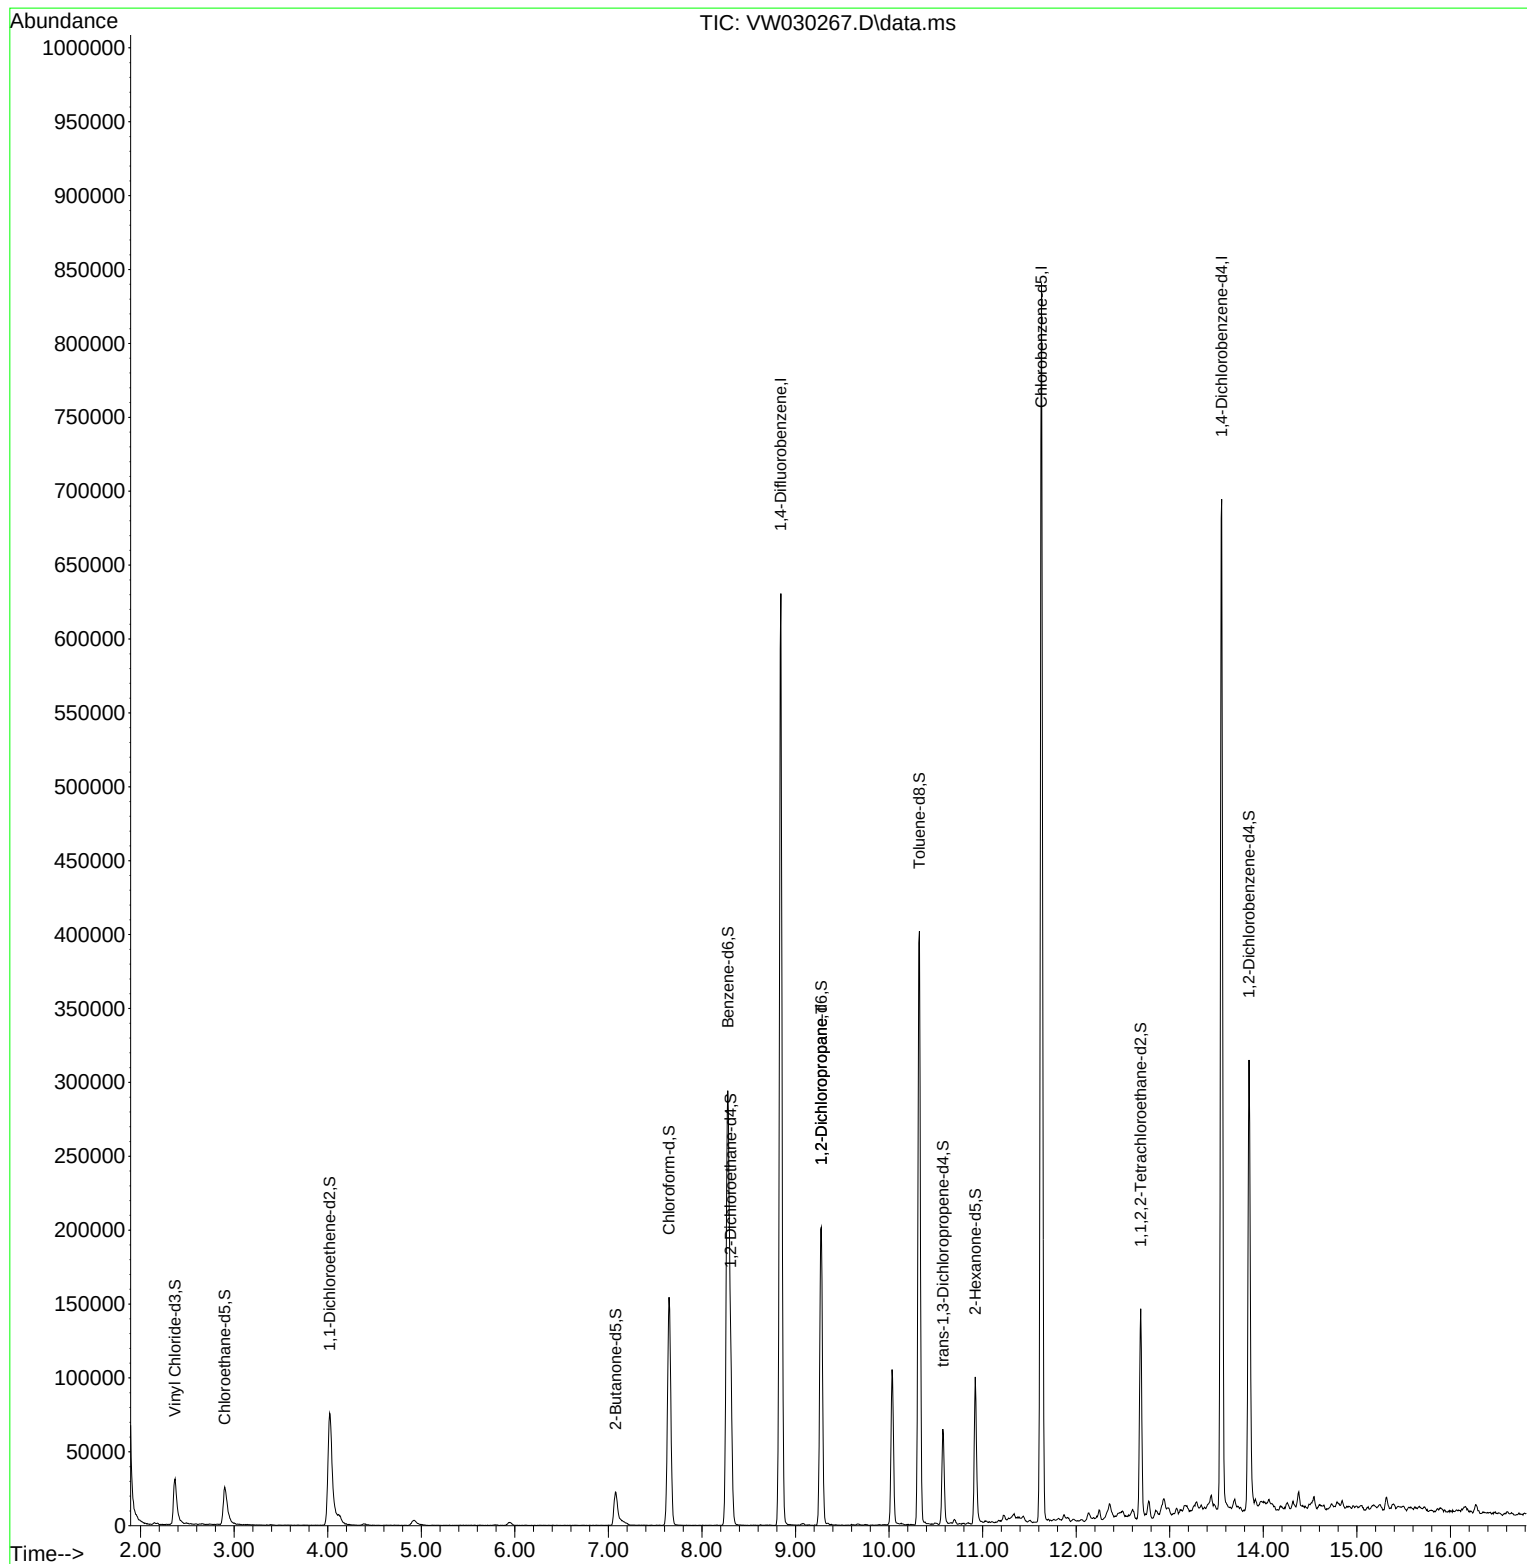

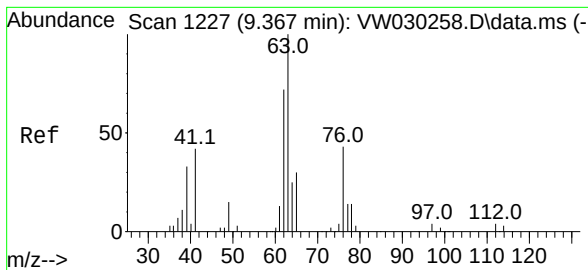

#37
 1,2-Dichloropropane
 Concen: 1.437 ug/L
 RT: 9.276 min Scan# 11
 Delta R.T. -0.091 min
 Lab File: VW030267.D
 Acq: 26 Sep 2024 18:32

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 63 Resp: 11130
 Ion Ratio Lower Upper
 63 100
 112 0.0 3.2 4.8#

