
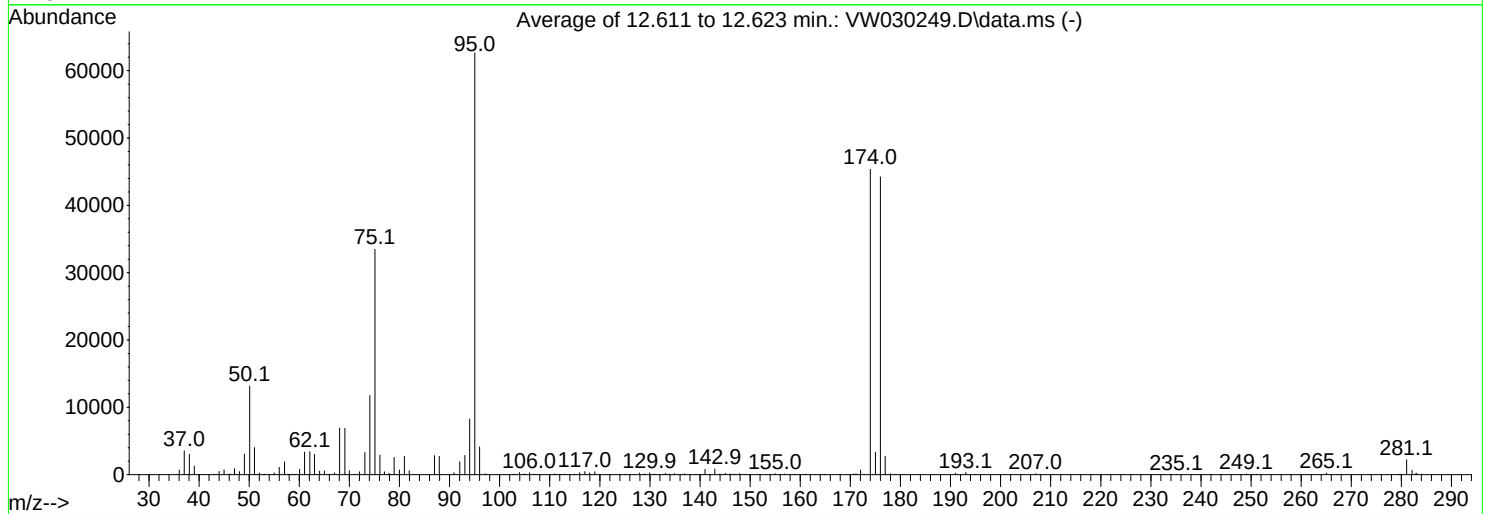


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092624\
Data File : VW030249.D
Acq On : 26 Sep 2024 09:57
Operator : SY/MD
Sample : BFB563
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB563

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092624SMA.M
Title : SFAM01.0
Last Update : Fri Sep 27 04:39:02 2024

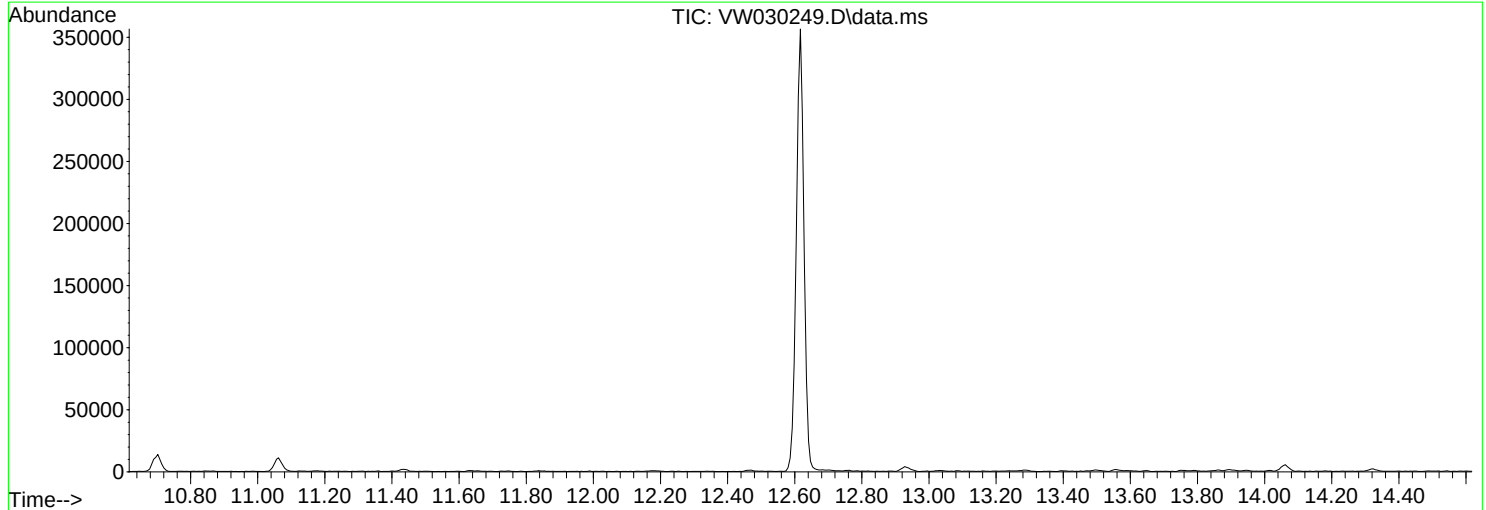

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	13173	PASS
75	95	30	80	53.4	33464	PASS
95	95	100	100	100.0	62653	PASS
96	95	5	9	6.6	4111	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	45349	PASS
175	174	5	9	7.3	3327	PASS
176	174	95	101	97.5	44221	PASS
177	176	5	9	6.2	2734	PASS

m/z	Abundance
39.90	150.0
44.00	142.0
45.80	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563

m/z	Abundance
36.00	736.0
37.10	3621.0
38.00	3054.0
39.10	1356.0
40.20	171.0
40.90	61.0
43.00	80.0
44.00	565.0
45.00	723.0
46.20	81.0
47.10	926.0
48.00	515.0
49.10	3136.0
50.10	13182.0
51.00	4195.0
52.10	142.0
52.90	115.0
53.10	116.0
54.90	306.0
56.00	970.0
57.00	1850.0
57.90	124.0
58.90	182.0
60.00	948.0
61.10	3312.0
62.10	3313.0
63.10	3268.0
64.00	494.0
65.00	675.0
66.10	88.0
67.00	248.0
68.10	6878.0
69.10	6677.0
70.00	569.0
72.00	422.0
73.10	3136.0
74.10	11485.0
75.10	32184.0
76.10	2829.0
77.00	336.0
77.90	306.0
79.00	2664.0
79.90	819.0
81.00	2843.0
82.00	675.0
82.80	52.0
86.00	102.0
87.00	2933.0
87.90	2707.0
90.90	343.0
92.00	1875.0
93.00	2774.0
94.00	7915.0
95.00	59320.0
96.00	4102.0
97.10	159.0
102.90	109.0
103.90	291.0
105.20	135.0
106.00	328.0
107.00	58.0
110.00	116.0
111.00	124.0
112.00	74.0
113.00	86.0
114.80	96.0
115.90	237.0
116.90	366.0
118.00	246.0
119.00	477.0
123.90	76.0
125.20	172.0
126.90	56.0
128.00	202.0
128.80	173.0
129.90	232.0
131.00	91.0
133.10	374.0
134.90	149.0
136.90	77.0
139.20	55.0
139.90	51.0
141.00	604.0
141.80	63.0
143.00	789.0
143.90	101.0
145.00	266.0
146.00	100.0
147.80	128.0
149.00	90.0
149.90	89.0
154.90	143.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563

155.80	65.0
156.90	62.0
159.10	62.0
161.10	84.0
163.00	127.0
164.90	77.0
170.70	144.0
172.10	579.0
174.00	39912.0
175.00	2856.0
176.00	38248.0
176.90	2155.0
178.00	163.0
179.10	107.0
191.00	342.0
192.30	65.0
193.00	453.0
194.00	81.0
195.00	94.0
207.10	204.0
207.90	108.0
235.10	54.0
249.10	178.0
250.20	77.0
251.10	188.0
265.10	328.0
265.90	102.0
267.20	105.0
268.10	55.0
278.00	79.0
279.40	126.0
279.80	120.0
281.00	3598.0
282.10	1147.0
282.90	479.0
284.10	178.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563

m/z	Abundance
36.00	761.0
37.10	3849.0
38.10	3551.0
39.10	1414.0
40.00	214.0
41.00	84.0
43.10	102.0
44.10	663.0
45.00	796.0
46.10	170.0
47.00	953.0
48.00	498.0
49.10	3311.0
50.10	15139.0
51.10	4512.0
52.00	251.0
53.10	91.0
54.00	144.0
55.00	249.0
56.00	1166.0
57.10	2069.0
58.40	54.0
59.10	58.0
60.00	770.0
61.00	3937.0
62.10	3850.0
63.10	3186.0
64.00	627.0
65.00	637.0
66.00	75.0
67.10	274.0
68.00	7669.0
69.10	7813.0
70.00	774.0
71.20	70.0
72.00	430.0
73.10	3742.0
74.10	12957.0
75.10	38880.0
76.10	3243.0
77.00	476.0
77.90	255.0
78.90	2747.0
80.00	680.0
81.00	2857.0
81.90	589.0
87.00	2945.0
87.90	3022.0
90.90	323.0
92.00	2057.0
93.00	2870.0
94.00	9084.0
95.10	71344.0
96.00	4539.0
97.00	144.0
102.80	121.0
104.00	338.0
104.90	138.0
106.00	399.0
106.80	86.0
110.80	59.0
111.20	69.0
112.00	77.0
113.00	66.0
115.00	121.0
116.00	329.0
117.00	536.0
118.00	307.0
119.00	423.0
123.90	79.0
124.90	87.0
127.00	78.0
128.00	290.0
129.00	144.0
130.00	315.0
130.80	104.0
133.20	177.0
133.80	80.0
134.10	91.0
135.00	142.0
137.00	134.0
139.20	54.0
141.00	864.0
142.10	97.0
143.00	1005.0
143.90	91.0
145.10	184.0
145.90	166.0
146.80	128.0
147.90	166.0
149.00	88.0
149.80	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563

155.00	138.0
155.90	85.0
157.00	96.0
158.90	70.0
161.00	144.0
163.10	53.0
164.80	57.0
170.70	127.0
171.20	186.0
172.00	927.0
174.00	51408.0
175.00	3675.0
176.00	51104.0
177.00	3241.0
178.10	104.0
191.10	206.0
193.10	406.0
194.10	79.0
195.10	51.0
206.90	174.0
249.00	123.0
251.10	61.0
265.10	214.0
267.10	51.0
279.70	95.0
281.10	2015.0
282.20	495.0
283.10	461.0
284.00	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563

m/z	Abundance
36.10	550.0
37.00	3173.0
38.10	2457.0
39.00	1085.0
40.00	195.0
44.00	654.0
45.00	656.0
46.20	89.0
47.00	751.0
48.10	367.0
49.00	2710.0
50.10	11199.0
51.10	3352.0
52.00	310.0
54.00	93.0
55.10	260.0
56.00	1162.0
57.10	1820.0
57.90	119.0
60.10	612.0
61.10	2799.0
62.10	3082.0
63.00	2566.0
64.10	418.0
65.10	361.0
66.10	55.0
67.00	247.0
68.00	6181.0
69.10	6179.0
70.00	441.0
71.00	52.0
72.00	459.0
73.10	2940.0
74.10	10797.0
75.10	29328.0
76.10	2628.0
77.00	450.0
78.10	322.0
79.00	2273.0
80.10	575.0
81.00	2419.0
81.90	526.0
82.90	107.0
87.00	2594.0
88.00	2384.0
91.00	188.0
92.10	1794.0
93.10	2949.0
94.00	7734.0
95.00	57296.0
96.00	3691.0
97.20	161.0
103.10	72.0
104.00	286.0
104.90	131.0
105.80	162.0
106.80	69.0
110.10	62.0
111.00	102.0
111.90	71.0
113.10	51.0
114.90	104.0
116.00	300.0
117.10	478.0
117.90	270.0
119.00	366.0
127.00	53.0
127.90	240.0
129.00	136.0
130.00	211.0
130.80	84.0
132.70	55.0
133.80	81.0
134.80	108.0
136.90	125.0
139.10	65.0
141.00	879.0
141.90	126.0
142.90	693.0
145.00	143.0
146.10	106.0
146.80	66.0
148.00	157.0
155.10	151.0
156.80	106.0
158.90	59.0
160.80	68.0
171.10	141.0
172.00	572.0
174.00	44728.0
175.00	3449.0
176.00	43312.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563

177.00	2807.0
177.90	61.0
178.20	68.0
190.90	114.0
193.20	127.0
207.00	52.0
207.90	71.0
248.80	75.0
264.90	103.0
281.00	1005.0
282.10	254.0
283.10	205.0

Instrument :
MSVOA_W
ClientSampleId :
BFB563