
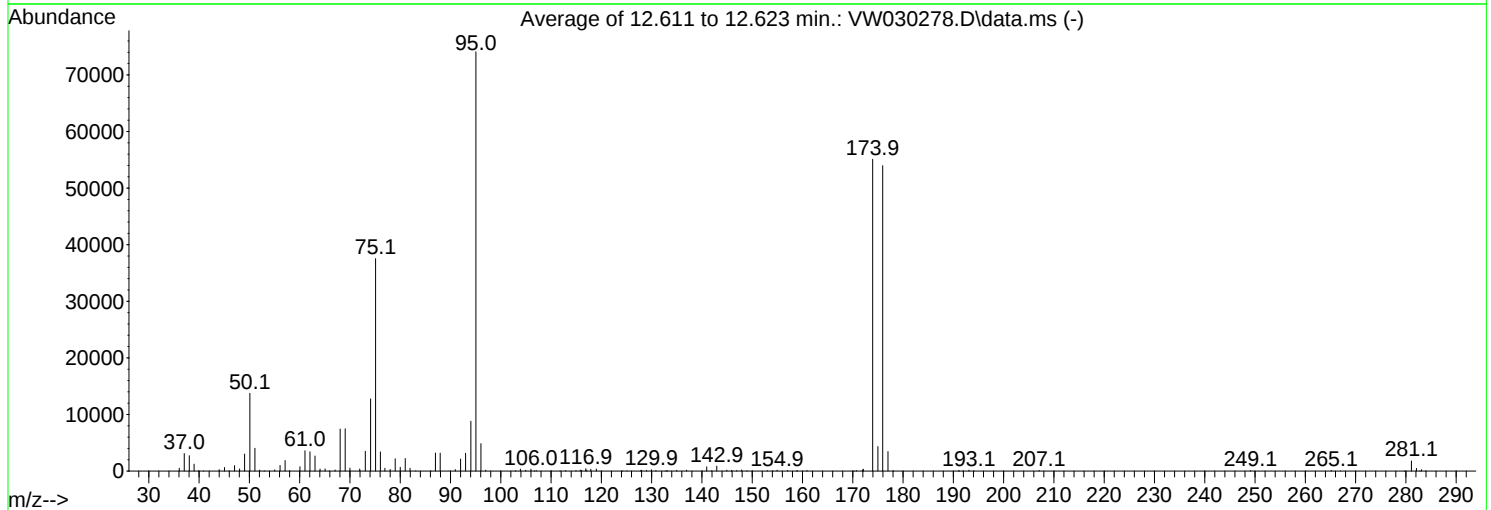


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092724\
Data File : VW030278.D
Acq On : 27 Sep 2024 13:40
Operator : SY/MD
Sample : BFB564
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB564

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Sat Sep 28 02:37:12 2024

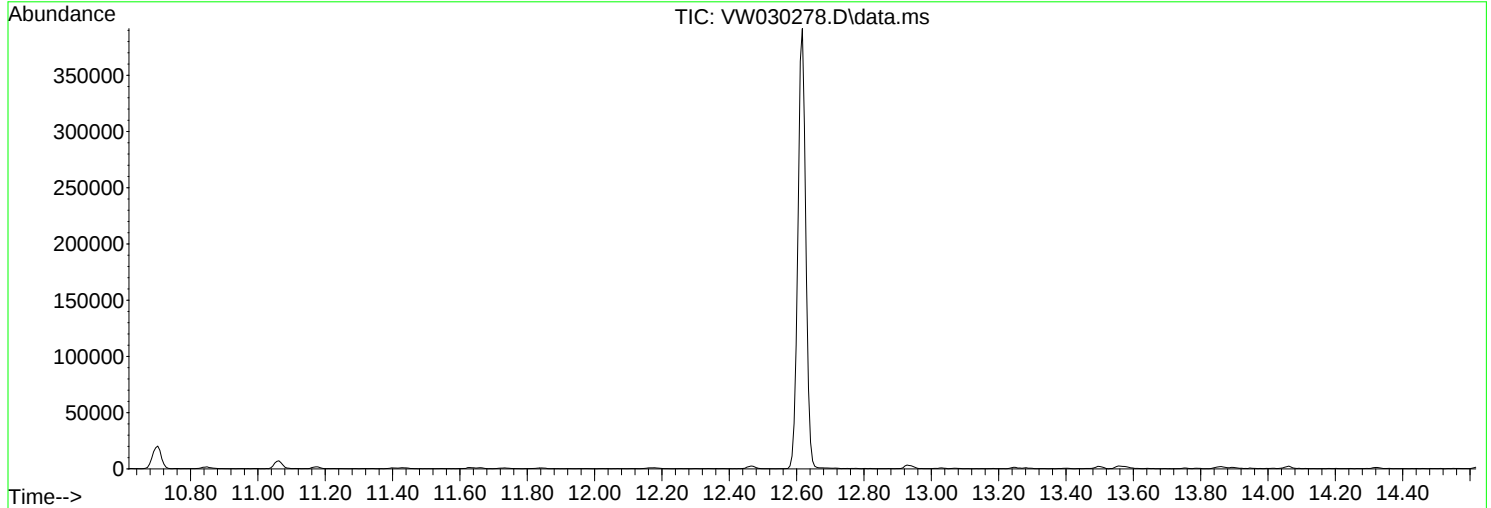

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	13742	PASS
75	95	30	80	50.7	37547	PASS
95	95	100	100	100.0	74101	PASS
96	95	5	9	6.6	4855	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.3	55088	PASS
175	174	5	9	7.9	4338	PASS
176	174	95	101	98.0	53971	PASS
177	176	5	9	6.4	3448	PASS

m/z	Abundance
39.90	113.0
44.00	177.0

Instrument :
MSVOA_W
ClientSampleId :
BFB564

m/z	Abundance
36.10	527.0
37.00	3292.0
38.10	3016.0
39.00	1383.0
40.00	202.0
44.00	555.0
45.10	736.0
46.00	116.0
47.10	989.0
48.10	358.0
49.10	3035.0
50.10	15423.0
51.10	4466.0
52.10	194.0
53.00	78.0
55.10	201.0
56.10	1087.0
57.10	2078.0
58.00	149.0
60.10	797.0
61.10	3634.0
62.00	3338.0
63.10	2895.0
64.00	413.0
65.00	436.0
67.10	152.0
68.00	8382.0
69.10	8189.0
70.00	567.0
72.00	335.0
73.10	3881.0
74.10	13488.0
75.10	38752.0
76.10	3375.0
77.00	371.0
78.00	203.0
79.00	2454.0
80.00	867.0
81.00	2316.0
82.00	547.0
87.00	3086.0
88.00	3404.0
91.00	386.0
92.00	2106.0
93.00	3185.0
94.10	9304.0
95.10	76080.0
96.10	5275.0
97.00	200.0
102.90	140.0
103.90	361.0
105.00	112.0
106.00	329.0
106.70	77.0
107.10	82.0
110.00	107.0
112.90	74.0
114.90	104.0
116.10	354.0
116.90	570.0
117.80	315.0
119.00	401.0
124.20	55.0
125.10	119.0
127.80	241.0
129.00	133.0
129.90	226.0
130.90	108.0
133.00	264.0
135.00	186.0
136.90	210.0
141.00	859.0
141.90	90.0
142.90	733.0
145.00	204.0
145.90	93.0
146.90	72.0
147.90	167.0
149.00	88.0
153.00	60.0
154.10	66.0
155.00	192.0
157.10	143.0
158.80	60.0
160.90	80.0
170.80	58.0
171.90	649.0
174.00	50272.0
175.00	4285.0
175.90	55128.0
177.00	3065.0
178.10	81.0

Instrument :
MSVOA_W
ClientSampleId :
BFB564

191.00	154.0
191.90	95.0
193.10	289.0
207.10	223.0
249.10	145.0
265.10	196.0
279.70	58.0
281.10	2756.0
282.20	752.0
283.10	461.0

Instrument :
MSVOA_W
ClientSampleId :
BFB564

m/z	Abundance
36.10	590.0
37.00	3393.0
38.00	3257.0
39.00	1301.0
39.80	163.0
40.90	75.0
44.00	409.0
45.00	588.0
47.00	1029.0
47.90	430.0
49.00	3356.0
50.10	15200.0
51.10	4303.0
52.00	203.0
52.90	68.0
55.00	249.0
56.10	1156.0
57.10	2122.0
58.10	77.0
60.00	804.0
61.00	4246.0
62.00	3870.0
63.00	2875.0
64.10	475.0
65.10	450.0
67.10	232.0
68.00	7762.0
69.00	7975.0
70.00	586.0
72.00	454.0
73.10	3990.0
74.10	14099.0
75.10	42984.0
76.10	3807.0
77.00	610.0
78.10	361.0
79.00	2298.0
80.00	592.0
81.00	2495.0
81.90	551.0
83.10	76.0
87.00	3649.0
88.00	3452.0
90.90	251.0
92.00	2468.0
93.00	3462.0
94.10	9907.0
95.10	82320.0
96.10	5135.0
97.00	161.0
103.00	98.0
103.90	404.0
104.90	185.0
106.00	441.0
107.00	112.0
111.80	65.0
112.90	141.0
114.90	80.0
115.80	333.0
116.90	670.0
117.90	373.0
119.00	376.0
124.30	68.0
128.00	264.0
128.90	117.0
130.00	267.0
130.80	106.0
132.70	69.0
133.20	121.0
135.00	147.0
137.00	151.0
141.00	788.0
142.00	65.0
143.00	1047.0
144.90	142.0
145.90	184.0
146.90	119.0
147.90	295.0
149.00	72.0
153.10	98.0
154.10	65.0
155.00	163.0
157.00	96.0
159.00	115.0
160.90	155.0
170.80	101.0
172.10	582.0
174.00	59320.0
175.00	4467.0
176.00	60456.0
177.00	4331.0
178.10	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB564

191.20	138.0
193.10	218.0
194.10	75.0
207.00	168.0
249.10	127.0
265.20	127.0
267.00	55.0
281.10	2076.0
282.00	490.0
283.10	282.0
283.90	59.0

Instrument : MSVOA_W
ClientSampleId : BFB564

m/z	Abundance
36.00	417.0
37.10	2600.0
38.10	1887.0
39.00	1018.0
39.90	113.0
44.00	342.0
45.10	560.0
47.00	849.0
48.10	371.0
49.10	2624.0
50.10	10604.0
51.10	3336.0
52.00	110.0
55.10	226.0
56.10	776.0
57.10	1436.0
60.00	683.0
61.00	2879.0
62.10	3000.0
63.10	2262.0
64.00	181.0
65.00	298.0
65.90	54.0
67.00	226.0
68.10	6161.0
69.00	6257.0
70.00	452.0
71.90	328.0
73.00	2625.0
74.10	10656.0
75.10	30904.0
76.00	3013.0
76.90	513.0
77.90	318.0
79.00	1785.0
80.00	547.0
81.00	1848.0
82.00	423.0
83.10	57.0
86.10	86.0
87.00	2849.0
87.90	2678.0
90.90	155.0
92.00	1830.0
93.00	2801.0
94.00	7239.0
95.00	63904.0
96.00	4155.0
96.90	103.0
103.90	257.0
104.90	139.0
106.00	291.0
107.00	72.0
112.90	63.0
115.00	75.0
115.80	222.0
117.10	515.0
118.00	286.0
119.00	319.0
128.00	194.0
129.10	127.0
129.90	248.0
130.90	85.0
135.00	106.0
137.00	124.0
140.90	584.0
142.00	55.0
143.00	842.0
144.90	172.0
145.90	148.0
146.90	69.0
147.90	150.0
148.80	54.0
150.00	67.0
152.90	106.0
154.80	155.0
157.00	144.0
159.00	93.0
161.00	71.0
170.30	55.0
170.70	74.0
172.10	418.0
173.90	55672.0
175.00	4262.0
175.90	46328.0
177.00	2949.0
178.00	94.0
265.10	58.0
281.10	529.0
282.10	159.0
282.80	125.0

Instrument :
MSVOA_W
ClientSampleId :
BFB564