
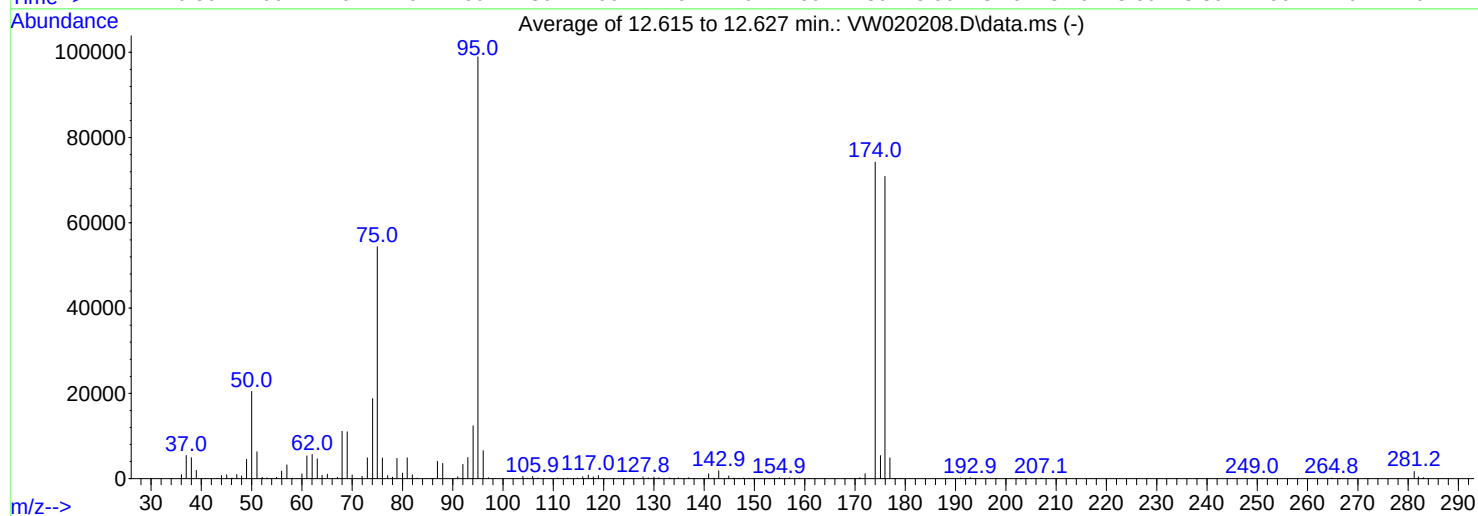


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092821\
 Data File : VW020208.D
 Acq On : 28 Sep 2021 07:58
 Operator : SY/VA
 Sample : BFB441
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB441

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092121SMA.M
 Title : SFAM01.0
 Last Update : Thu Sep 30 02:06:51 2021

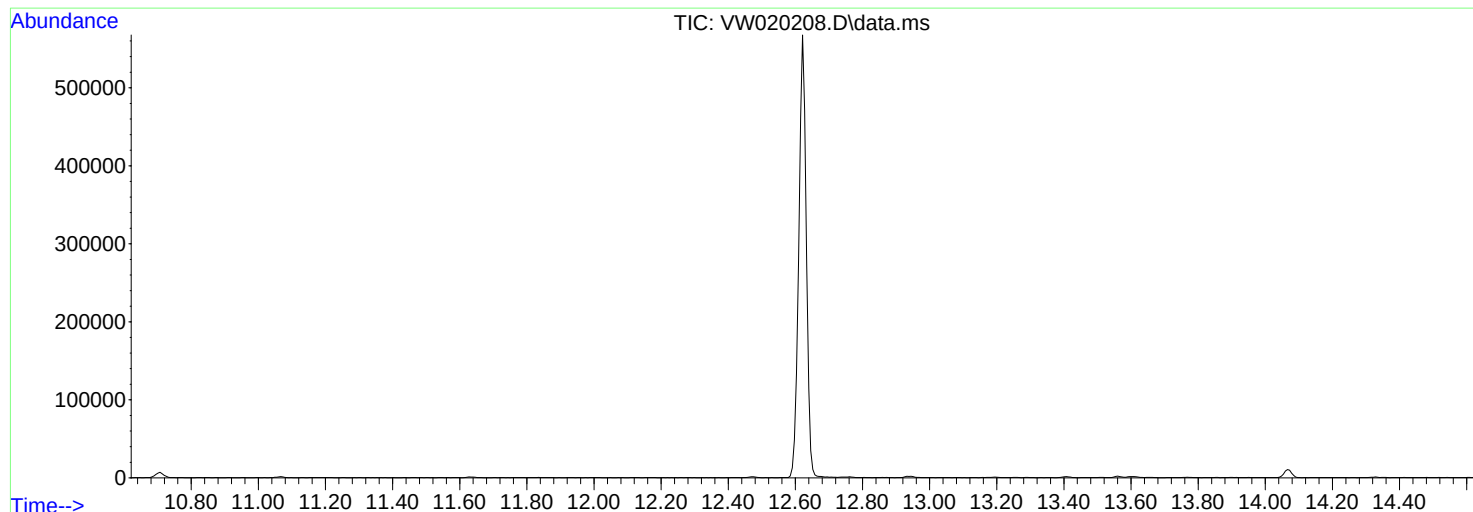

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	20451	PASS
75	95	30	80	55.0	54429	PASS
95	95	100	100	100.0	98936	PASS
96	95	5	9	6.6	6556	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.0	74243	PASS
175	174	5	9	7.3	5400	PASS
176	174	95	105	95.5	70915	PASS
177	176	5	10	6.9	4880	PASS

m/z	Abundance
40.10	130.0
44.00	227.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.10	856.0
37.00	5190.0
38.00	4880.0
39.00	2000.0
40.10	256.0
43.10	86.0
44.00	887.0
45.00	906.0
46.00	246.0
47.00	981.0
47.90	607.0
49.00	4403.0
50.00	19712.0
51.00	6644.0
52.10	258.0
53.10	166.0
55.10	340.0
56.00	1624.0
57.00	2912.0
58.00	110.0
58.20	109.0
59.00	100.0
60.00	1057.0
61.00	5297.0
62.10	5923.0
63.10	4584.0
64.00	964.0
65.10	1117.0
66.10	76.0
67.10	354.0
68.00	10509.0
69.00	10295.0
70.00	861.0
72.00	490.0
73.00	4765.0
74.10	18016.0
75.00	51312.0
76.00	4582.0
77.10	824.0
78.00	346.0
78.90	4590.0
80.00	1132.0
81.00	4777.0
82.00	840.0
83.00	93.0
85.80	149.0
86.90	3667.0
88.00	3224.0
91.10	379.0
92.00	2950.0
93.00	4790.0
94.10	11775.0
95.00	90240.0
96.10	6489.0
97.10	245.0
103.00	93.0
104.00	502.0
105.00	102.0
105.90	538.0
106.90	151.0
108.00	54.0
109.80	56.0
110.80	140.0
111.90	120.0
112.80	76.0
114.90	163.0
115.90	464.0
116.90	822.0
117.90	401.0
119.00	685.0
125.20	96.0
125.80	58.0
127.80	332.0
129.00	165.0
130.00	311.0
131.00	286.0
133.10	254.0
134.80	252.0
136.90	200.0
140.00	68.0
140.90	961.0
141.90	123.0
142.90	1735.0
144.10	89.0
144.90	637.0
145.70	156.0
146.80	104.0
148.10	178.0
148.90	75.0
149.90	115.0
152.90	103.0
153.70	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

155.00	160.0
157.10	173.0
157.90	63.0
158.90	116.0
160.60	56.0
170.90	341.0
172.00	1256.0
174.00	64280.0
175.00	4947.0
176.00	59968.0
176.90	4365.0
178.00	76.0
179.00	104.0
191.00	308.0
192.90	450.0
193.90	86.0
205.10	76.0
206.00	60.0
207.10	184.0
249.10	188.0
250.90	52.0
264.80	313.0
266.30	56.0
267.00	98.0
281.20	2315.0
282.10	625.0
283.00	327.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	1052.0
37.00	6183.0
38.00	5503.0
39.00	2303.0
40.10	227.0
40.80	78.0
43.10	82.0
44.10	1113.0
45.10	1093.0
46.10	175.0
47.00	1057.0
48.00	764.0
49.00	5404.0
50.00	23040.0
51.00	6852.0
52.10	316.0
53.10	221.0
54.90	319.0
56.00	2237.0
57.00	3840.0
58.00	126.0
60.00	1338.0
61.00	6061.0
62.00	6139.0
63.10	5384.0
64.00	797.0
65.00	1216.0
66.20	90.0
66.90	381.0
68.00	12334.0
69.00	12538.0
70.00	979.0
72.00	753.0
73.00	5396.0
74.00	21552.0
75.00	62200.0
76.00	5753.0
77.10	575.0
78.10	454.0
78.90	5178.0
80.00	1561.0
80.90	5623.0
81.90	1052.0
82.90	139.0
86.10	219.0
86.90	4785.0
88.00	4118.0
91.00	492.0
92.00	3902.0
93.00	5438.0
94.00	13862.0
95.00	114216.0
96.00	7162.0
97.20	178.0
102.90	97.0
103.90	608.0
104.80	148.0
105.90	575.0
107.00	187.0
108.00	91.0
110.00	92.0
110.80	159.0
111.90	89.0
112.80	152.0
114.80	147.0
115.90	449.0
117.00	916.0
118.00	461.0
118.90	844.0
125.10	75.0
127.90	467.0
128.90	243.0
130.00	407.0
131.00	187.0
133.10	160.0
134.90	234.0
136.90	200.0
140.90	1272.0
142.00	117.0
142.90	1987.0
143.90	94.0
144.90	579.0
145.90	202.0
147.00	86.0
147.80	195.0
148.90	110.0
149.90	136.0
152.00	50.0
152.90	64.0
153.70	77.0
155.00	276.0
156.90	205.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

158.00	95.0
158.90	142.0
160.70	83.0
160.90	83.0
171.10	314.0
172.00	1238.0
174.00	82344.0
175.10	5807.0
176.00	82080.0
177.00	5512.0
179.10	87.0
191.10	101.0
192.90	293.0
202.90	56.0
207.00	125.0
248.90	175.0
265.00	189.0
281.20	1888.0
282.00	489.0
283.10	304.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	875.0
37.00	4922.0
38.00	4415.0
39.00	1575.0
40.10	192.0
43.10	68.0
44.00	794.0
45.10	657.0
45.80	103.0
46.20	103.0
47.10	892.0
48.10	581.0
49.00	3787.0
50.00	18600.0
51.10	5466.0
52.10	370.0
53.00	154.0
54.90	304.0
55.90	1447.0
57.00	2928.0
58.10	181.0
60.00	952.0
61.00	4672.0
62.00	4996.0
63.00	3970.0
64.00	654.0
65.00	856.0
66.20	101.0
67.10	302.0
68.00	10546.0
69.00	10184.0
70.00	757.0
71.90	475.0
73.00	4495.0
74.00	16744.0
75.00	49776.0
76.00	4198.0
77.00	757.0
77.90	329.0
78.90	4530.0
80.00	1253.0
80.90	4284.0
82.00	841.0
82.80	110.0
85.80	83.0
87.00	3749.0
88.00	3355.0
90.90	503.0
92.00	3137.0
93.00	4648.0
94.00	11541.0
95.00	92352.0
96.10	6016.0
97.00	257.0
103.10	90.0
104.00	481.0
104.90	141.0
105.90	439.0
106.90	100.0
108.00	101.0
109.70	81.0
110.90	150.0
112.00	126.0
112.90	98.0
114.90	136.0
115.80	405.0
116.90	806.0
117.90	356.0
118.90	671.0
124.00	58.0
127.90	393.0
128.80	171.0
130.00	441.0
131.00	150.0
133.40	155.0
134.90	182.0
137.00	225.0
140.90	1182.0
141.90	129.0
142.90	1800.0
144.10	99.0
144.90	710.0
145.90	229.0
146.90	65.0
147.90	271.0
149.90	112.0
154.90	211.0
157.00	149.0
158.00	55.0
159.00	121.0
161.00	67.0
170.90	227.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

172.00	1034.0
174.00	76104.0
175.00	5446.0
175.90	70696.0
177.00	4763.0
177.80	77.0
191.10	70.0
192.90	96.0
207.00	114.0
265.00	63.0
281.10	911.0
282.10	182.0
282.80	132.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441