




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
 Data File : VW024670.D
 Acq On : 29 Sep 2022 12:10
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK411

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:37:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 02:36:56 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

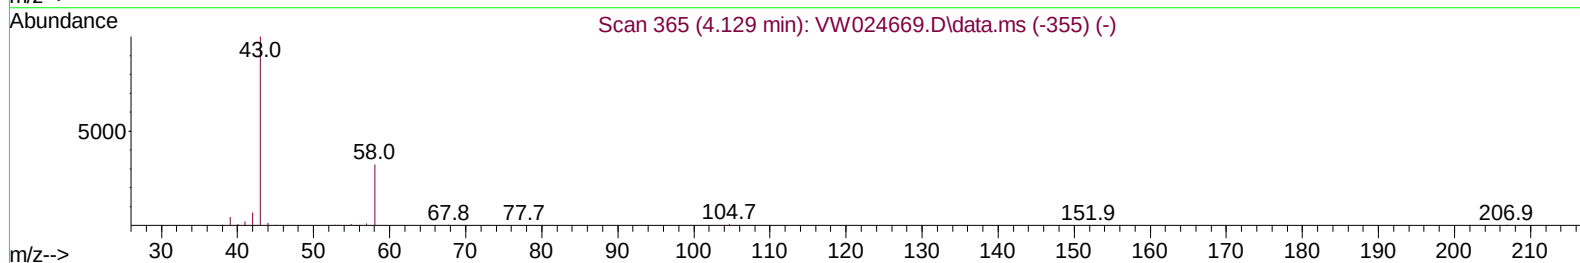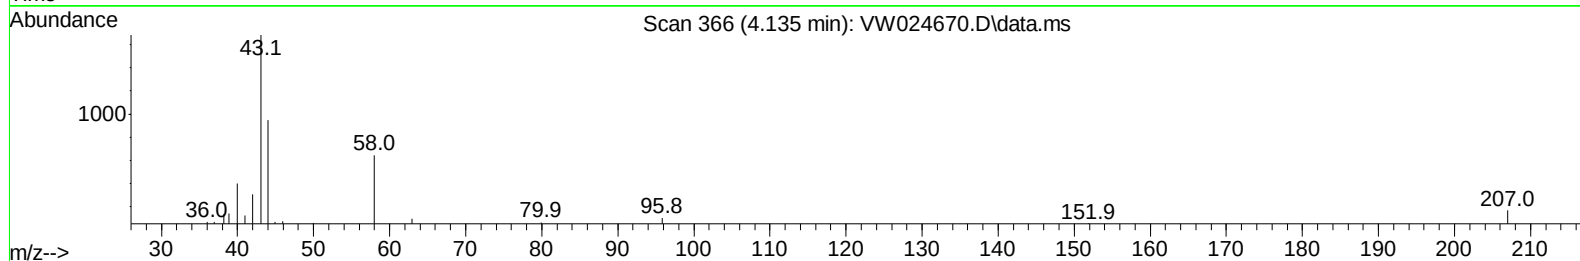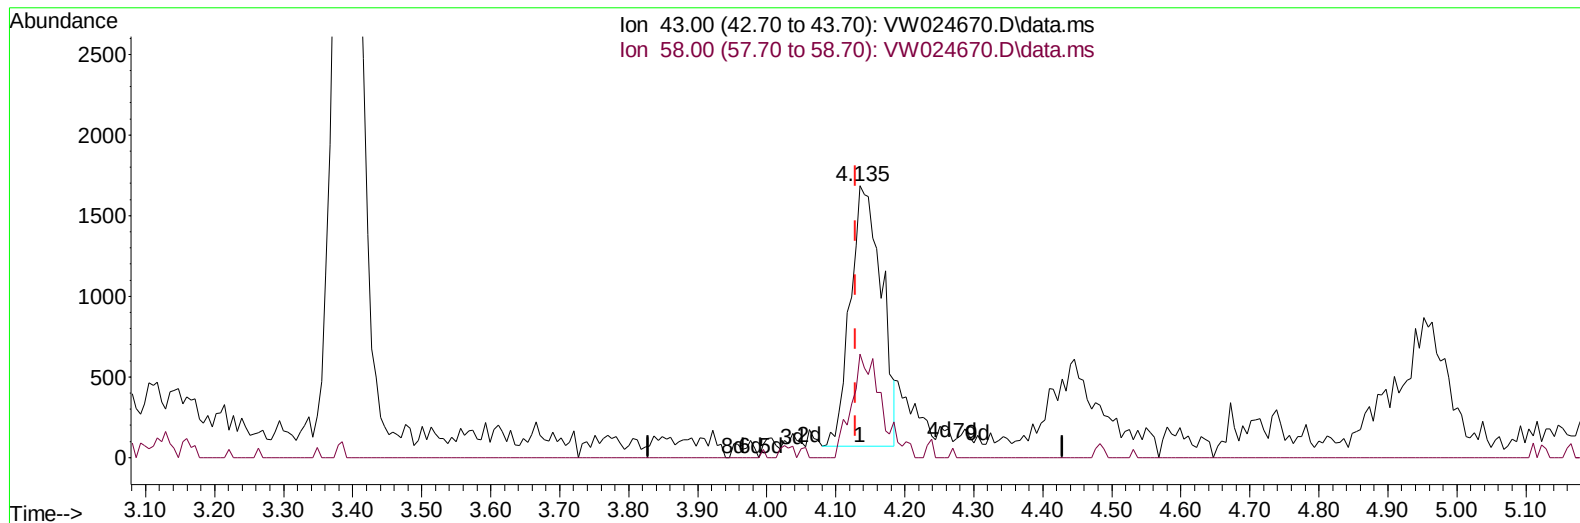

TIC: VW024670.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 3.18 ug/L

response 5064

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.80	21.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
 Data File : VW024670.D
 Acq On : 29 Sep 2022 12:10
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK411

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:37:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 02:36:56 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

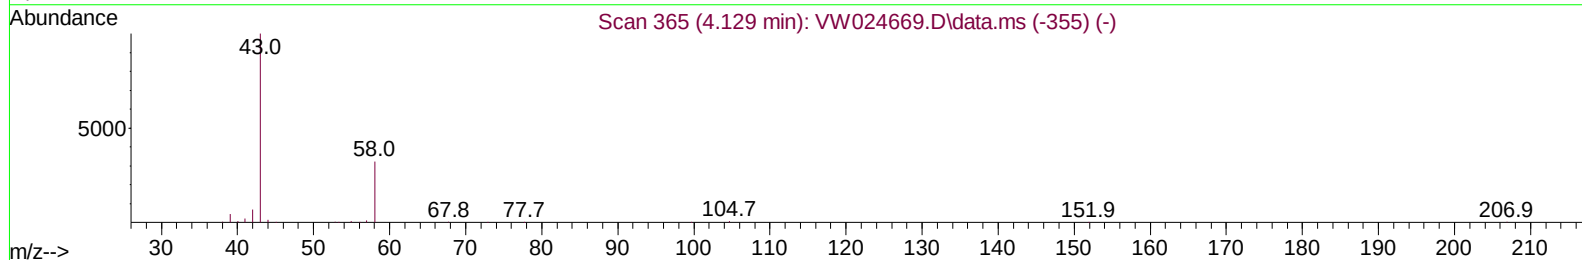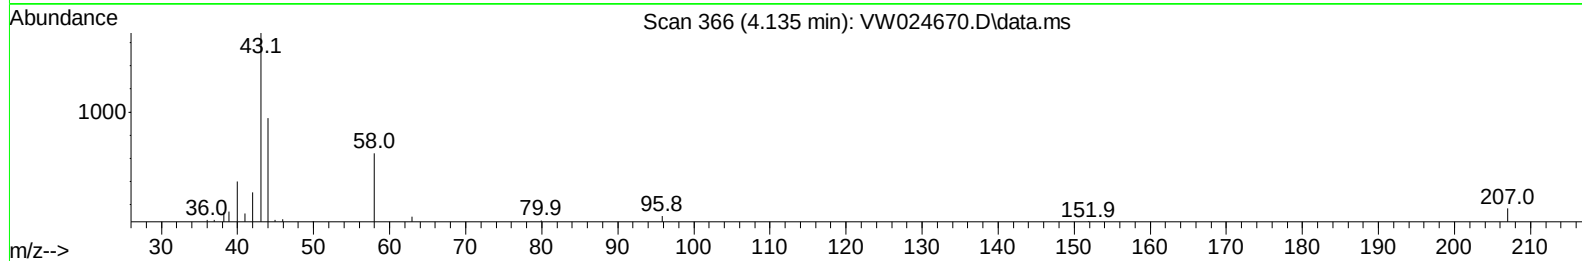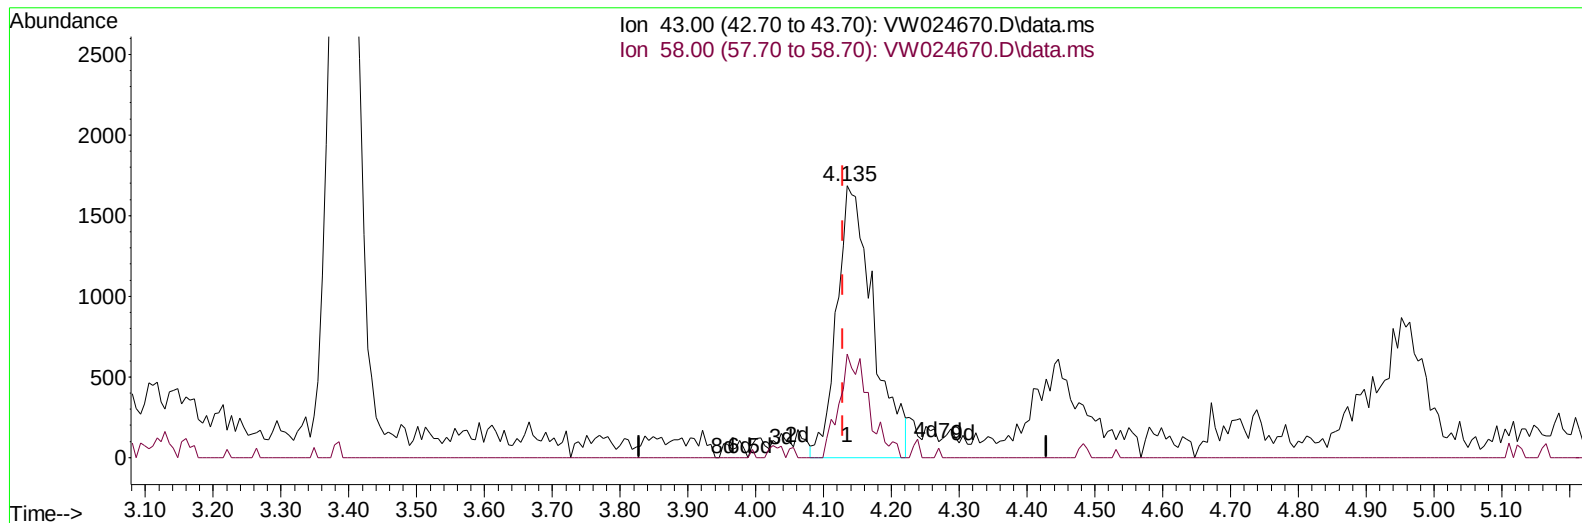

TIC: VW024670.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 3.93 ug/L m

response 6254

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.80	17.68
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
 Data File : VW024670.D
 Acq On : 29 Sep 2022 12:10
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK411

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

Quant Time: Sep 30 02:37:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 02:36:56 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		579559	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		502562	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		233159	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		172412	28.433	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.720%	
7) Chloroethane-d5	2.891	69		94409	26.793	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	107.160%	
11) 1,1-Dichloroethene-d2	4.019	63		277733	19.789	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	79.160%	
21) 2-Butanone-d5	7.080	46		101158	46.401	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	92.800%	
24) Chloroform-d	7.647	84		386135	24.922	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	99.680%	
26) 1,2-Dichloroethane-d4	8.305	65		198686	24.720	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	98.880%	
32) Benzene-d6	8.275	84		825994	25.714	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	102.840%	
36) 1,2-Dichloropropane-d6	9.274	67		244337	24.896	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	99.600%	
41) Toluene-d8	10.323	98		729414	25.407	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	101.640%	
43) trans-1,3-Dichloroprop...	10.579	79		102688	23.495	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	93.960%	
47) 2-Hexanone-d5	10.920	63		77670	46.254	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	92.500%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		171148	24.474	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	97.880%	
66) 1,2-Dichlorobenzene-d4	13.853	152		218926	26.683	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	106.720%	
Target Compounds							
13) Acetone	4.135	43		6254m	3.932	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
Data File : VW024670.D
Acq On : 29 Sep 2022 12:10
Operator : SY/VA
Sample : VW0929SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK411

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2022
Supervised By :Mahesh Dadoda 09/30/2022

Quant Time: Sep 30 02:37:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 02:36:56 2022
Response via : Initial Calibration

