




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
Data File : VW024673.D
Acq On : 29 Sep 2022 13:40
Operator : SY/VA
Sample : N4852-09
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW813

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:38:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 02:36:56 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2022
Supervised By :Mahesh Dadoda 09/30/2022

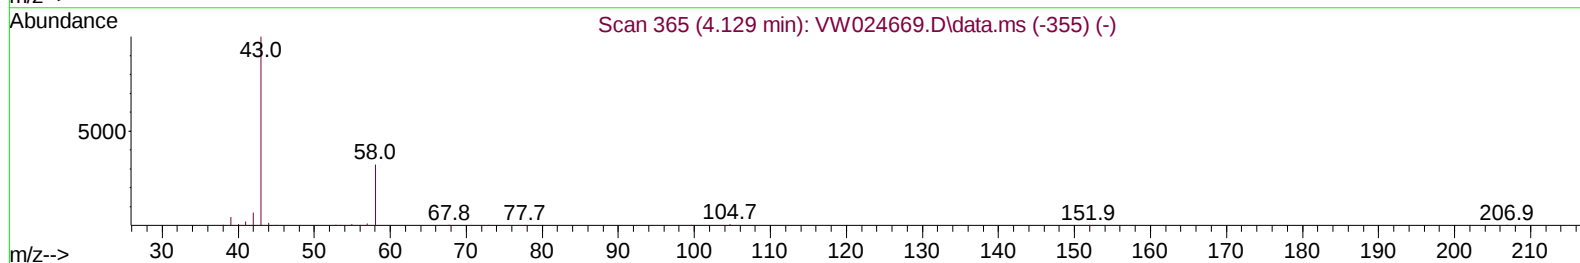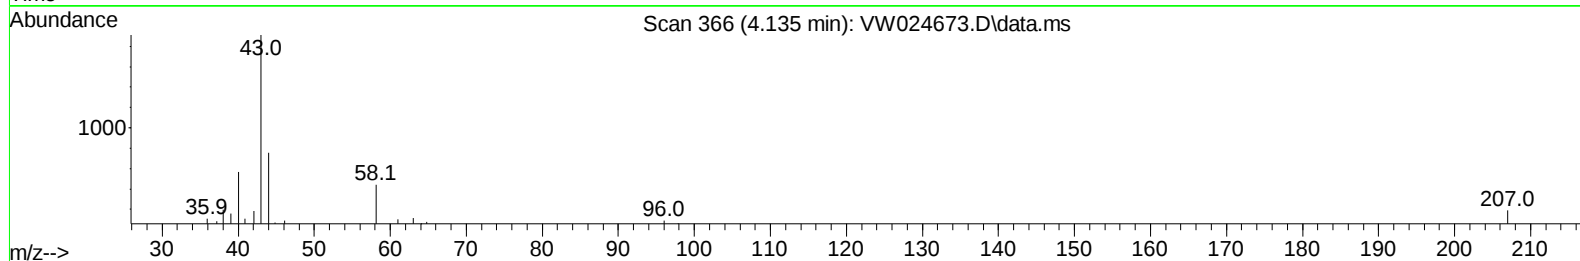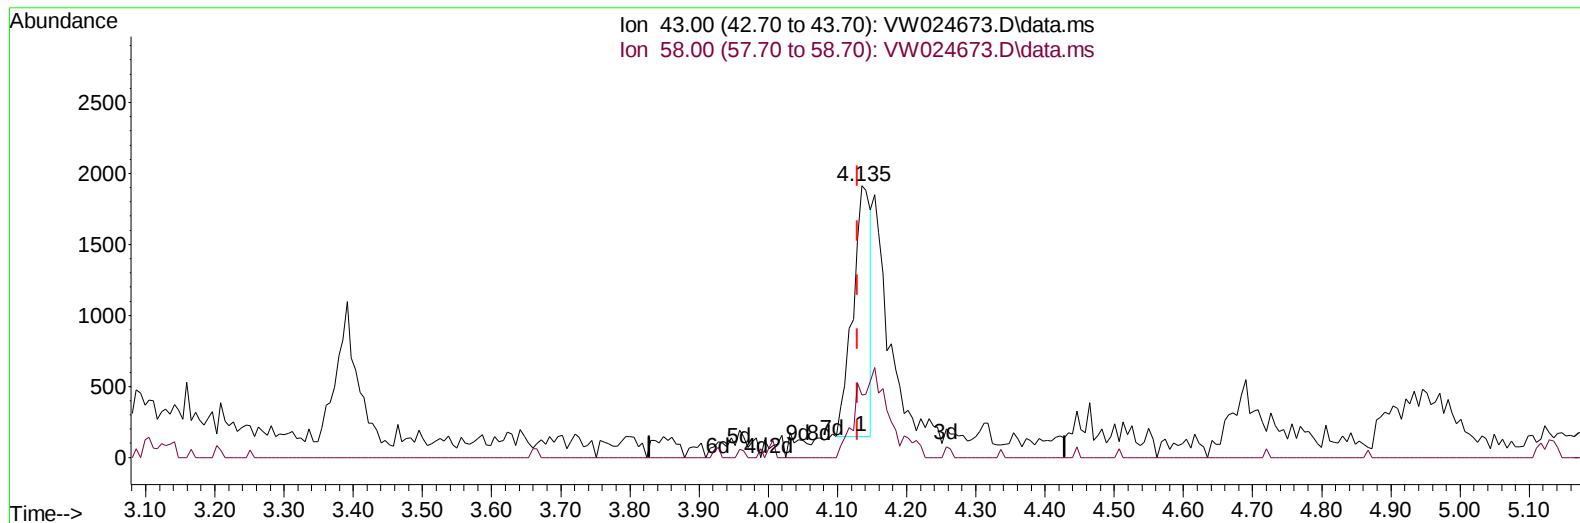

TIC: VW024673.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 1.62 ug/L

response 3157

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.80	11.21
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
 Data File : VW024673.D
 Acq On : 29 Sep 2022 13:40
 Operator : SY/VA
 Sample : N4852-09
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW813

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:38:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 02:36:56 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

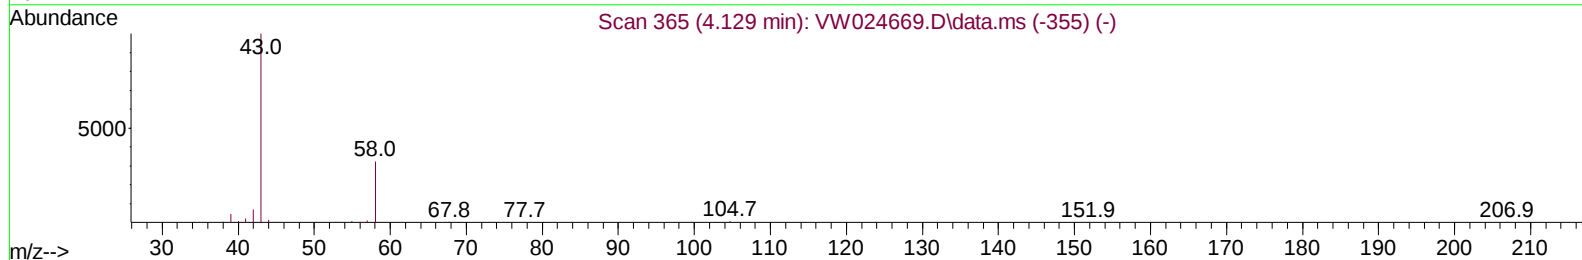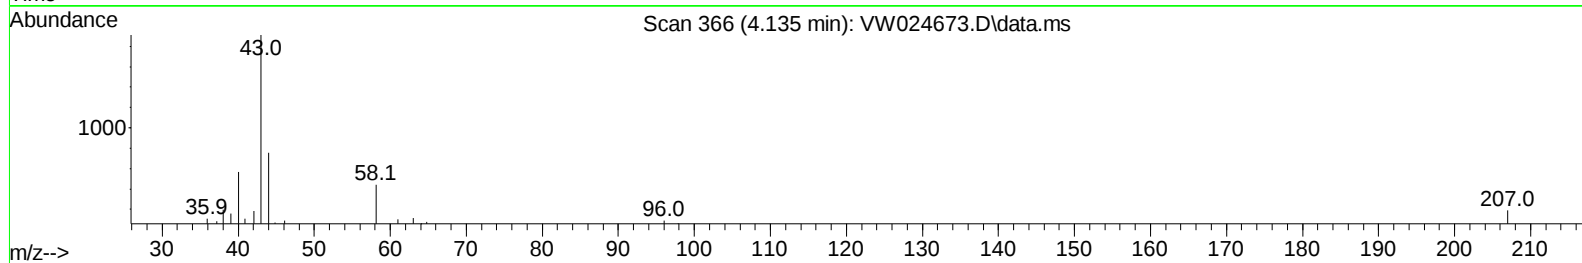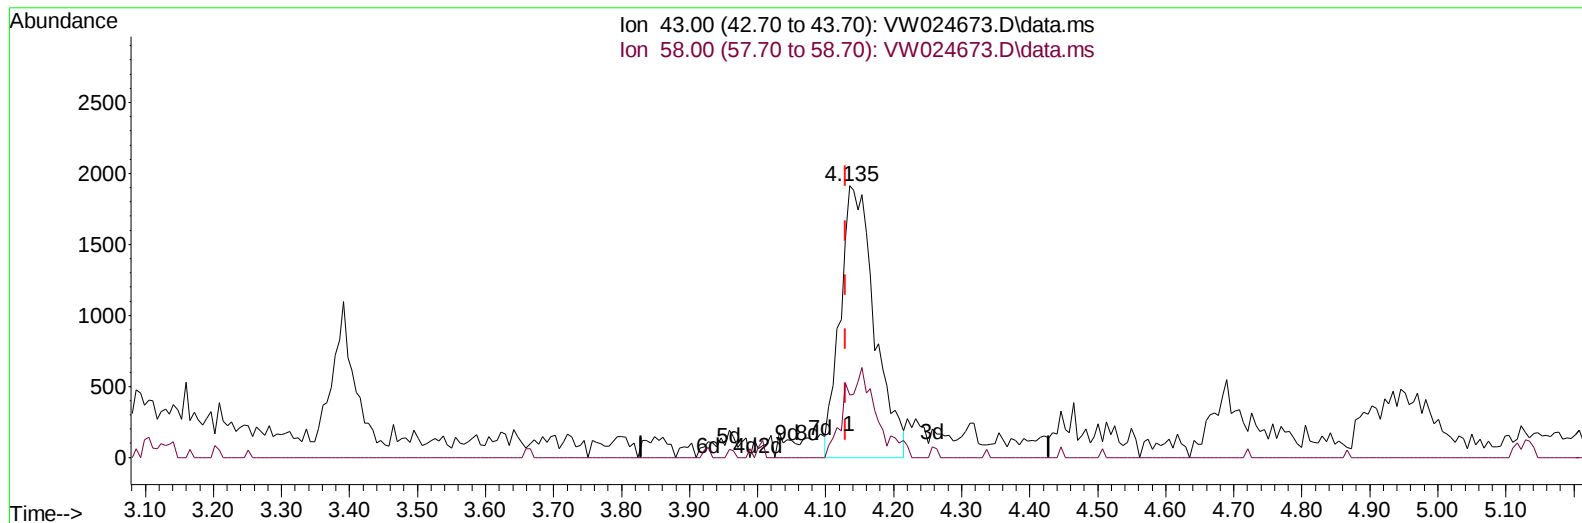

TIC: VW024673.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 3.44 ug/L m

response 6702

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	33.80	5.28
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
 Data File : VW024673.D
 Acq On : 29 Sep 2022 13:40
 Operator : SY/VA
 Sample : N4852-09
 Misc : 5.04g/10mL/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW813

Manual IntegrationsAPPROVED

Quant Time: Sep 30 02:38:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 02:36:56 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		709568	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		603197	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		246088	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		132418	17.837	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	71.360%	
7) Chloroethane-d5	2.891	69		88693	20.559	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	82.240%	
11) 1,1-Dichloroethene-d2	4.019	63		185704	10.807	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	43.240%#	
21) 2-Butanone-d5	7.080	46		127582	47.800	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	95.600%	
24) Chloroform-d	7.647	84		455460	24.010	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	96.040%	
26) 1,2-Dichloroethane-d4	8.305	65		244235	24.820	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	99.280%	
32) Benzene-d6	8.275	84		754239	19.563	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	78.240%	
36) 1,2-Dichloropropane-d6	9.274	67		287122	24.374	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	97.480%	
41) Toluene-d8	10.323	98		556819	16.159	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	64.640%	
43) trans-1,3-Dichloroprop...	10.579	79		93966	17.912	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	71.640%	
47) 2-Hexanone-d5	10.920	63		91272	45.286	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	90.580%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84		252620	30.098	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	120.400%#	
66) 1,2-Dichlorobenzene-d4	13.853	152		183161	21.151	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	84.600%	
Target Compounds							
13) Acetone	4.135	43		6702m	3.442	ug/L	
16) Methylene chloride	4.915	84		129909	9.322	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
Data File : VW024673.D
Acq On : 29 Sep 2022 13:40
Operator : SY/VA
Sample : N4852-09
Misc : 5.04g/10mL/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW813

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2022
Supervised By :Mahesh Dadoda 09/30/2022

Quant Time: Sep 30 02:38:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 02:36:56 2022
Response via : Initial Calibration

