

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
 Data File : VW024670.D
 Acq On : 29 Sep 2022 12:10
 Operator : SY/VA
 Sample : VW0929SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK411

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

Quant Time: Sep 30 02:37:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 30 02:36:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	579559	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	502562	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	233159	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	172412	28.433	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 113.720%			
7) Chloroethane-d5	2.891	69	94409	26.793	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 107.160%			
11) 1,1-Dichloroethene-d2	4.019	63	277733	19.789	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 79.160%			
21) 2-Butanone-d5	7.080	46	101158	46.401	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 92.800%			
24) Chloroform-d	7.647	84	386135	24.922	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 99.680%			
26) 1,2-Dichloroethane-d4	8.305	65	198686	24.720	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 98.880%			
32) Benzene-d6	8.275	84	825994	25.714	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 102.840%			
36) 1,2-Dichloropropane-d6	9.274	67	244337	24.896	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 99.600%			
41) Toluene-d8	10.323	98	729414	25.407	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 101.640%			
43) trans-1,3-Dichloroprop...	10.579	79	102688	23.495	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 93.960%			
47) 2-Hexanone-d5	10.920	63	77670	46.254	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 92.500%			
56) 1,1,2,2-Tetrachloroeth...	12.688	84	171148	24.474	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 97.880%			
66) 1,2-Dichlorobenzene-d4	13.853	152	218926	26.683	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 106.720%			
Target Compounds					Qvalue	
13) Acetone	4.135	43	6254m	3.932	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW092922\
Data File : VW024670.D
Acq On : 29 Sep 2022 12:10
Operator : SY/VA
Sample : VW0929SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 3 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VBLK411

Quant Time: Sep 30 02:37:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092622SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 30 02:36:56 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 09/30/2022
Supervised By :Mahesh Dadoda 09/30/2022

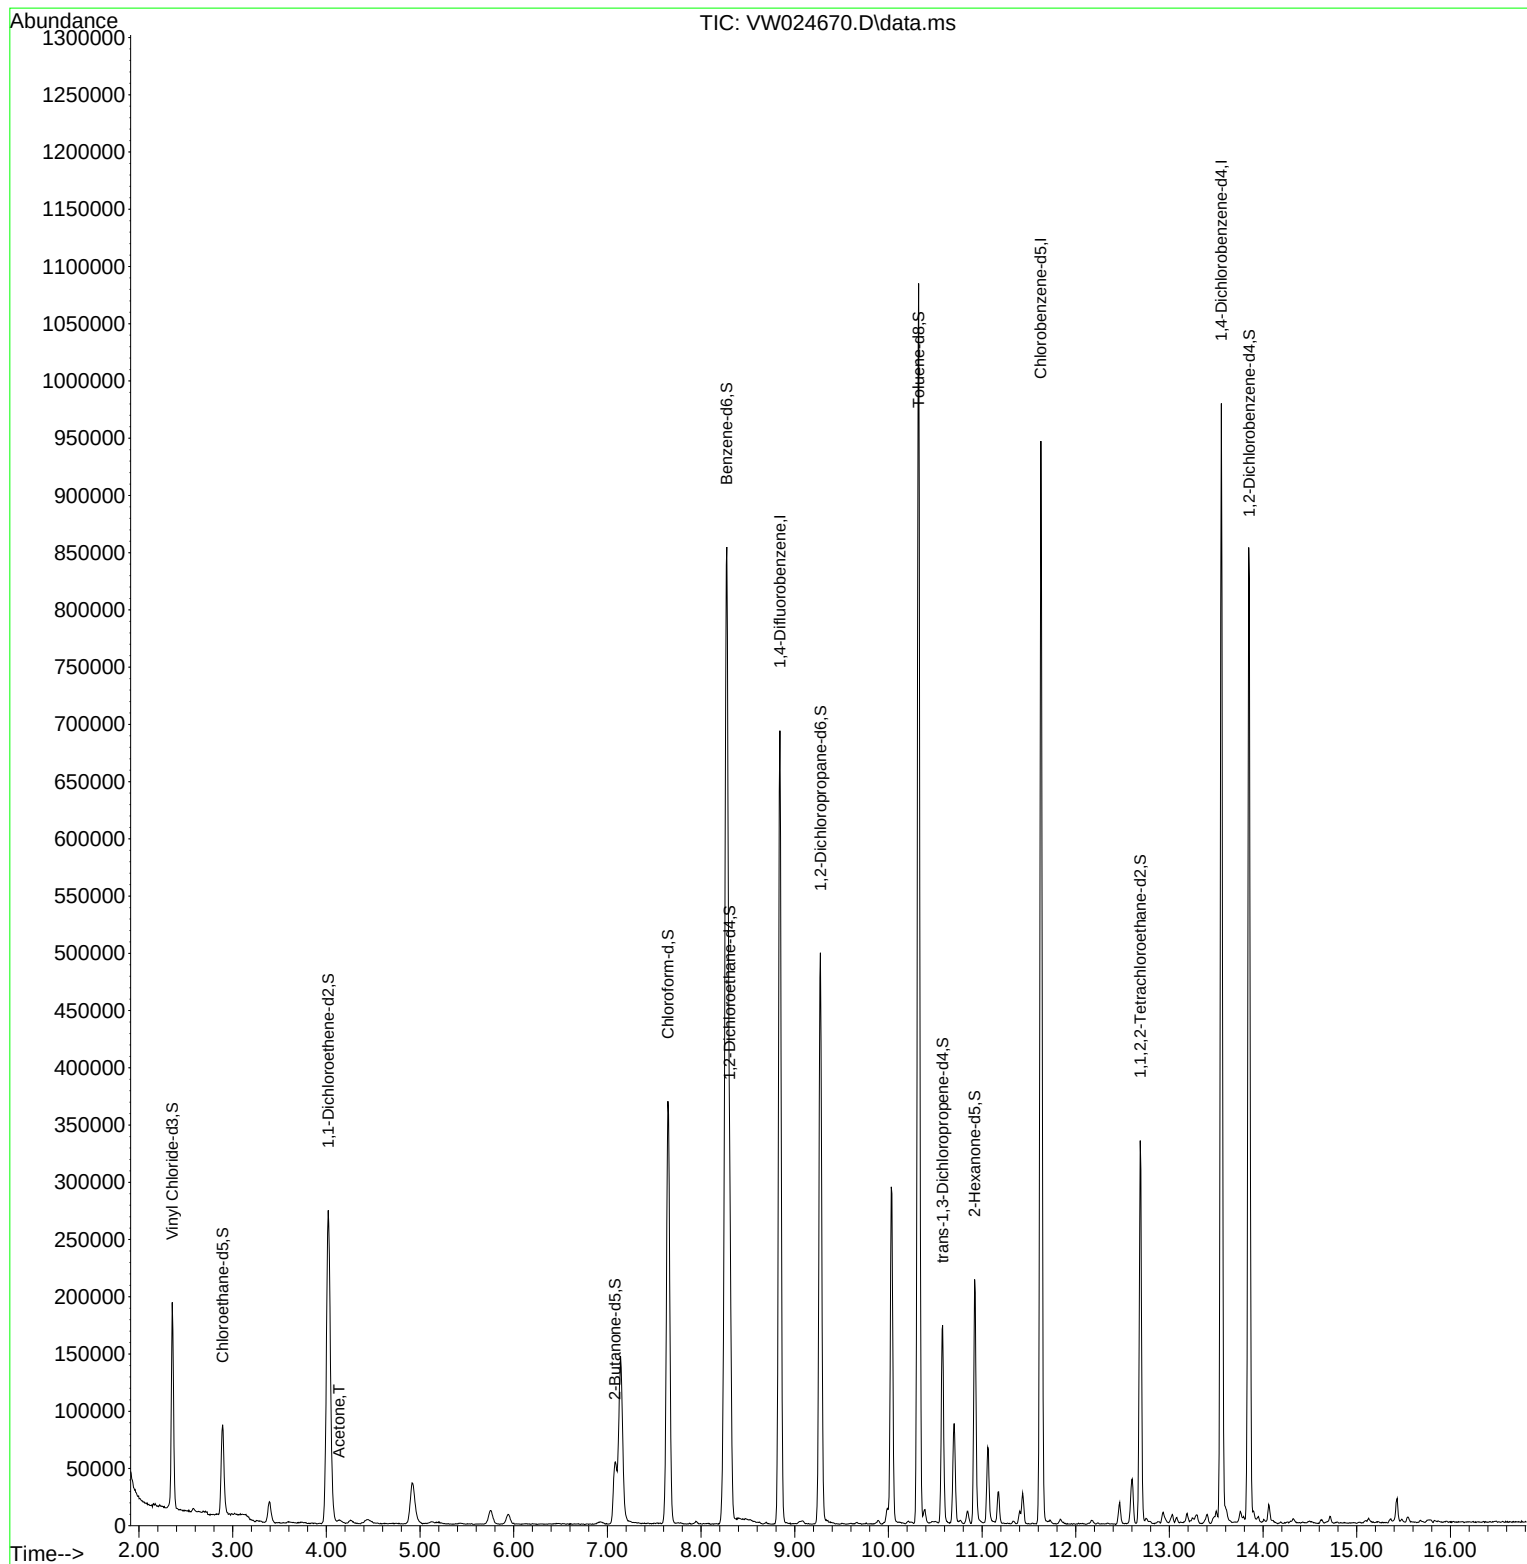

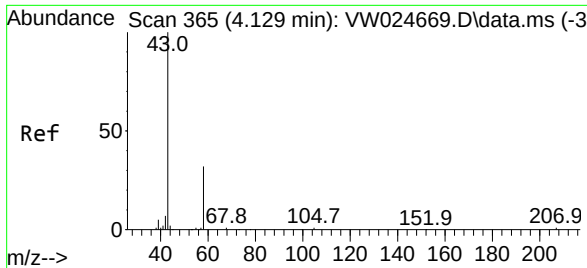

#13
 Acetone
 Concen: 3.932 ug/L m
 RT: 4.135 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024670.D
 Acq: 29 Sep 2022 12:10

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK411

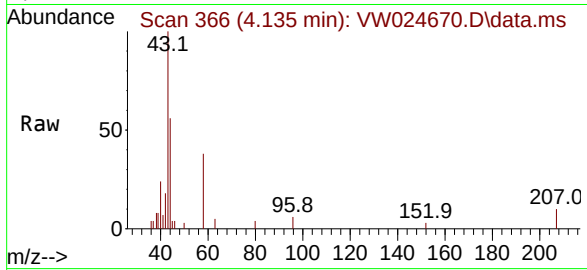

Tgt Ion: 43 Resp: 6254
 Ion Ratio Lower Upper
 43 100
 58 17.7 0.0 67.6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2022
 Supervised By :Mahesh Dadoda 09/30/2022

