

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093024\
 Data File : VW030290.D
 Acq On : 30 Sep 2024 12:38
 Operator : SY/MD
 Sample : VW0930SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 01 01:02:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 01 01:01:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	151828	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	142626	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	66146	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	33000	27.815	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.240%
7) Chloroethane-d5	2.905	69	23177	26.849	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.400%
11) 1,1-Dichloroethene-d2	4.021	65	22688	26.197	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	104.800%
21) 2-Butanone-d5	7.081	46	23336	48.910	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.820%
24) Chloroform-d	7.654	84	100148	24.553	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.200%
26) 1,2-Dichloroethane-d4	8.307	65	58158	27.317	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.280%
32) Benzene-d6	8.276	84	195521	24.459	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.840%
36) 1,2-Dichloropropane-d6	9.276	67	60263	25.065	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.280%
41) Toluene-d8	10.325	98	178546	24.358	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.440%
43) trans-1,3-Dichloroprop...	10.581	79	25441	25.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.760%
47) 2-Hexanone-d5	10.922	63	19211	48.389	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.780%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	45001	25.048	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.200%
66) 1,2-Dichlorobenzene-d4	13.848	152	58655	26.708	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.840%
Target Compounds			Qvalue			
39) cis-1,3-Dichloropropene	10.038	75	1807	0.514	ug/L #	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093024\
Data File : VW030290.D
Acq On : 30 Sep 2024 12:38
Operator : SY/MD
Sample : VW0930SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 01 01:02:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 01 01:01:52 2024
Response via : Initial Calibration

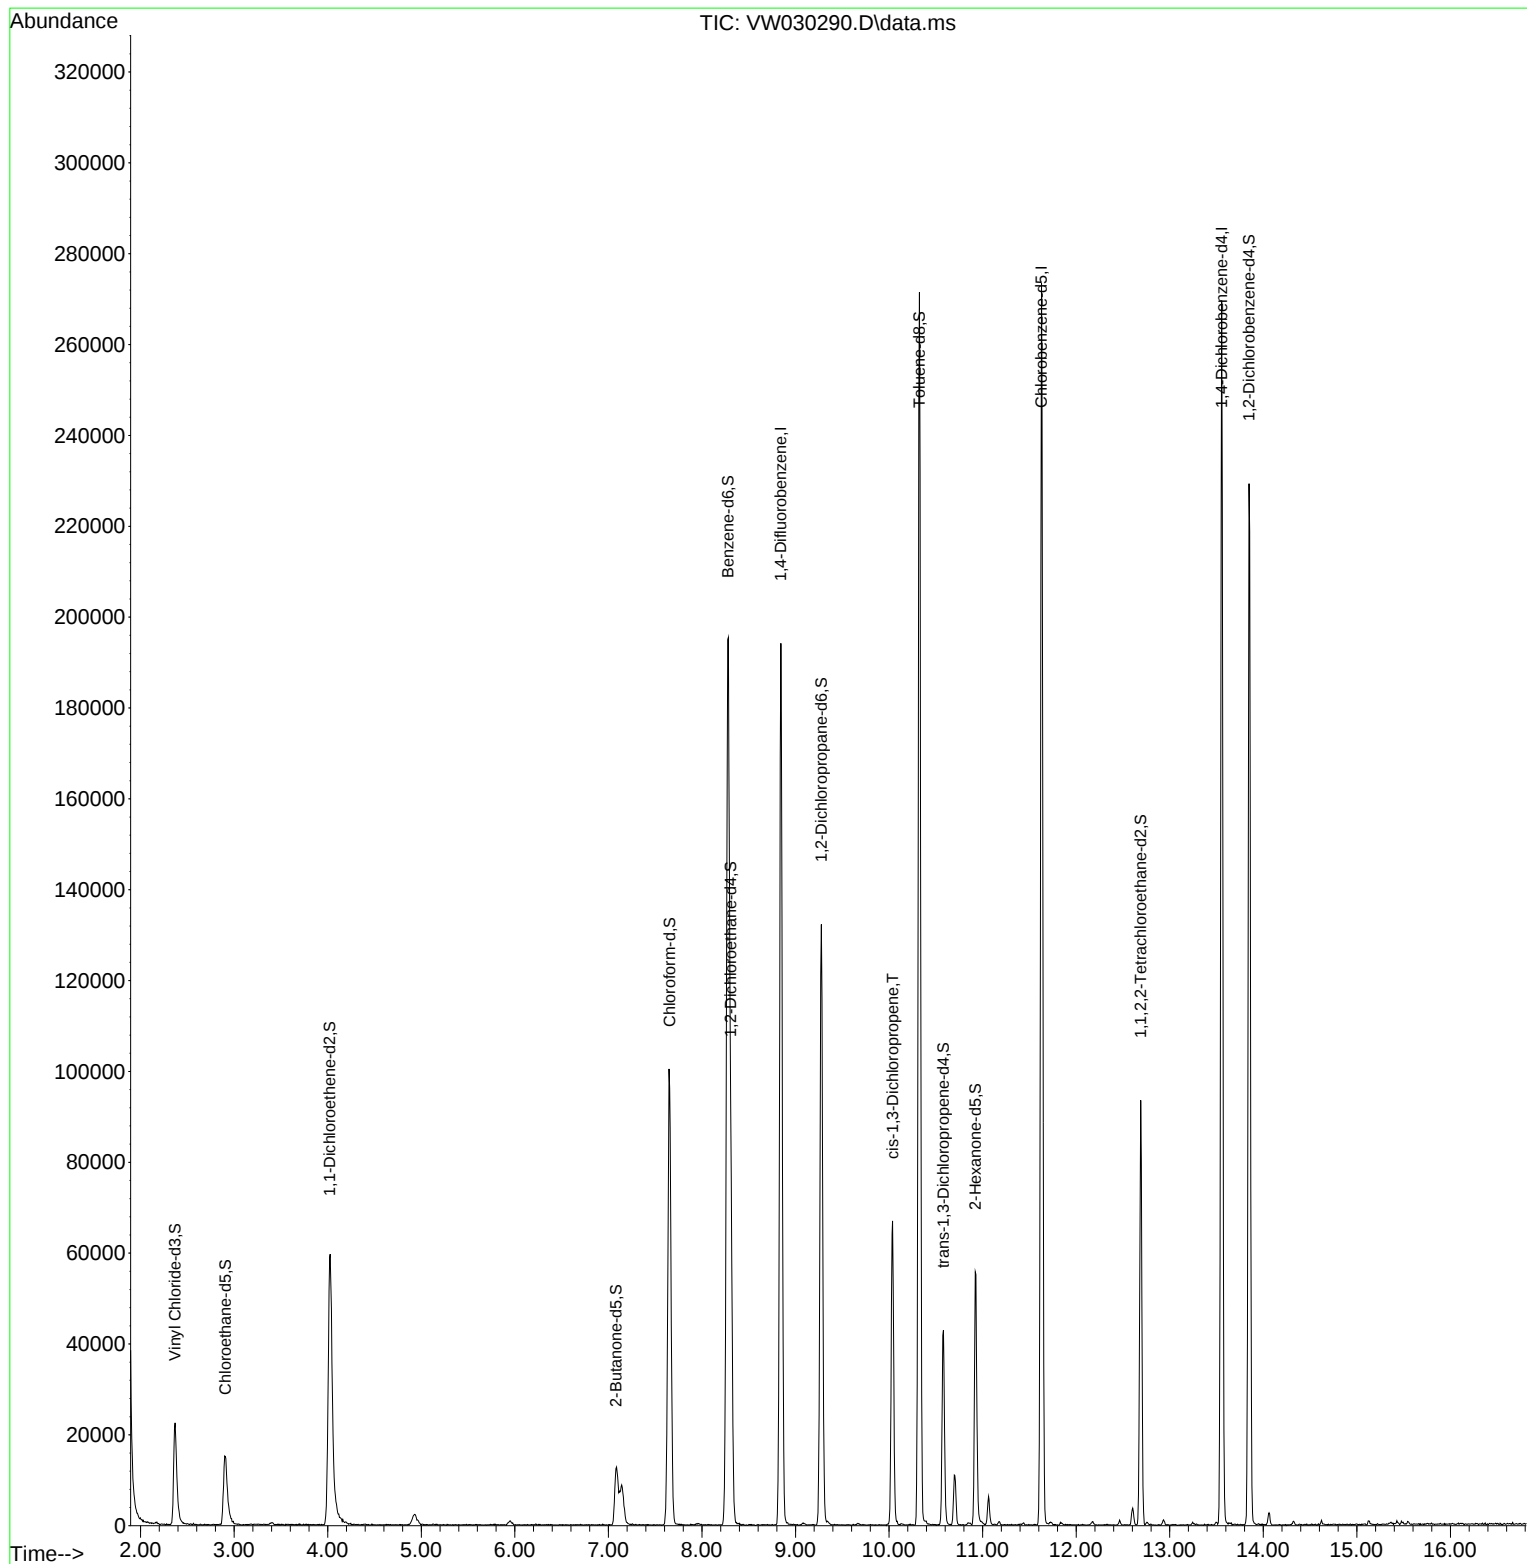

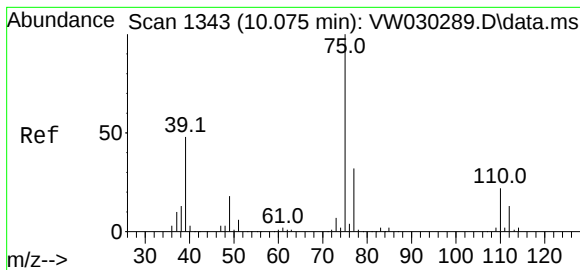

#39
 cis-1,3-Dichloropropene
 Concen: 0.514 ug/L
 RT: 10.038 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW030290.D
 Acq: 30 Sep 2024 12:38

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 1807
 Ion Ratio Lower Upper
 75 100
 77 69.5 22.0 40.8#

