
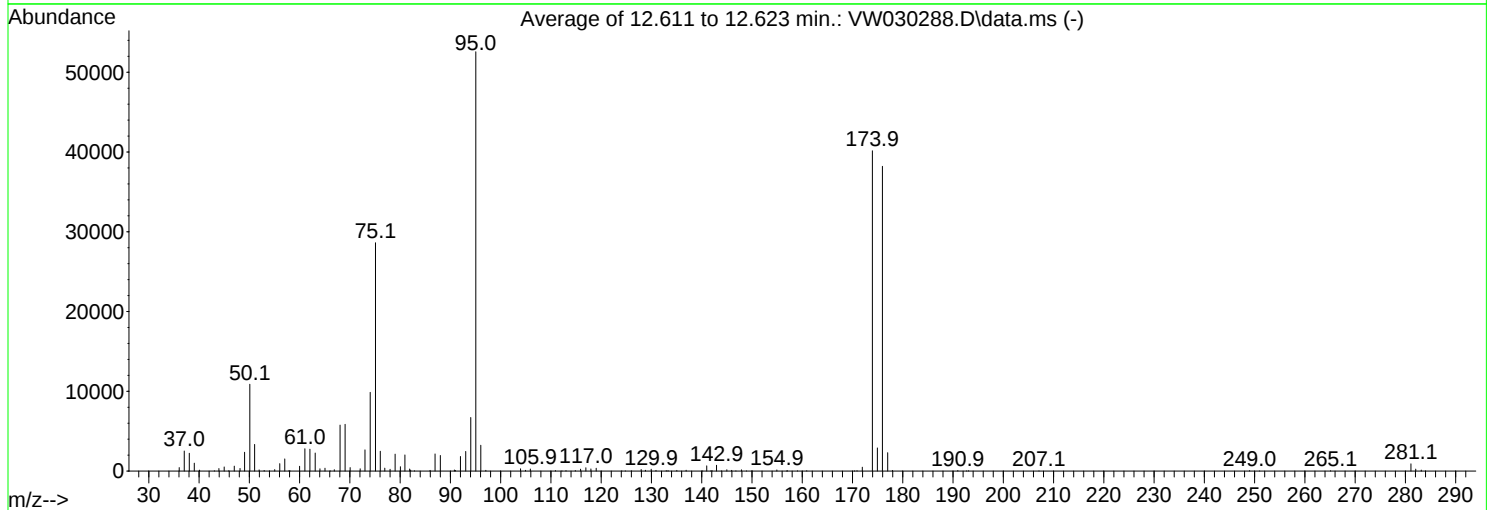


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093024\
Data File : VW030288.D
Acq On : 30 Sep 2024 10:29
Operator : SY/MD
Sample : BFB565
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB565

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Tue Oct 01 01:01:52 2024

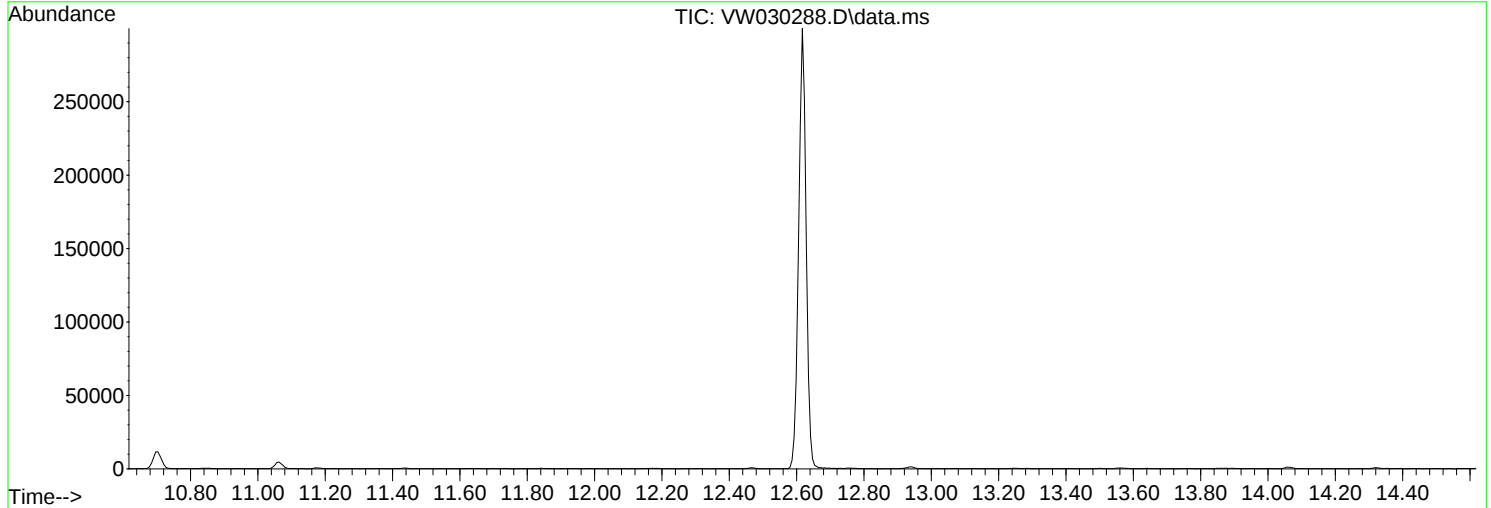

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	10885	PASS
75	95	30	80	54.5	28627	PASS
95	95	100	100	100.0	52571	PASS
96	95	5	9	6.2	3238	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.4	40155	PASS
175	174	5	9	7.2	2901	PASS
176	174	95	101	95.2	38208	PASS
177	176	5	9	6.0	2303	PASS

m/z	Abundance
39.90	121.0
43.90	103.0

Instrument :
MSVOA_W
ClientSampleId :
BFB565

m/z	Abundance
36.00	464.0
37.00	2489.0
38.10	2206.0
39.00	1123.0
39.80	114.0
40.10	108.0
44.00	469.0
45.10	523.0
47.00	680.0
48.10	316.0
49.00	2071.0
50.10	10946.0
51.00	3238.0
51.90	143.0
52.90	80.0
54.00	79.0
55.10	192.0
56.00	863.0
57.10	1345.0
57.90	91.0
60.00	555.0
61.00	2701.0
62.10	2427.0
63.10	2244.0
64.00	347.0
65.10	402.0
66.90	160.0
68.10	5463.0
69.00	5290.0
70.00	456.0
72.00	328.0
73.00	2599.0
74.00	9217.0
75.10	25552.0
76.10	2312.0
77.00	414.0
78.00	260.0
79.00	2036.0
80.00	508.0
81.00	2016.0
81.90	342.0
86.10	82.0
87.00	2169.0
88.00	1980.0
90.80	195.0
92.00	1510.0
93.00	2293.0
94.00	6336.0
95.10	46424.0
96.00	2921.0
97.00	76.0
103.90	308.0
105.00	105.0
105.90	246.0
114.90	79.0
115.90	152.0
116.90	457.0
117.90	204.0
119.00	260.0
124.80	66.0
128.00	182.0
128.80	80.0
130.00	220.0
130.90	93.0
132.90	108.0
133.30	129.0
135.10	144.0
136.90	145.0
141.00	637.0
141.80	77.0
142.90	707.0
145.00	253.0
146.00	74.0
147.90	152.0
154.90	99.0
156.90	58.0
159.00	57.0
160.90	59.0
172.00	562.0
174.00	34384.0
174.90	2067.0
176.00	29800.0
177.00	1944.0
190.90	135.0
193.10	139.0
207.10	83.0
249.00	109.0
251.00	53.0
265.10	125.0
281.20	1263.0
282.10	354.0
283.20	226.0

Instrument :
MSVOA_W
ClientSampleId :
BFB565

284.00

64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB565

m/z	Abundance
36.10	443.0
37.10	2716.0
38.10	2512.0
39.10	1093.0
40.10	108.0
43.00	61.0
44.00	489.0
45.00	636.0
45.90	118.0
47.00	600.0
48.10	390.0
49.00	2739.0
50.10	12222.0
51.00	3575.0
52.00	176.0
53.00	84.0
55.00	176.0
56.00	1179.0
57.00	1724.0
57.90	107.0
60.10	843.0
61.00	3198.0
62.00	3174.0
63.10	2462.0
64.10	317.0
65.10	454.0
66.10	70.0
66.80	145.0
68.10	6319.0
69.10	6627.0
70.10	477.0
72.10	252.0
73.00	3080.0
74.10	11382.0
75.10	34016.0
76.10	2877.0
77.00	344.0
78.10	265.0
79.00	2399.0
80.10	606.0
81.00	2248.0
81.90	427.0
82.90	51.0
85.90	96.0
86.90	2314.0
88.00	2090.0
91.00	231.0
92.00	2203.0
93.10	2959.0
94.00	7687.0
95.00	61712.0
96.10	3708.0
97.10	96.0
104.00	316.0
105.00	101.0
105.90	356.0
110.90	99.0
112.20	64.0
113.00	85.0
114.80	66.0
116.00	334.0
116.90	464.0
117.90	379.0
119.00	401.0
124.10	58.0
126.00	61.0
128.00	235.0
128.80	113.0
129.90	255.0
130.90	115.0
133.00	66.0
135.00	120.0
136.90	114.0
140.20	78.0
141.00	690.0
142.00	112.0
143.00	816.0
143.90	57.0
145.00	140.0
145.90	83.0
147.90	192.0
150.10	53.0
155.00	199.0
157.10	84.0
160.90	84.0
170.90	149.0
172.00	495.0
174.00	44056.0
175.00	3473.0
175.90	44624.0
177.00	2602.0
177.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB565

191.00	79.0
192.70	70.0
249.00	73.0
281.00	894.0
282.00	285.0
283.10	161.0

Instrument :
MSVOA_W
ClientSampleId :
BFB565

m/z	Abundance
36.10	422.0
37.00	2351.0
38.00	1971.0
39.10	774.0
40.10	147.0
43.10	56.0
43.90	314.0
44.90	391.0
47.00	584.0
48.20	285.0
49.10	2275.0
50.10	9487.0
51.10	3206.0
52.00	126.0
53.00	66.0
55.00	193.0
56.10	751.0
57.00	1503.0
58.10	71.0
59.90	418.0
61.10	2504.0
62.00	2631.0
63.10	2074.0
64.00	205.0
64.90	233.0
67.00	227.0
68.00	5509.0
69.10	5670.0
70.10	394.0
72.10	288.0
73.00	2295.0
74.10	9016.0
75.10	26312.0
76.00	2279.0
76.90	339.0
77.90	164.0
79.00	1930.0
80.00	531.0
80.90	1811.0
82.10	357.0
82.80	64.0
85.90	101.0
86.90	1970.0
88.00	1799.0
90.80	216.0
92.00	1786.0
93.10	2131.0
94.10	6121.0
95.00	49576.0
96.10	3085.0
97.00	119.0
103.90	247.0
104.90	77.0
105.90	166.0
110.90	82.0
113.00	91.0
114.80	53.0
115.80	235.0
117.00	333.0
118.00	222.0
119.00	416.0
127.90	173.0
128.80	118.0
129.90	224.0
130.90	67.0
133.30	52.0
137.00	61.0
141.00	641.0
142.10	70.0
143.00	660.0
145.10	116.0
145.90	106.0
146.80	96.0
147.90	146.0
148.90	67.0
149.90	52.0
155.00	139.0
157.00	67.0
159.10	59.0
170.40	70.0
171.90	404.0
173.90	42024.0
175.00	3163.0
176.00	40200.0
177.00	2362.0
178.00	87.0
281.00	567.0
281.90	100.0

Instrument :
MSVOA_W
ClientSampleId :
BFB565