

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093025\
 Data File : VW032309.D
 Acq On : 30 Sep 2025 17:26
 Operator : SY/MD
 Sample : Q3256-03
 Misc : 4.75g/5mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SOIL-PILE-1-WC-VOC

Quant Time: Oct 01 00:56:30 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W092525S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 26 07:11:42 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.965	168	194802	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.849	114	414330	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.629	117	425217	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.556	152	218009	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.319	65	179577	58.382	ug/l	0.00
Spiked Amount	50.000	Range	63 - 155	Recovery	=	116.760%
35) Dibromofluoromethane	7.898	113	148629	49.880	ug/l	0.00
Spiked Amount	50.000	Range	70 - 134	Recovery	=	99.760%
50) Toluene-d8	10.324	98	549507	51.170	ug/l	0.00
Spiked Amount	50.000	Range	74 - 123	Recovery	=	102.340%
62) 4-Bromofluorobenzene	12.617	95	203840	50.321	ug/l	0.00
Spiked Amount	50.000	Range	17 - 146	Recovery	=	100.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW093025\
Data File : VW032309.D
Acq On : 30 Sep 2025 17:26
Operator : SY/MD
Sample : Q3256-03
Misc : 4.75g/5mL/MSVOA_W/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SOIL-PILE-1-WC-VOC

Quant Time: Oct 01 00:56:30 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W092525S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 26 07:11:42 2025
Response via : Initial Calibration




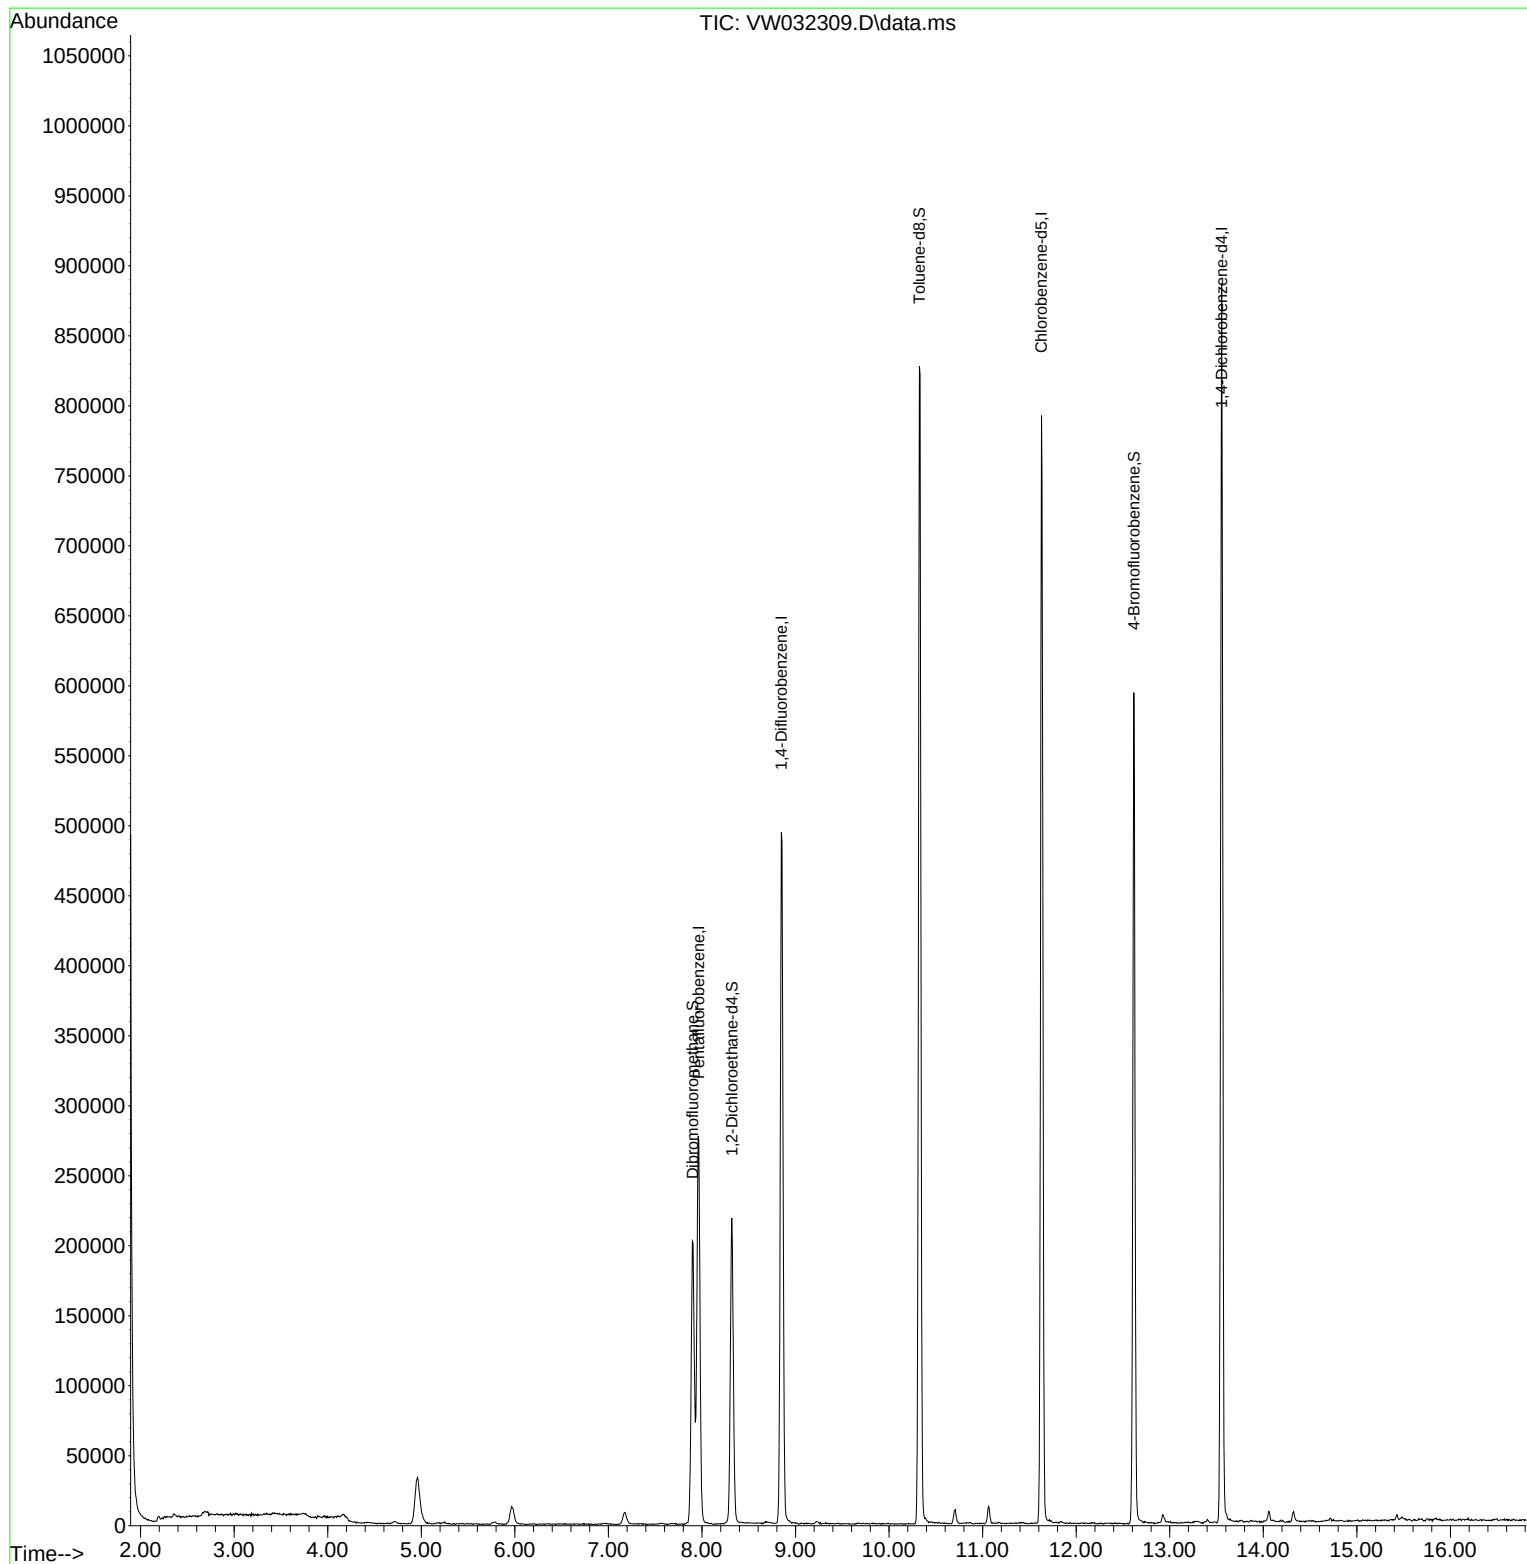


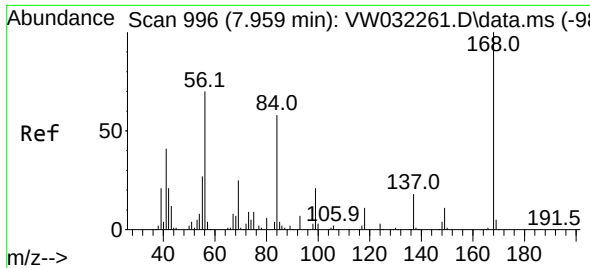

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.965 min Scan# 99
Delta R.T. 0.006 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26




Instrument :
MSVOA_W
ClientSampleId :
SOIL-PILE-1-WC-VOC


Tgt Ion:168 Resp: 194802
Ion Ratio Lower Upper
168 100
99 67.0 55.0 82.4

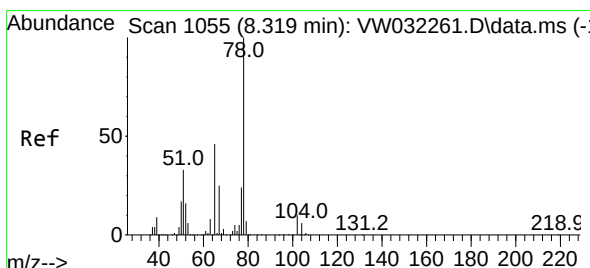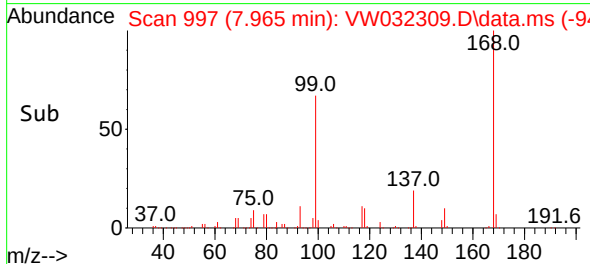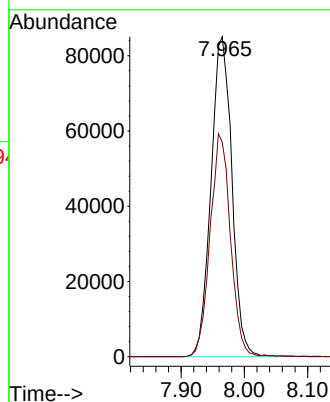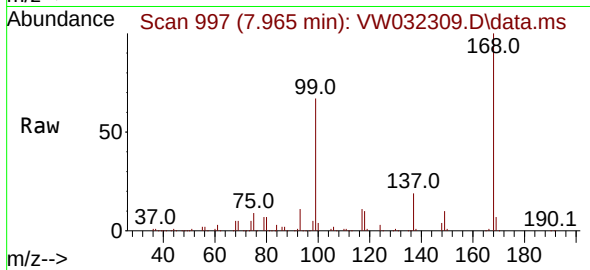

#33
1,2-Dichloroethane-d4
Concen: 58.382 ug/l
RT: 8.319 min Scan# 1055
Delta R.T. -0.000 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26

Tgt Ion: 65 Resp: 179577
Ion Ratio Lower Upper
65 100
67 51.6 0.0 105.8


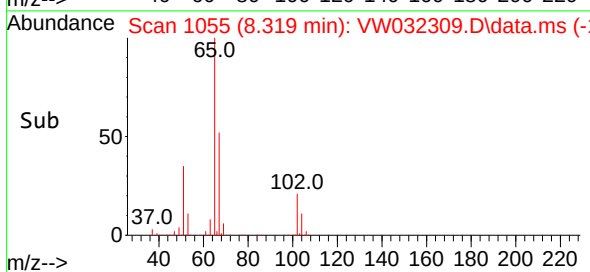
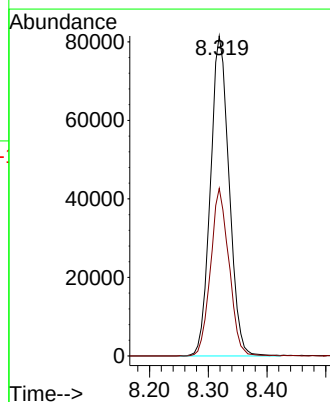
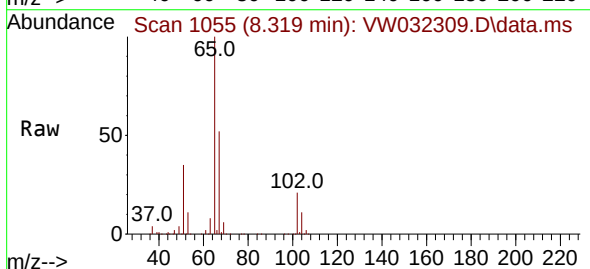


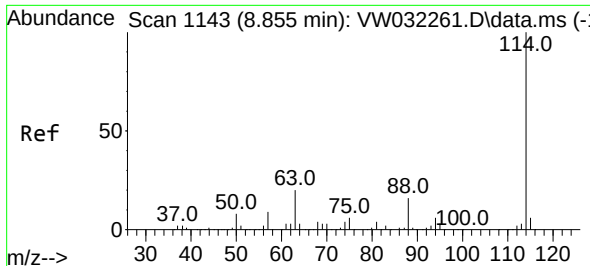

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.849 min Scan# 1143
Delta R.T. -0.006 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26




Instrument :
MSVOA_W
ClientSampleId :
SOIL-PILE-1-WC-VOC


Tgt Ion:114 Resp: 414330
Ion Ratio Lower Upper
114 100
63 22.5 0.0 40.2
88 16.3 0.0 32.0

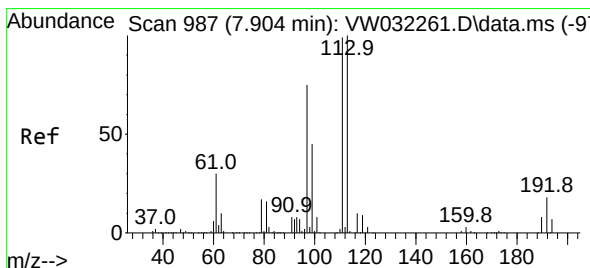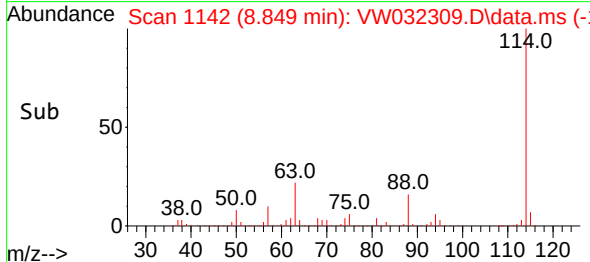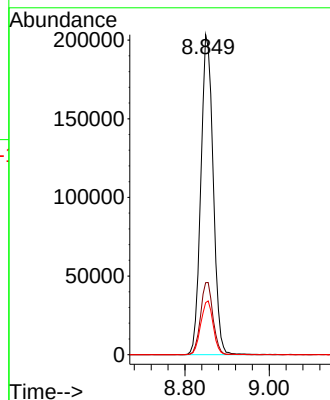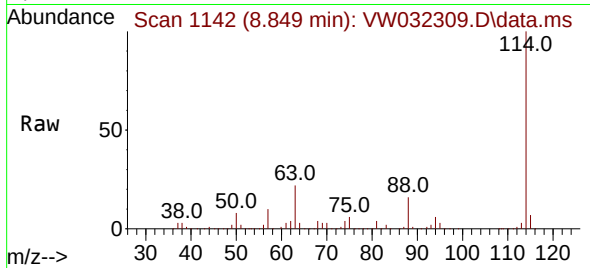

#35
Dibromofluoromethane
Concen: 49.880 ug/l
RT: 7.898 min Scan# 986
Delta R.T. -0.006 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26

Tgt Ion:113 Resp: 148629
Ion Ratio Lower Upper
113 100
111 103.1 81.8 122.8
192 16.4 13.0 19.4


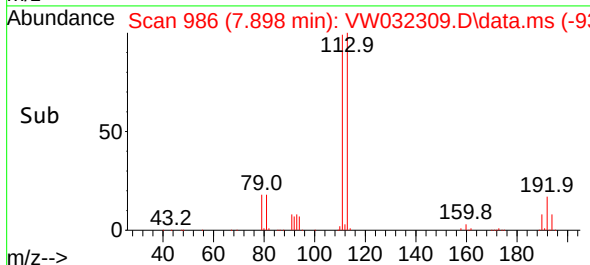
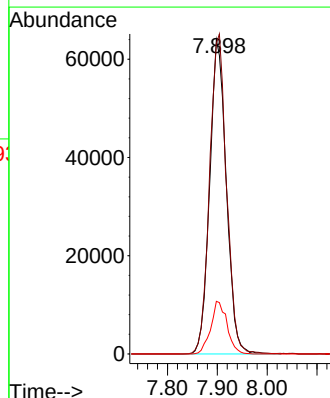
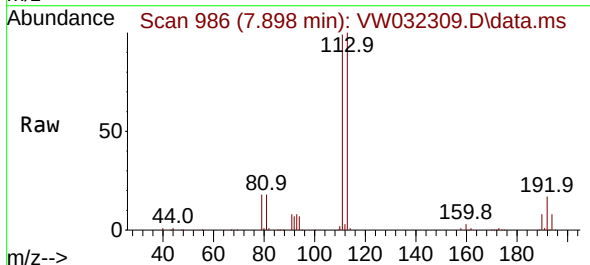


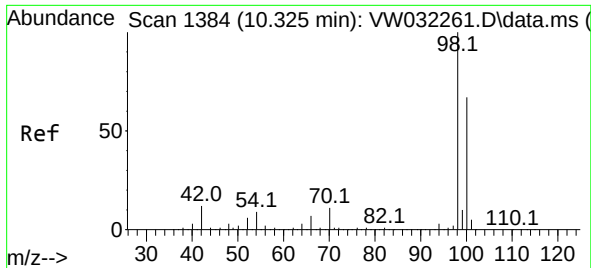

#50
Toluene-d8
Concen: 51.170 ug/l
RT: 10.324 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26




Instrument :
MSVOA_W
ClientSampleId :
SOIL-PILE-1-WC-VOC


Tgt Ion: 98 Resp: 549507
Ion Ratio Lower Upper
98 100
100 66.4 53.0 79.4

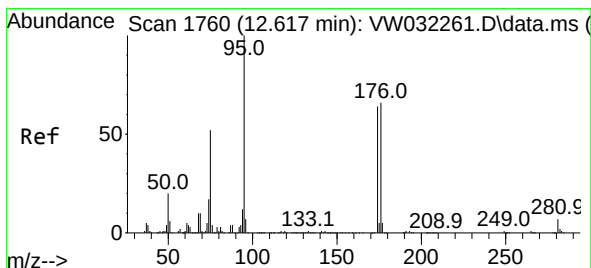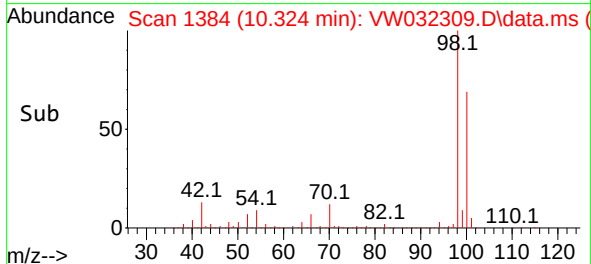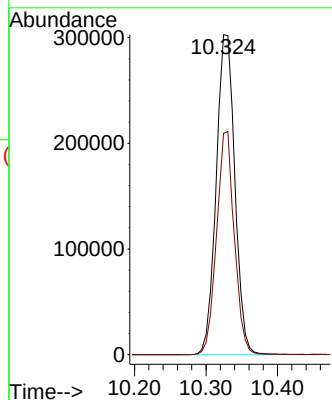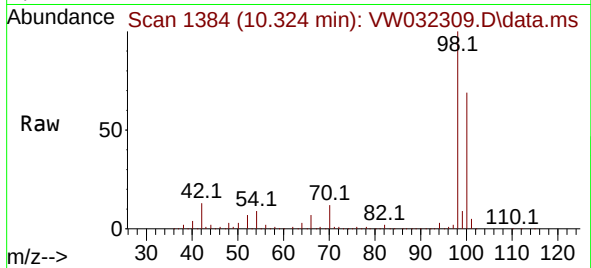

#62
4-Bromofluorobenzene
Concen: 50.321 ug/l
RT: 12.617 min Scan# 1760
Delta R.T. -0.000 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26

Tgt Ion: 95 Resp: 203840
Ion Ratio Lower Upper
95 100
174 67.0 0.0 130.6
176 63.8 0.0 127.0


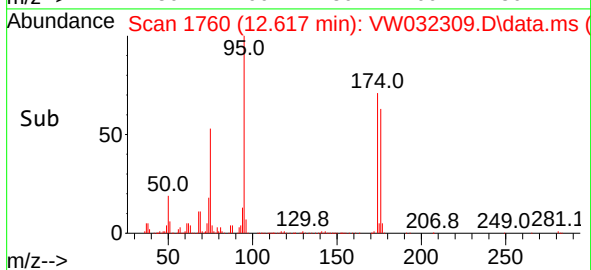
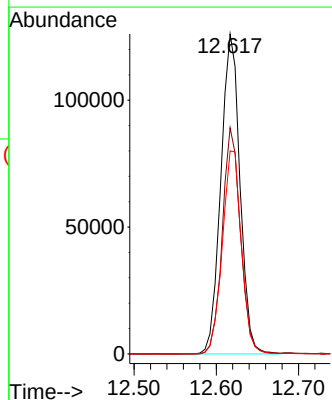
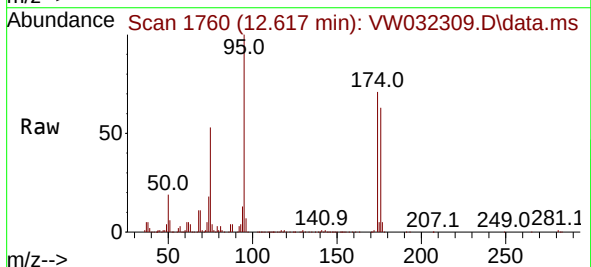


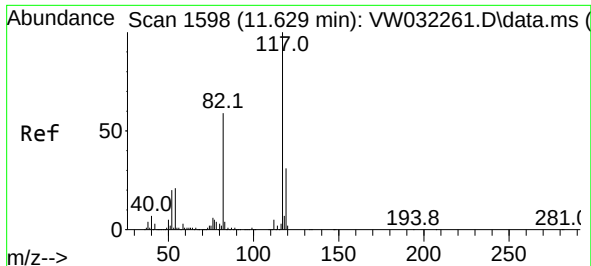

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.629 min Scan# 11
Delta R.T. -0.000 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26

Instrument :
MSVOA_W
ClientSampleId :
SOIL-PILE-1-WC-VOC

Tgt Ion:117 Resp: 425217
Ion Ratio Lower Upper
117 100
82 61.5 46.9 70.3
119 32.8 24.9 37.3

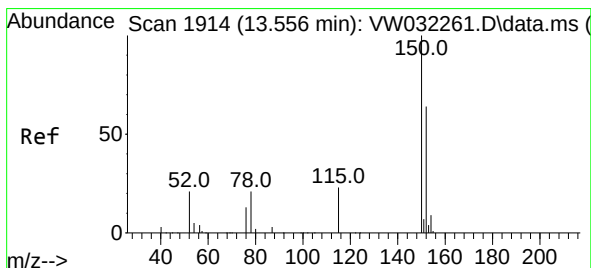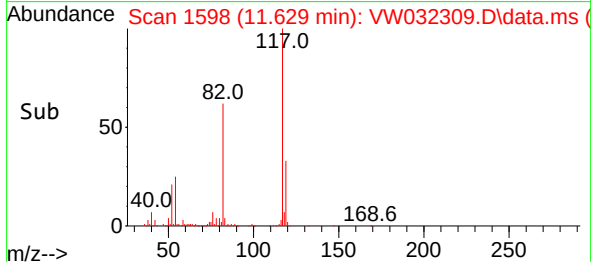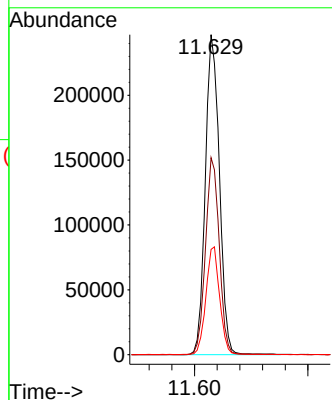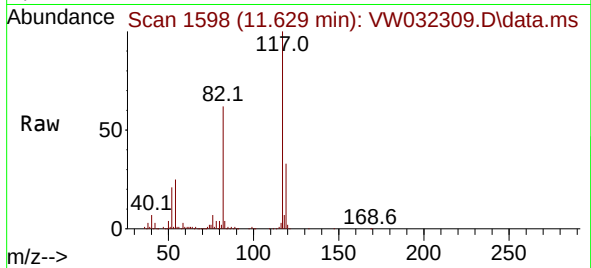

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.556 min Scan# 1914
Delta R.T. -0.000 min
Lab File: VW032309.D
Acq: 30 Sep 2025 17:26

Tgt Ion:152 Resp: 218009
Ion Ratio Lower Upper
152 100
115 65.6 32.5 97.5
150 155.1 0.0 370.2

