

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100124\
 Data File : VW030314.D
 Acq On : 01 Oct 2024 16:32
 Operator : SY/MD
 Sample : P4237-09
 Misc : 5.68g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F23

Quant Time: Oct 02 07:43:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 01 01:01:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	330370	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	278598	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	95504	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	64586	25.018	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	100.080%	
7) Chloroethane-d5	2.893	69	45029	23.973	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	95.880%	
11) 1,1-Dichloroethene-d2	4.021	65	37079	19.676	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	78.720%	
21) 2-Butanone-d5	7.075	46	33235	32.013	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	64.020%	
24) Chloroform-d	7.648	84	167240	18.843	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	75.360%	
26) 1,2-Dichloroethane-d4	8.307	65	88886	19.187	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	76.760%	
32) Benzene-d6	8.276	84	324348	20.772	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	83.080%	
36) 1,2-Dichloropropane-d6	9.276	67	98354	20.943	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	83.760%	
41) Toluene-d8	10.325	98	276628	19.320	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	77.280%	
43) trans-1,3-Dichloroprop...	10.575	79	37330	19.110	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	76.440%	
47) 2-Hexanone-d5	10.922	63	25491	32.870	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	65.740%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	60447	17.225	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	68.880%	
66) 1,2-Dichlorobenzene-d4	13.849	152	61895	19.520	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	78.080%	
Target Compounds					Qvalue	
13) Acetone	4.125	43	8281	7.519	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100124\
Data File : VW030314.D
Acq On : 01 Oct 2024 16:32
Operator : SY/MD
Sample : P4237-09
Misc : 5.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F23

Quant Time: Oct 02 07:43:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 01 01:01:52 2024
Response via : Initial Calibration

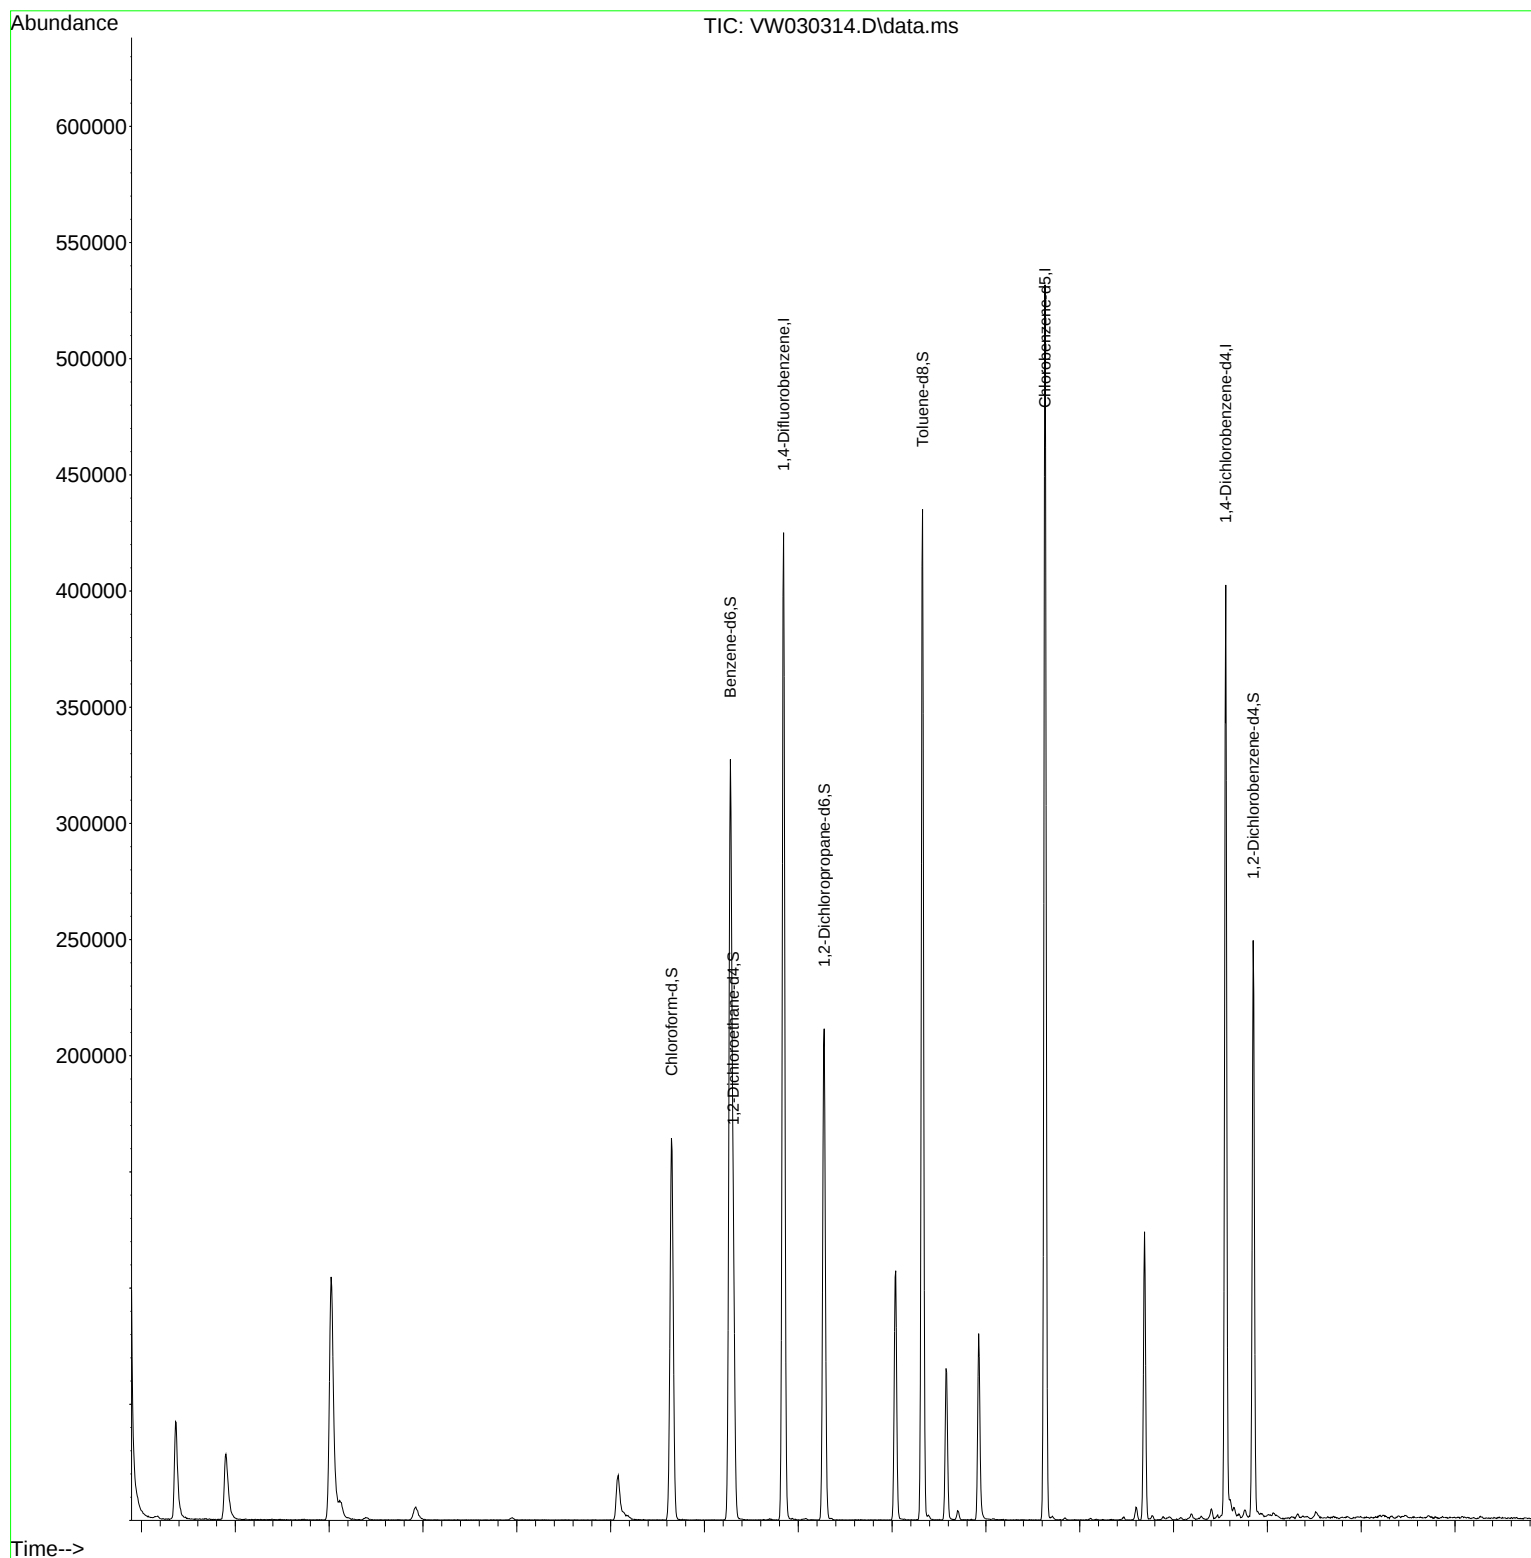

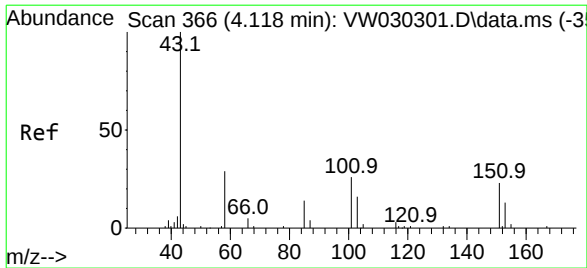

#13
 Acetone
 Concen: 7.519 ug/L
 RT: 4.125 min Scan# 36
 Delta R.T. -0.012 min
 Lab File: VW030314.D
 Acq: 01 Oct 2024 16:32

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F23

Tgt Ion: 43 Resp: 8281
 Ion Ratio Lower Upper
 43 100
 58 32.0 0.0 64.0

