




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
Data File : VW030351.D
Acq On : 03 Oct 2024 02:28
Operator : SY/MD
Sample : P4238-12
Misc : 5.50g/10mL/MSVOA_W/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EY8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/03/2024
Supervised By :Semsettin Yesilyurt 10/03/2024

Quant Time: Oct 03 05:13:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 03 05:10:23 2024
Response via : Initial Calibration

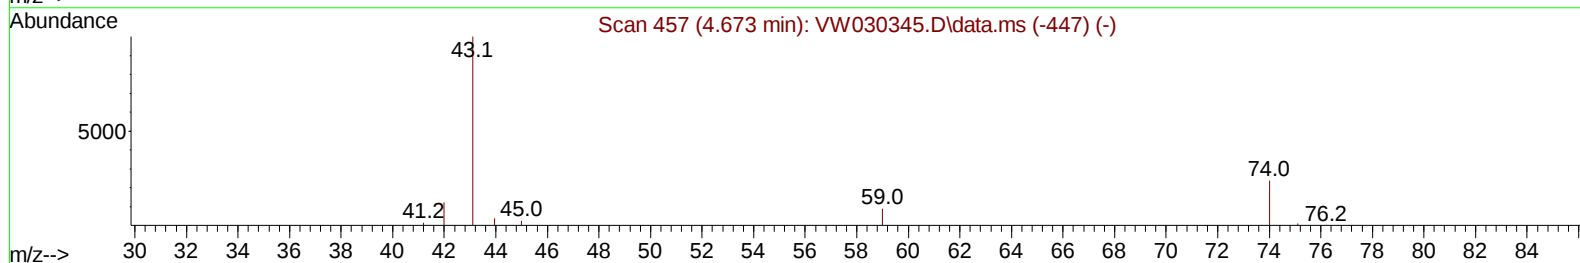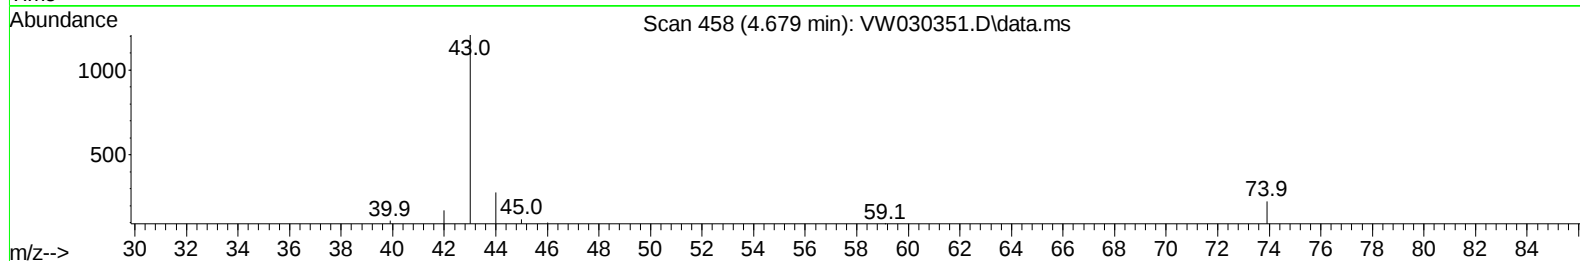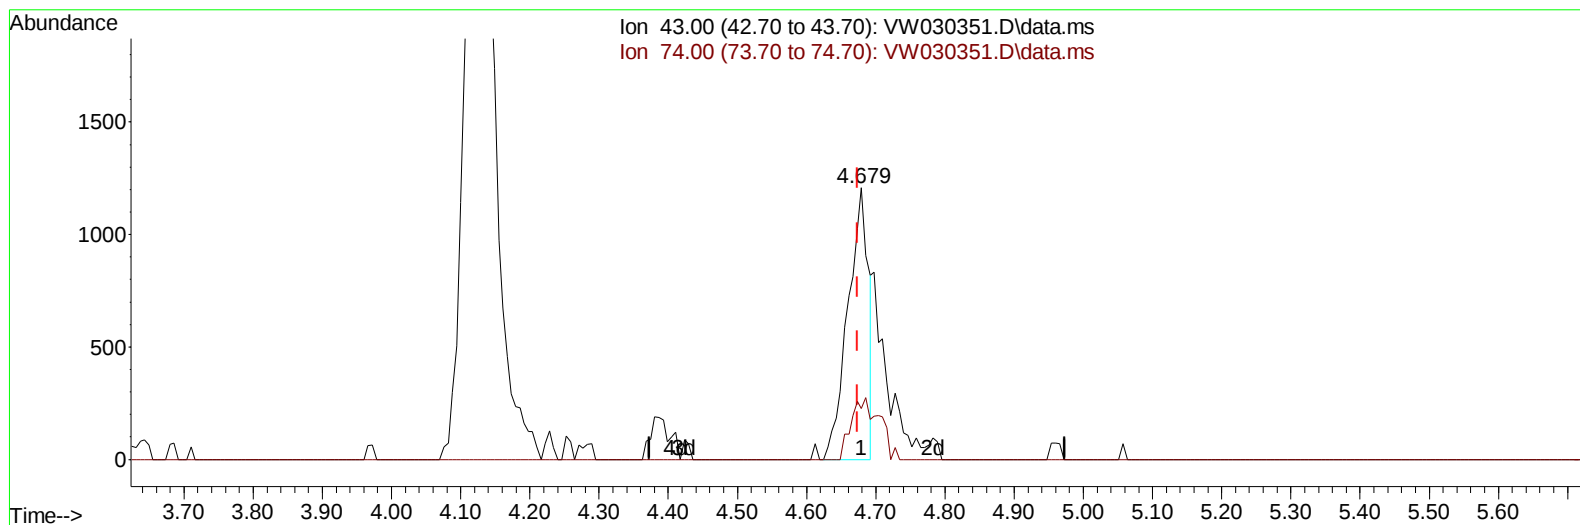

TIC: VW030351.D\data.ms

(15) Methyl Acetate (T)

4.679min (+ 0.006) 1.62 ug/L

response 2471

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.70	20.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
Data File : VW030351.D
Acq On : 03 Oct 2024 02:28
Operator : SY/MD
Sample : P4238-12
Misc : 5.50g/10mL/MSVOA_W/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EY8

Manual IntegrationsAPPROVED

Quant Time: Oct 03 05:13:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 03 05:10:23 2024
Response via : Initial Calibration

Reviewed By :Romaben Patel 10/03/2024
Supervised By :Semsettin Yesilyurt 10/03/2024

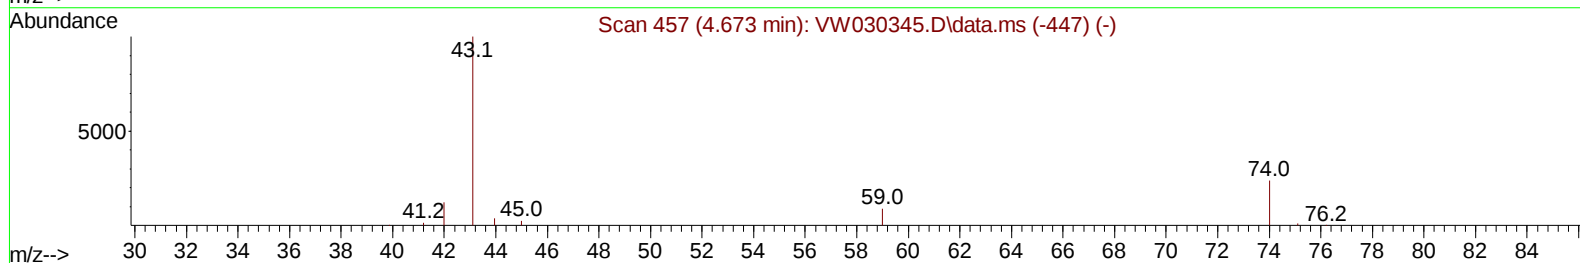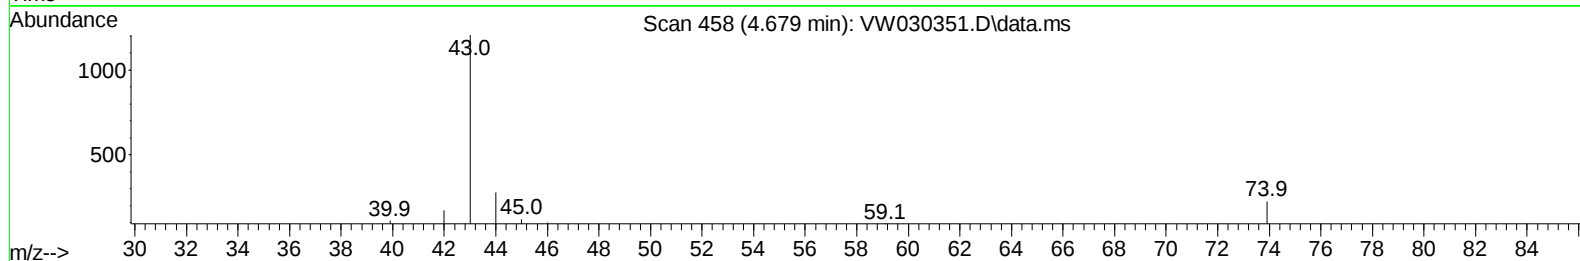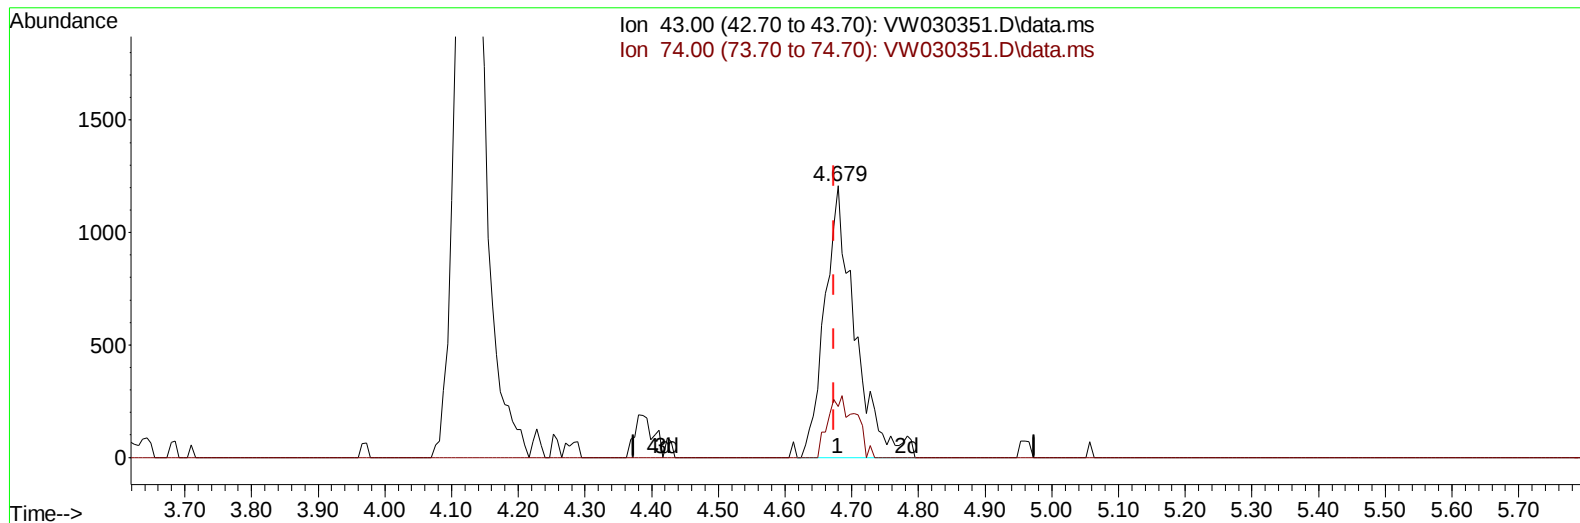

TIC: VW030351.D\data.ms

(15) Methyl Acetate (T)

4.679min (+ 0.006) 2.49 ug/L m

response 3805

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	24.70	13.01#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100224\
 Data File : VW030351.D
 Acq On : 03 Oct 2024 02:28
 Operator : SY/MD
 Sample : P4238-12
 Misc : 5.50g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EY8

Manual IntegrationsAPPROVED

Quant Time: Oct 03 05:13:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 03 05:10:23 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 10/03/2024
 Supervised By :Semsettin Yesilyurt 10/03/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		280706	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		211854	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		74389	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		61396	27.990	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	111.960%	
7) Chloroethane-d5	2.905	69		45303	28.386	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.560%	
11) 1,1-Dichloroethene-d2	4.021	65		35013	21.867	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	87.480%	
21) 2-Butanone-d5	7.081	46		20838	23.623	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	47.240%	
24) Chloroform-d	7.654	84		147733	19.590	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	78.360%	
26) 1,2-Dichloroethane-d4	8.307	65		87518	22.234	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	88.920%	
32) Benzene-d6	8.276	84		276069	23.250	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	9.276	67		90465	25.332	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	101.320%	
41) Toluene-d8	10.325	98		218029	20.025	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	80.080%	
43) trans-1,3-Dichloroprop...	10.581	79		19990	13.457	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	53.840%	
47) 2-Hexanone-d5	10.928	63		13626	23.106	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	46.220%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		62042	23.249	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	13.848	152		44661	18.083	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	72.320%#	
Target Compounds							
13) Acetone	4.131	43		9170	9.800	ug/L	96
15) Methyl Acetate	4.679	43		3805m	2.493	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
Data File : VW030351.D
Acq On : 03 Oct 2024 02:28
Operator : SY/MD
Sample : P4238-12
Misc : 5.50g/10mL/MSVOA_W/SOIL/A
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EY8

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 10/03/2024
Supervised By :Semsettin Yesilyurt 10/03/2024

Quant Time: Oct 03 05:13:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 03 05:10:23 2024
Response via : Initial Calibration

