

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
 Data File : VW030328.D
 Acq On : 02 Oct 2024 15:45
 Operator : SY/MD
 Sample : VIBLK532
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK532

Quant Time: Oct 03 04:11:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 03 04:10:12 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	166388	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	152381	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	70389	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.369	65	37912	29.159	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.640%	
7) Chloroethane-d5		2.905	69	28993	30.647	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.600%	
11) 1,1-Dichloroethene-d2		4.027	65	23671	24.941	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	99.760%	
21) 2-Butanone-d5		7.075	46	26625	50.921	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.840%	
24) Chloroform-d		7.655	84	106480	23.821	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.280%	
26) 1,2-Dichloroethane-d4		8.307	65	60042	25.734	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.920%	
32) Benzene-d6		8.276	84	208093	24.365	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.480%	
36) 1,2-Dichloropropane-d6		9.276	67	64383	25.064	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.240%	
41) Toluene-d8		10.325	98	185641	23.705	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	94.800%	
43) trans-1,3-Dichloroprop...		10.575	79	24609	23.033	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.120%	
47) 2-Hexanone-d5		10.922	63	20904	49.282	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.560%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	48628	25.335	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.320%	
66) 1,2-Dichlorobenzene-d4		13.849	152	61448	26.294	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.160%	
Target Compounds							Qvalue
16) Methylene chloride		4.923	84	10483	4.093	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
Data File : VW030328.D
Acq On : 02 Oct 2024 15:45
Operator : SY/MD
Sample : VIBLK532
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK532


Quant Time: Oct 03 04:11:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 03 04:10:12 2024
Response via : Initial Calibration

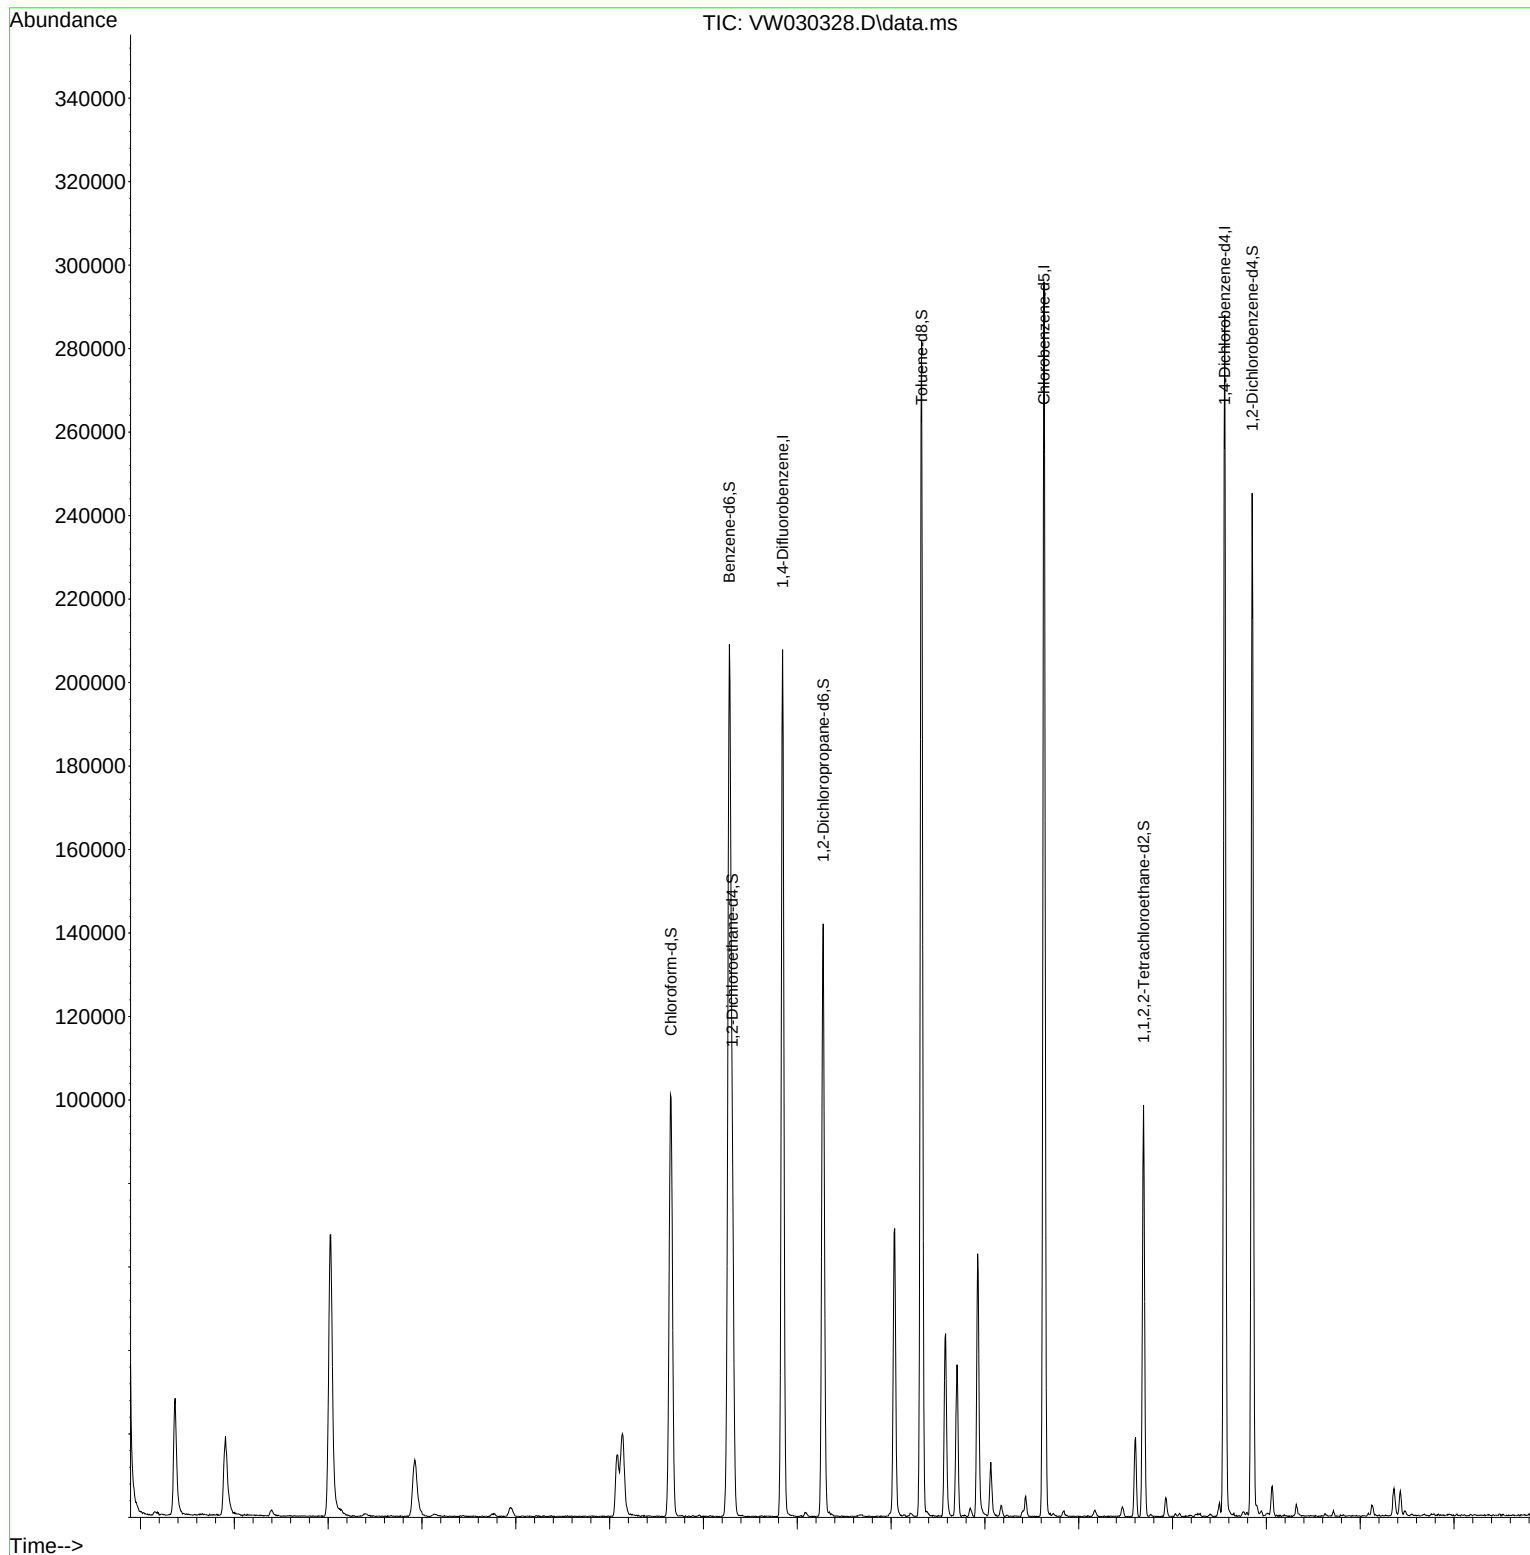

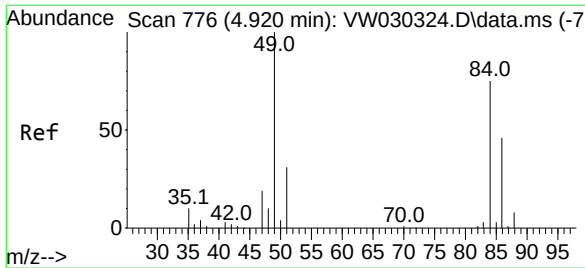

#16
Methylene chloride
Concen: 4.093 ug/L
RT: 4.923 min Scan# 49
Delta R.T. 0.004 min
Lab File: VW030328.D
Acq: 02 Oct 2024 15:45

Instrument :
MSVOA_W
ClientSampleId :
VIBLK532

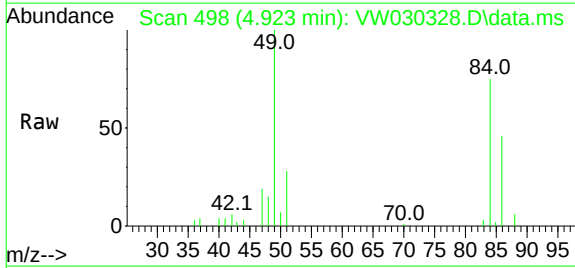

Tgt Ion:	84	Resp:	10483
Ion	Ratio	Lower	Upper
84	100		
86	61.1	44.8	83.2
49	134.1	83.6	155.2

