

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
 Data File : VW030335.D
 Acq On : 02 Oct 2024 18:29
 Operator : SY/MD
 Sample : P4237-16RE
 Misc : 5.63g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EN9RE

Quant Time: Oct 03 04:13:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 03 04:10:12 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	240964	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	163110	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	37264	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	56654	30.088	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	120.360%	
7) Chloroethane-d5		2.905	69	39087	28.530	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	114.120%	
11) 1,1-Dichloroethene-d2		4.021	65	30761	22.380	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.520%	
21) 2-Butanone-d5		7.081	46	30772	40.638	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.280%	
24) Chloroform-d		7.654	84	125375	19.367	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.480%	
26) 1,2-Dichloroethane-d4		8.307	65	71217	21.077	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.320%	
32) Benzene-d6		8.276	84	241229	26.387	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.560%	
36) 1,2-Dichloropropane-d6		9.276	67	76208	27.716	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.880%	
41) Toluene-d8		10.325	98	183079	21.840	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	87.360%	
43) trans-1,3-Dichloroprop...		10.575	79	26378	23.065	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.240%	
47) 2-Hexanone-d5		10.922	63	22664	49.917	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.840%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	40768	19.842	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	79.360%	
66) 1,2-Dichlorobenzene-d4		13.848	152	21757	17.586	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	70.360%#	
Target Compounds							
13) Acetone		4.125	43	10528	13.107	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
Data File : VW030335.D
Acq On : 02 Oct 2024 18:29
Operator : SY/MD
Sample : P4237-16RE
Misc : 5.63g/10mL/MSVOA_W/SOIL/B
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EN9RE

Quant Time: Oct 03 04:13:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 03 04:10:12 2024
Response via : Initial Calibration

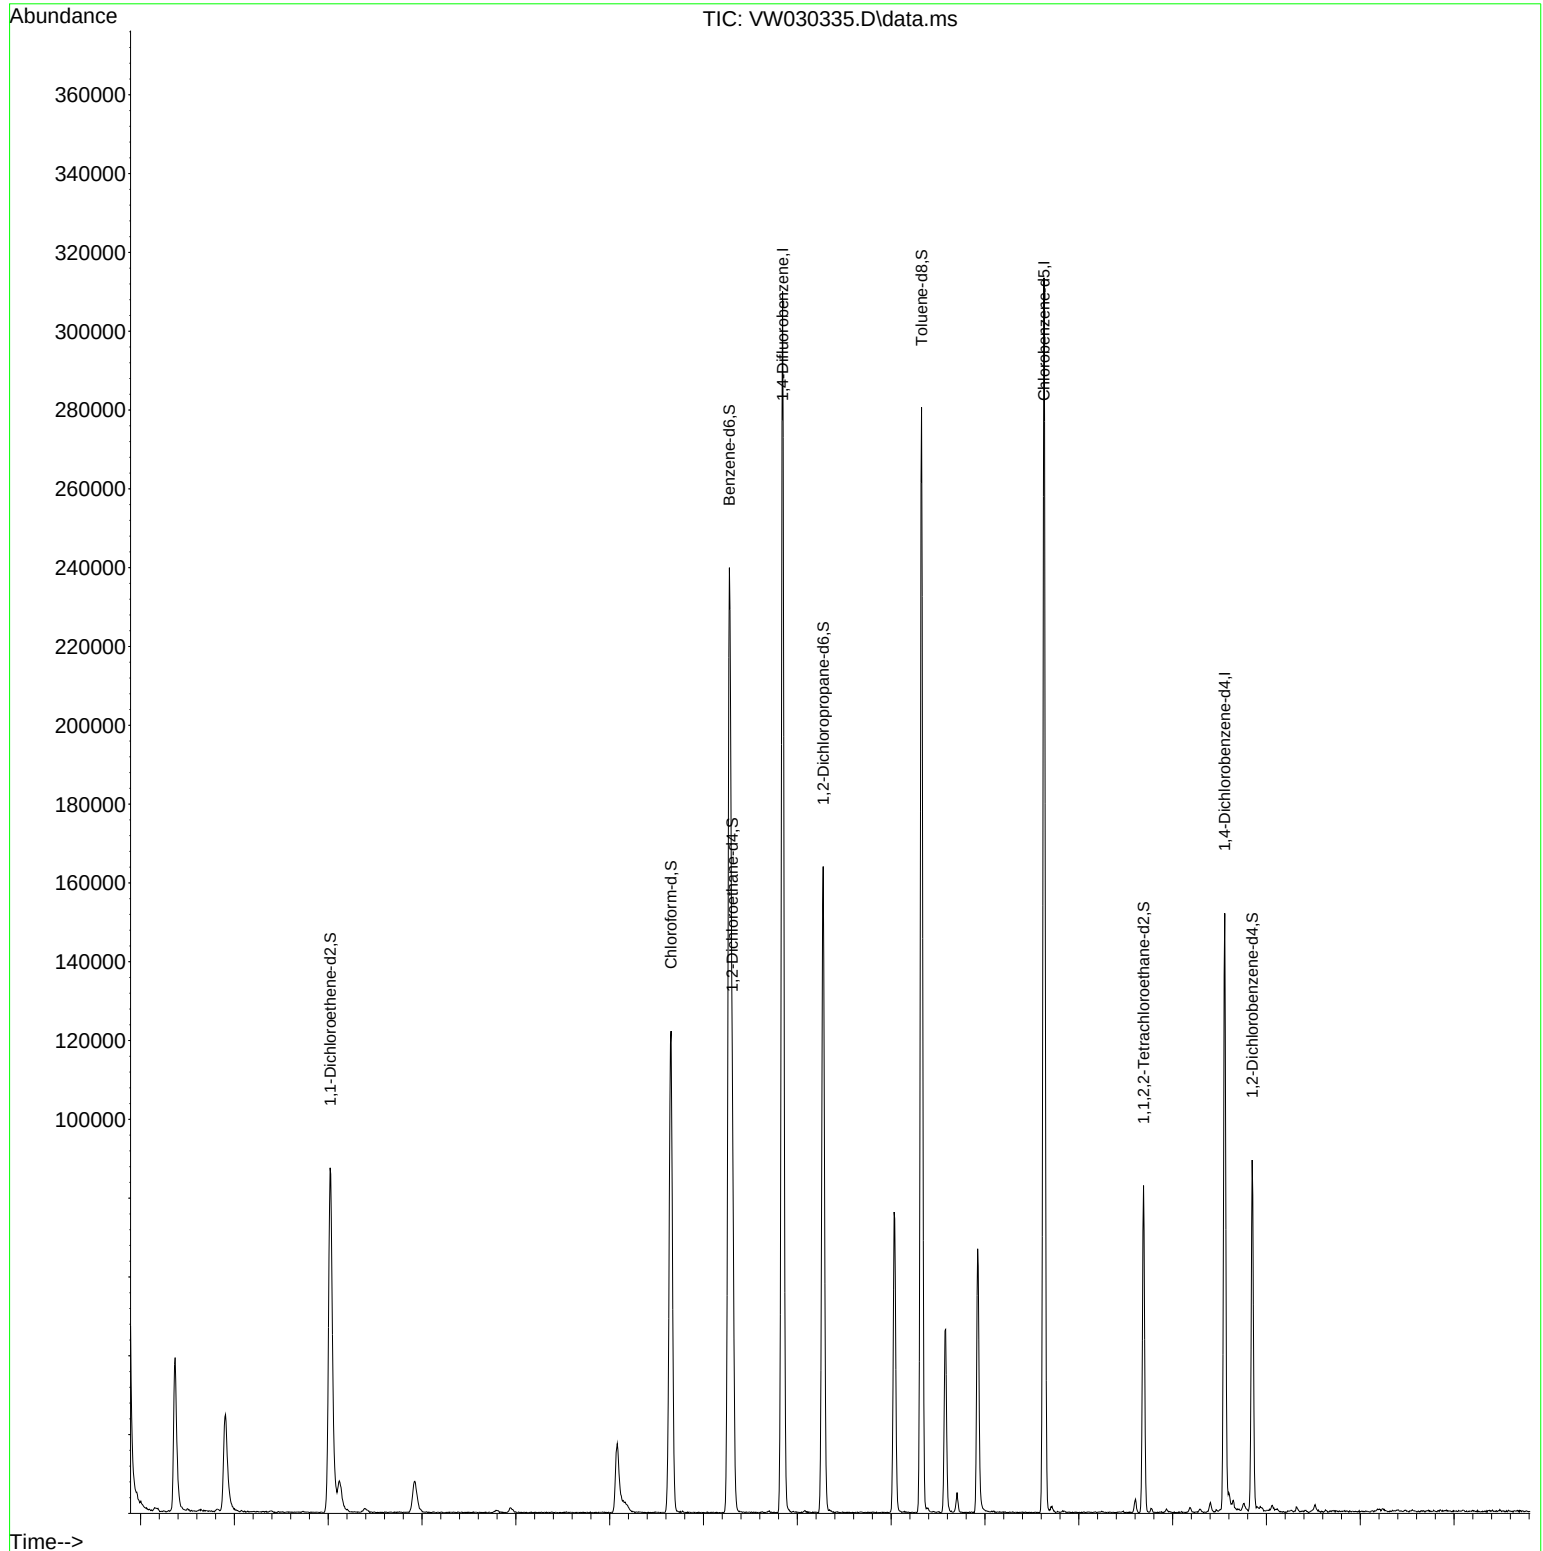

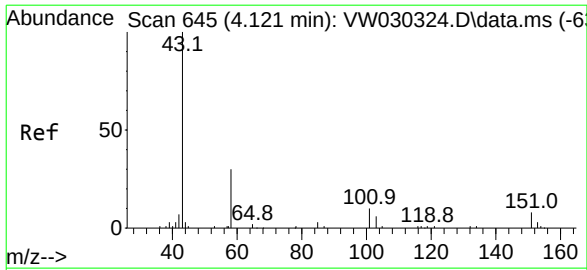

#13
 Acetone
 Concen: 13.107 ug/L
 RT: 4.125 min Scan# 36
 Delta R.T. 0.003 min
 Lab File: VW030335.D
 Acq: 02 Oct 2024 18:29

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EN9RE

Tgt Ion: 43 Resp: 10528
 Ion Ratio Lower Upper
 43 100
 58 30.1 0.0 64.0

