
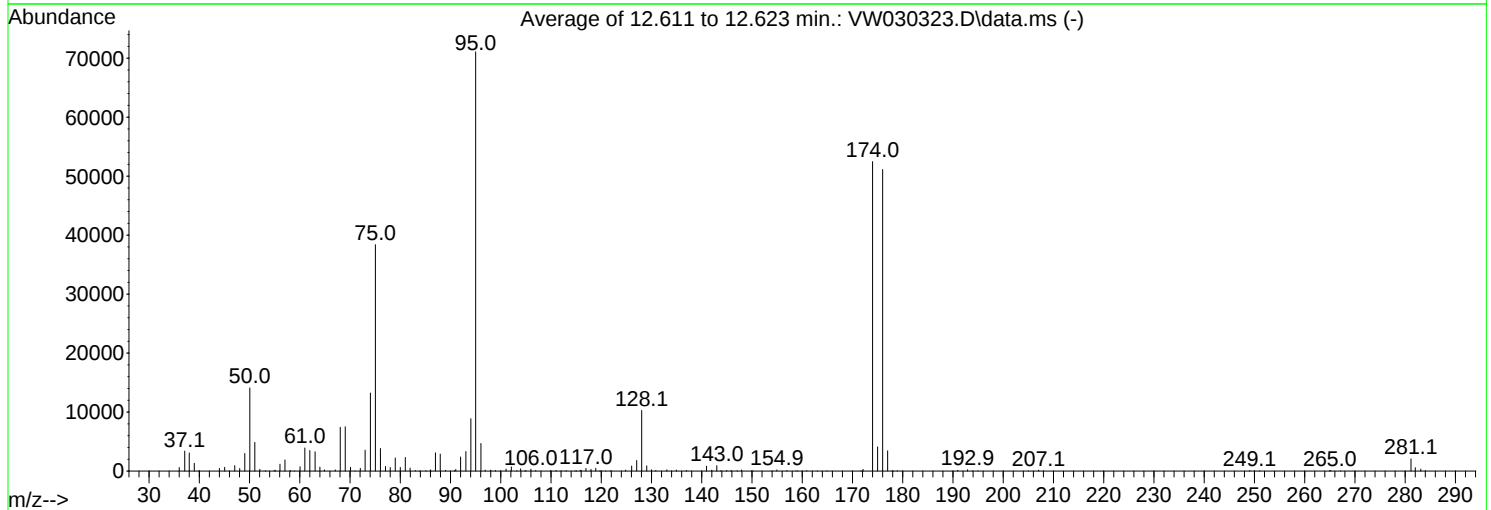


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100224\
Data File : VW030323.D
Acq On : 02 Oct 2024 12:58
Operator : SY/MD
Sample : BFB567
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB567

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Title : SFAM01.0
Last Update : Fri Oct 04 01:05:34 2024

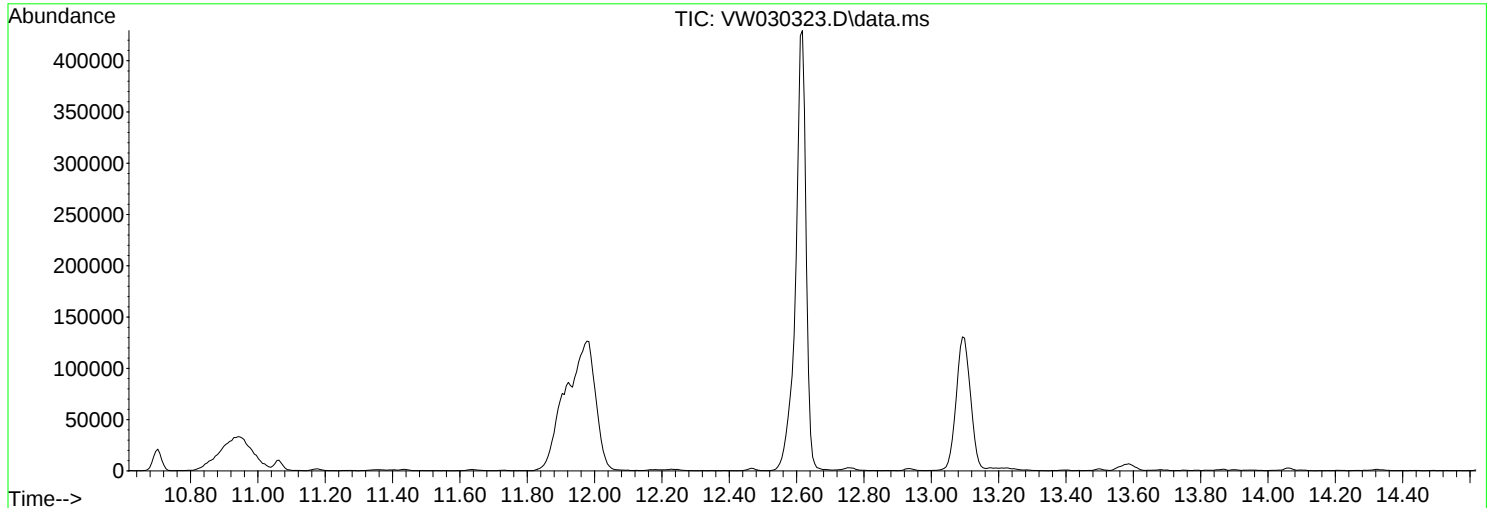

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1752

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	14101	PASS
75	95	30	80	54.0	38386	PASS
95	95	100	100	100.0	71096	PASS
96	95	5	9	6.6	4690	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	52467	PASS
175	174	5	9	7.8	4102	PASS
176	174	95	101	97.5	51131	PASS
177	176	5	9	6.7	3438	PASS

m/z	Abundance
35.90	58.0
36.90	53.0
38.00	177.0
39.00	418.0
39.90	115.0
42.90	57.0
44.00	67.0
49.10	85.0
50.00	892.0
51.10	1450.0
52.00	235.0
60.90	182.0
62.00	534.0
63.00	1169.0
64.00	1125.0
72.90	87.0
74.00	758.0
75.00	923.0
76.00	515.0
77.10	606.0
78.00	454.0
85.20	96.0
86.10	241.0
87.10	316.0
89.10	168.0
96.90	70.0
98.00	307.0
98.90	152.0
99.90	123.0
101.10	370.0
102.10	1660.0
103.20	176.0
124.70	51.0
126.10	1140.0
127.00	2016.0
128.10	15929.0
129.10	1953.0
130.00	139.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567

m/z	Abundance
36.00	699.0
37.10	3526.0
38.00	3489.0
39.10	2090.0
40.10	219.0
43.10	83.0
44.00	533.0
45.00	670.0
47.00	1055.0
48.00	407.0
49.00	3053.0
50.10	16488.0
51.10	7385.0
52.10	691.0
53.20	123.0
54.90	187.0
56.10	1159.0
57.00	2028.0
58.20	60.0
58.90	101.0
60.10	898.0
61.00	4379.0
62.00	4238.0
63.10	4810.0
64.00	2408.0
64.90	270.0
67.10	260.0
68.10	7452.0
69.10	7426.0
70.10	557.0
72.00	586.0
73.10	3652.0
74.10	15639.0
75.10	42424.0
76.10	4885.0
77.10	1778.0
78.00	1359.0
79.00	2322.0
80.00	682.0
81.00	2252.0
81.90	495.0
83.10	108.0
83.90	51.0
85.00	233.0
86.00	638.0
87.00	3758.0
87.90	2819.0
89.00	284.0
90.80	235.0
91.10	240.0
92.00	2432.0
93.10	3311.0
94.10	8760.0
95.00	71160.0
96.10	4584.0
97.00	297.0
98.10	609.0
99.00	359.0
100.10	186.0
101.10	1041.0
102.10	3123.0
103.20	256.0
104.00	333.0
104.80	138.0
106.00	292.0
106.90	106.0
110.00	115.0
111.00	103.0
113.10	103.0
115.10	89.0
115.80	224.0
117.00	534.0
118.00	323.0
118.90	449.0
119.70	57.0
120.90	95.0
121.90	84.0
124.90	303.0
126.00	2753.0
127.10	5066.0
128.10	34968.0
129.10	3655.0
130.00	366.0
130.80	99.0
133.10	405.0
134.00	63.0
135.00	180.0
137.00	86.0
140.90	802.0
142.00	193.0
143.00	883.0
143.80	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567

145.00	117.0
145.80	97.0
147.10	72.0
147.90	166.0
154.00	57.0
155.00	237.0
156.90	75.0
158.80	54.0
161.00	99.0
163.00	103.0
164.90	76.0
171.70	214.0
172.20	271.0
174.00	49536.0
175.00	3759.0
176.00	48664.0
177.00	3629.0
178.90	134.0
191.00	327.0
192.90	377.0
195.00	72.0
205.00	103.0
207.00	249.0
208.00	67.0
249.10	203.0
251.10	71.0
265.00	287.0
267.20	63.0
281.10	3299.0
282.00	905.0
283.10	533.0
284.10	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567

m/z	Abundance
36.00	737.0
37.10	3847.0
38.10	3752.0
39.00	1763.0
40.00	192.0
43.10	77.0
44.00	549.0
45.10	655.0
47.10	1024.0
48.10	540.0
49.00	3377.0
50.10	15741.0
51.10	6661.0
52.10	588.0
53.20	80.0
55.10	280.0
56.00	1378.0
57.00	2038.0
58.10	140.0
60.00	770.0
61.10	4618.0
62.10	4493.0
63.10	4894.0
64.00	1874.0
64.90	207.0
67.00	241.0
68.10	8110.0
69.00	8730.0
70.10	850.0
71.00	57.0
72.00	375.0
73.00	3982.0
74.10	14202.0
75.10	41448.0
76.10	4477.0
77.00	1342.0
78.10	1113.0
79.00	2438.0
80.00	627.0
81.00	2662.0
82.00	606.0
82.90	90.0
83.90	62.0
85.10	203.0
86.20	413.0
87.00	3546.0
88.00	3435.0
88.90	337.0
91.10	365.0
92.00	2462.0
93.00	3724.0
94.10	9999.0
95.00	79504.0
96.00	5060.0
96.90	242.0
98.10	442.0
99.00	213.0
100.00	192.0
101.00	713.0
102.10	2285.0
103.20	291.0
104.00	406.0
105.00	151.0
106.00	444.0
107.00	75.0
109.90	63.0
110.90	95.0
112.10	54.0
112.90	115.0
115.00	113.0
116.00	351.0
116.90	389.0
117.90	348.0
118.90	646.0
119.90	54.0
121.90	107.0
124.90	206.0
126.10	1718.0
127.10	3607.0
128.10	25192.0
129.10	3179.0
130.00	449.0
130.90	94.0
132.90	208.0
134.90	188.0
136.90	115.0
141.00	910.0
142.00	170.0
143.00	1113.0
143.80	83.0
145.00	160.0
145.90	144.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567

147.00	67.0
147.90	266.0
150.20	53.0
154.90	222.0
156.90	119.0
158.70	50.0
159.20	58.0
160.80	103.0
164.90	55.0
172.10	290.0
174.00	58240.0
175.00	4631.0
176.00	51304.0
177.00	3511.0
177.90	143.0
178.90	75.0
190.90	113.0
192.90	232.0
193.90	50.0
195.00	52.0
207.10	157.0
249.00	87.0
250.00	64.0
251.00	75.0
265.20	189.0
267.00	57.0
281.20	2096.0
282.00	537.0
283.10	311.0
284.10	67.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567

m/z	Abundance
36.10	562.0
37.10	2803.0
38.00	2533.0
39.00	1381.0
40.10	191.0
44.00	481.0
45.00	572.0
46.00	68.0
47.00	714.0
48.10	376.0
49.10	2795.0
50.10	12749.0
51.00	4890.0
52.00	330.0
55.10	215.0
56.10	942.0
57.10	1610.0
58.20	88.0
60.00	562.0
61.10	3289.0
62.10	3356.0
63.10	3627.0
64.10	1121.0
65.00	129.0
67.10	141.0
68.00	6731.0
69.10	6393.0
70.10	516.0
72.10	394.0
73.10	3281.0
74.10	12151.0
75.10	34056.0
76.10	3673.0
77.10	1031.0
78.10	702.0
79.00	1904.0
80.00	557.0
81.00	2021.0
81.90	448.0
82.90	51.0
85.10	81.0
86.10	353.0
87.00	2928.0
88.00	2390.0
89.00	256.0
91.00	219.0
92.00	2290.0
93.00	2923.0
94.00	7891.0
95.00	62624.0
96.00	4426.0
97.00	178.0
98.00	382.0
99.10	168.0
99.90	109.0
101.10	375.0
102.10	1731.0
103.20	187.0
103.90	384.0
105.00	140.0
106.00	252.0
107.00	105.0
110.00	51.0
111.10	128.0
111.90	60.0
113.00	70.0
114.80	98.0
115.80	195.0
116.90	453.0
117.90	241.0
119.00	336.0
121.90	64.0
125.00	149.0
126.10	1517.0
127.10	2768.0
128.10	18472.0
129.10	1691.0
129.90	261.0
130.80	93.0
133.10	79.0
134.90	169.0
137.00	173.0
141.00	784.0
142.00	105.0
143.00	753.0
143.80	67.0
144.80	54.0
145.90	104.0
147.00	83.0
147.90	140.0
149.90	76.0
154.90	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567

157.00	122.0
159.00	56.0
172.00	299.0
174.00	49624.0
175.00	3915.0
176.00	53424.0
177.00	3175.0
178.10	98.0
193.00	79.0
206.90	60.0
265.00	126.0
281.00	839.0
282.10	288.0
283.10	164.0
284.00	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB567