




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100323\
Data File : VW027198.D
Acq On : 03 Oct 2023 13:56
Operator : SY/MD
Sample : 04707-04
Misc : 4.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY1A3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/04/2023
Supervised By :Mahesh Dadoda 10/04/2023

Quant Time: Oct 04 01:39:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 01:37:43 2023
Response via : Initial Calibration

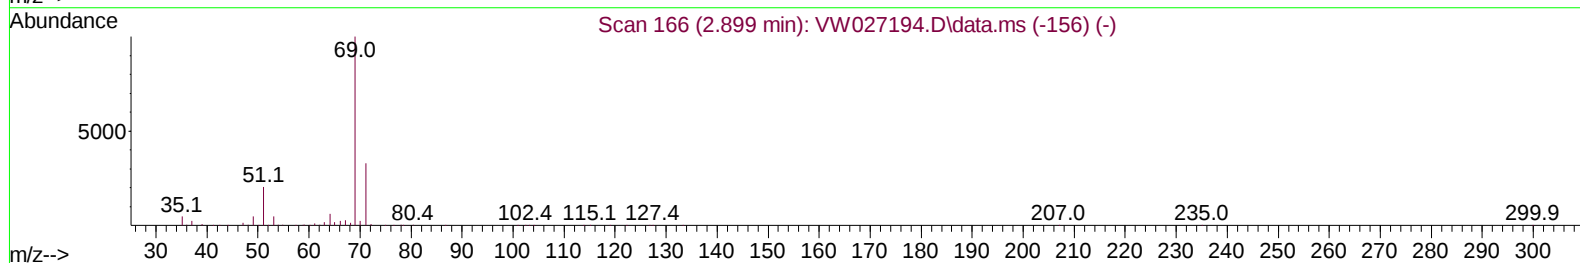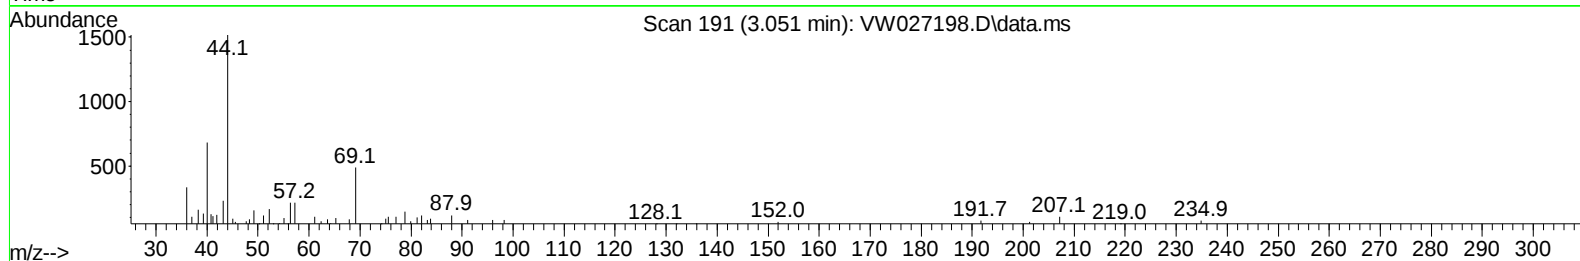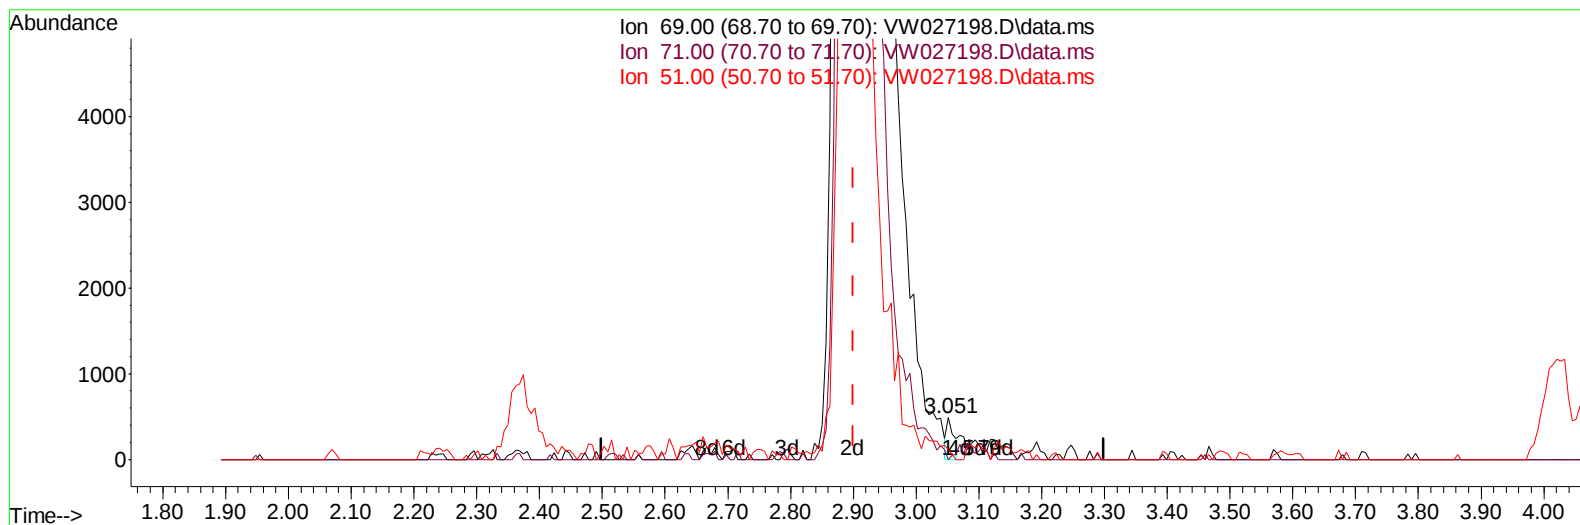

TIC: VW027198.D\data.ms

(7) Chloroethane-d5 (S)

3.051min (+ 0.152) 0.03 ug/L

response 374

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.60	27.27
51.00	25.20	32.35
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100323\
 Data File : VW027198.D
 Acq On : 03 Oct 2023 13:56
 Operator : SY/MD
 Sample : 04707-04
 Misc : 4.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY1A3

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:39:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 01:37:43 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/04/2023
 Supervised By :Mahesh Dadoda 10/04/2023

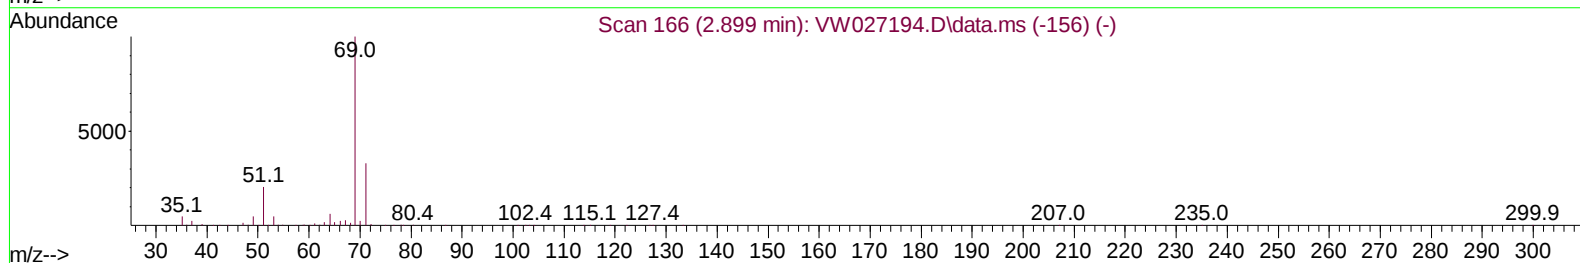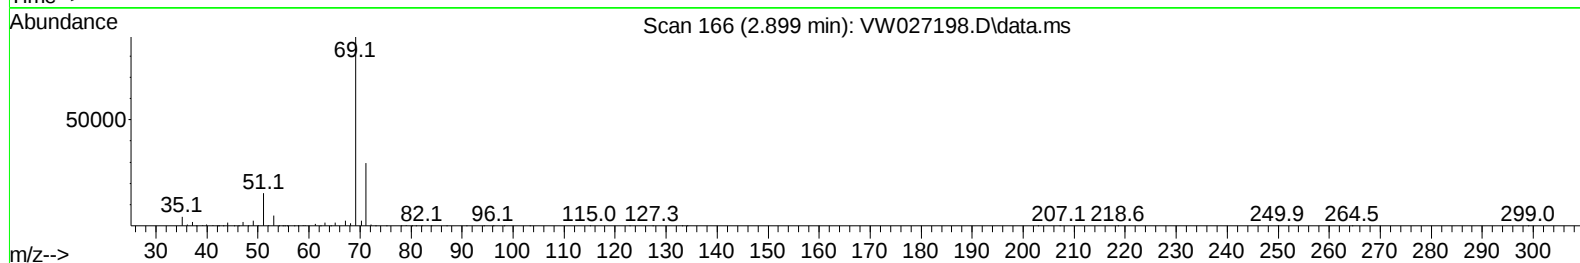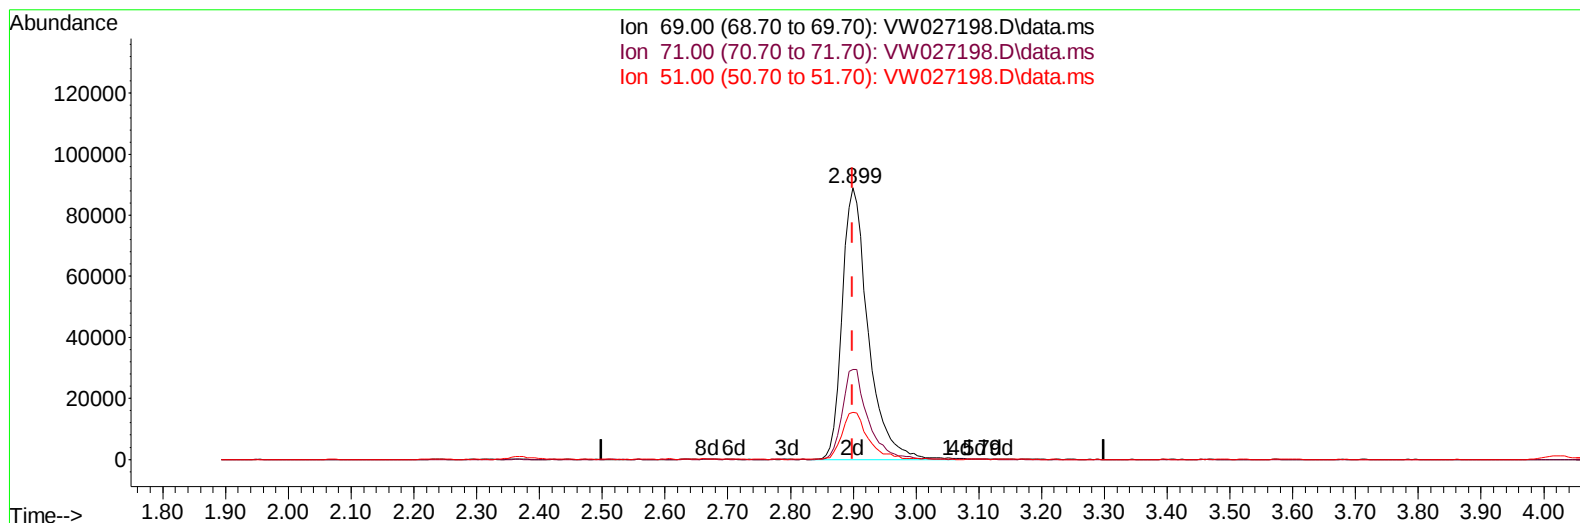

TIC: VW027198.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.000) 22.55 ug/L m

response 256346

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.60	0.04#
51.00	25.20	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100323\
 Data File : VW027198.D
 Acq On : 03 Oct 2023 13:56
 Operator : SY/MD
 Sample : 04707-04
 Misc : 4.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY1A3

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:39:18 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 01:37:43 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/04/2023
 Supervised By :Mahesh Dadoda 10/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	915263	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	871454	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	451619	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	326276	22.689	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	90.760%	
7) Chloroethane-d5	2.899	69	256346m	22.555	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	90.200%	
11) 1,1-Dichloroethene-d2	4.021	65	136005	22.764	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	91.040%	
21) 2-Butanone-d5	7.075	46	143886	48.401	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.800%	
24) Chloroform-d	7.648	84	589947	22.024	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.080%	
26) 1,2-Dichloroethane-d4	8.307	65	299800	23.354	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.400%	
32) Benzene-d6	8.276	84	1255519	23.508	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	94.040%	
36) 1,2-Dichloropropane-d6	9.276	67	382509	23.923	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	95.680%	
41) Toluene-d8	10.318	98	1098298	23.304	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	93.200%	
43) trans-1,3-Dichloroprop...	10.574	79	154091	24.557	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	98.240%	
47) 2-Hexanone-d5	10.922	63	122887	50.241	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.480%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	290913	23.774	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	95.080%	
66) 1,2-Dichlorobenzene-d4	13.854	152	378348	24.986	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	99.960%	
Target Compounds						
16) Methylene chloride	4.923	84	102566	5.725	ug/L	97
22) 2-Butanone	7.179	43	13716	3.019	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100323\
Data File : VW027198.D
Acq On : 03 Oct 2023 13:56
Operator : SY/MD
Sample : 04707-04
Misc : 4.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY1A3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/04/2023
Supervised By :Mahesh Dadoda 10/04/2023

Quant Time: Oct 04 01:39:18 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 01:37:43 2023
Response via : Initial Calibration

