




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100323\
Data File : VW027204.D
Acq On : 03 Oct 2023 16:19
Operator : SY/MD
Sample : 04707-01
Misc : 4.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY1A2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 10/04/2023
Supervised By :Mahesh Dadoda 10/04/2023

Quant Time: Oct 04 01:40:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 01:37:43 2023
Response via : Initial Calibration

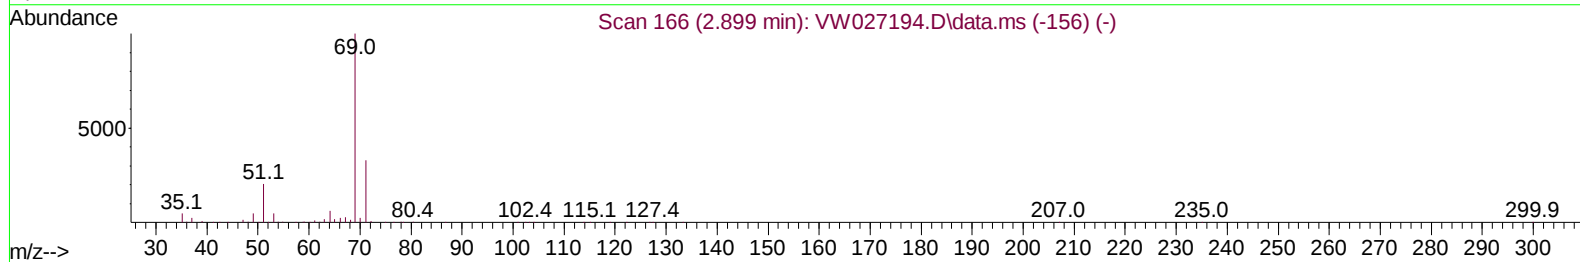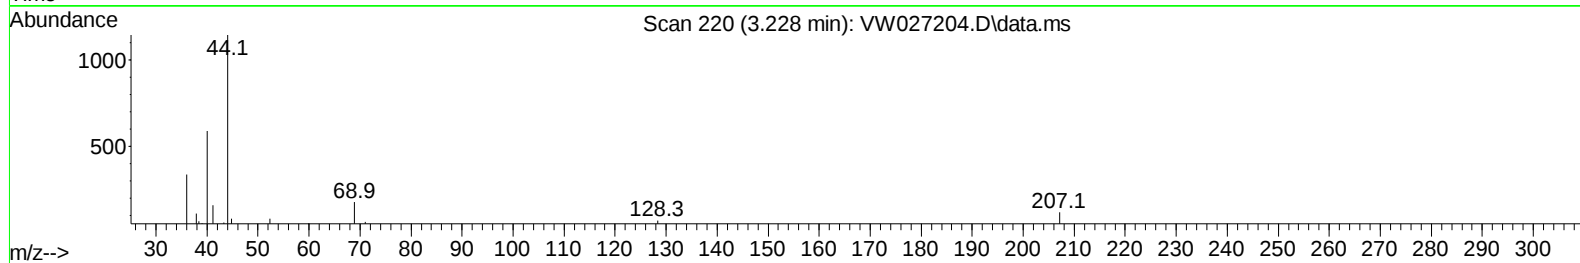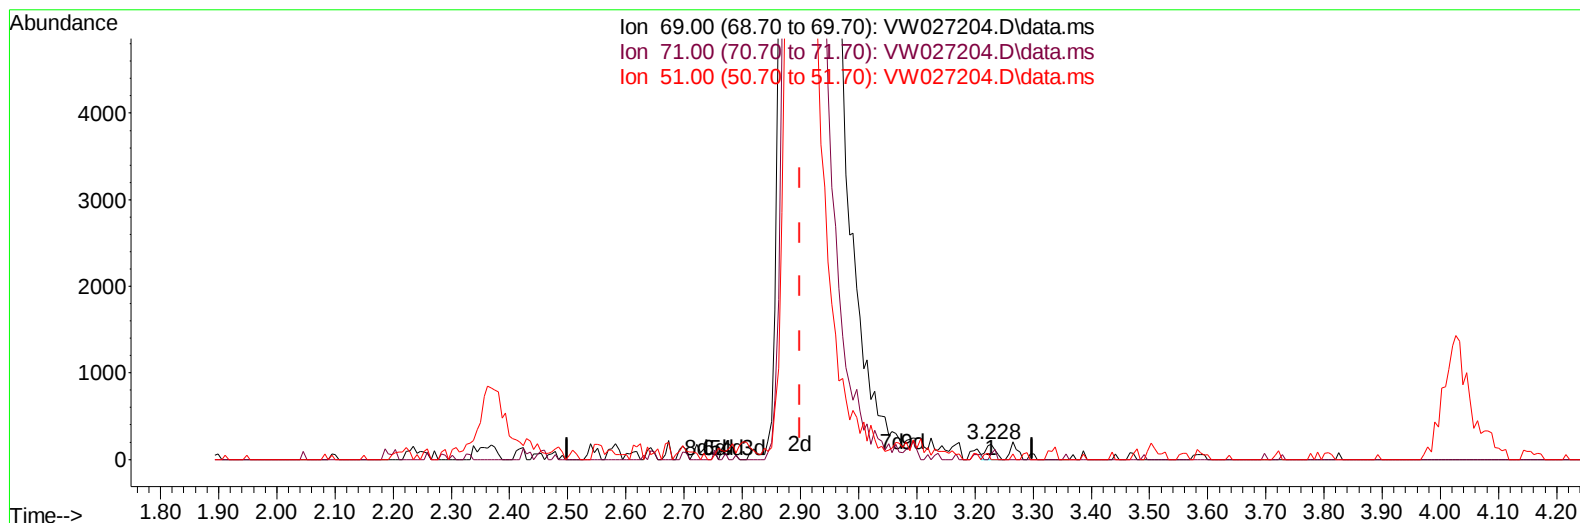

TIC: VW027204.D\data.ms

(7) Chloroethane-d5 (S)

3.228min (+ 0.329) 0.02 ug/L

response 206

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.60	31.55
51.00	25.20	22.33
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100323\
 Data File : VW027204.D
 Acq On : 03 Oct 2023 16:19
 Operator : SY/MD
 Sample : 04707-01
 Misc : 4.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY1A2

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:40:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 01:37:43 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/04/2023
 Supervised By :Mahesh Dadoda 10/04/2023

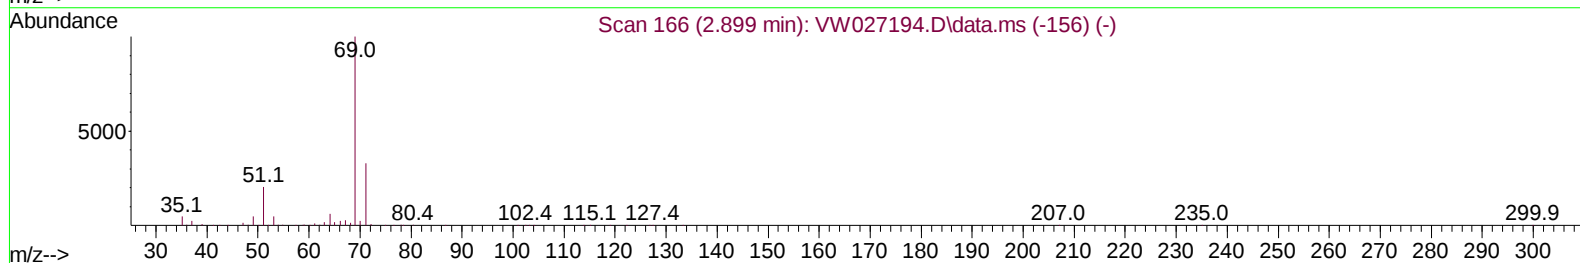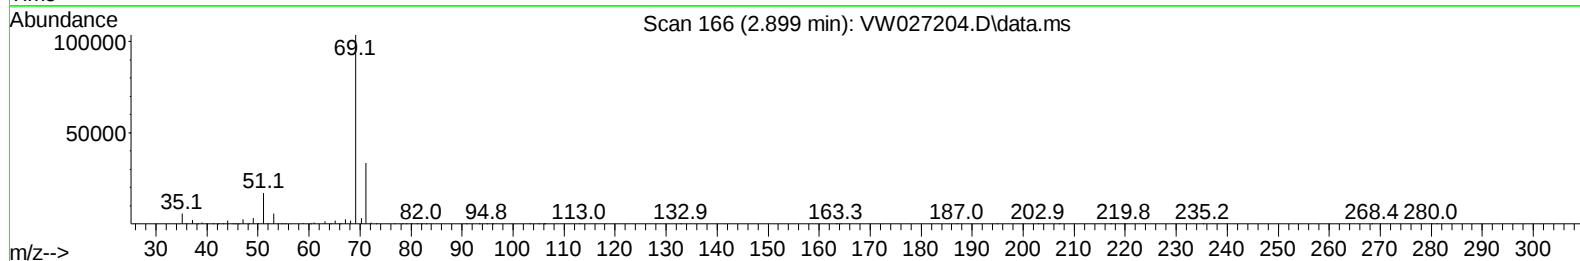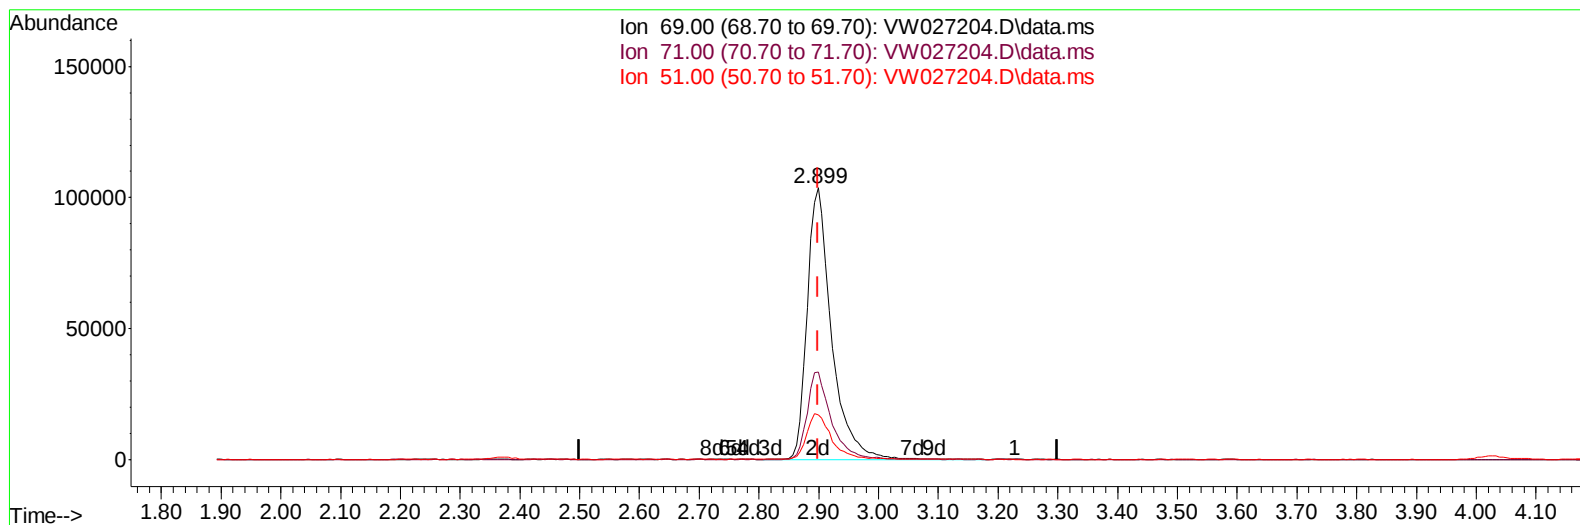

TIC: VW027204.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.000) 26.79 ug/L m

response 294652

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.60	0.02#
51.00	25.20	0.02#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100323\
 Data File : VW027204.D
 Acq On : 03 Oct 2023 16:19
 Operator : SY/MD
 Sample : 04707-01
 Misc : 4.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EY1A2

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:40:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 04 01:37:43 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/04/2023
 Supervised By :Mahesh Dadoda 10/04/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	885597	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	852908	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	422630	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	358828	25.789	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	103.160%	
7) Chloroethane-d5	2.899	69	294652m	26.794	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	107.160%	
11) 1,1-Dichloroethene-d2	4.021	65	150277	25.995	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	103.960%	
21) 2-Butanone-d5	7.075	46	180668	62.809	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	125.620%	
24) Chloroform-d	7.648	84	694339	26.789	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	107.160%	
26) 1,2-Dichloroethane-d4	8.307	65	363514	29.265	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	117.080%	
32) Benzene-d6	8.276	84	1464645	28.020	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	112.080%	
36) 1,2-Dichloropropane-d6	9.276	67	447651	28.605	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	114.440%	
41) Toluene-d8	10.325	98	1313770	28.482	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	113.920%	
43) trans-1,3-Dichloroprop...	10.575	79	180233	29.348	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	117.400%	
47) 2-Hexanone-d5	10.922	63	164273	68.622	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	137.240%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	365831	30.546	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	122.200%#	
66) 1,2-Dichlorobenzene-d4	13.854	152	426426	30.093	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	120.360%#	
Target Compounds						
16) Methylene chloride	4.923	84	95043	5.482	ug/L	94
46) Tetrachloroethene	10.861	164	27364	2.211	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100323\
Data File : VW027204.D
Acq On : 03 Oct 2023 16:19
Operator : SY/MD
Sample : 04707-01
Misc : 4.98g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EY1A2

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:40:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092723SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 04 01:37:43 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 10/04/2023
Supervised By :Mahesh Dadoda 10/04/2023

