

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030363.D
 Acq On : 03 Oct 2024 10:42
 Operator : SY/MD
 Sample : VW1003SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 04 01:06:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	168510	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	162029	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	72267	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	39730	30.172	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	120.680%
7) Chloroethane-d5	2.899	69	30999	32.355	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	129.440%
11) 1,1-Dichloroethene-d2	4.027	65	23178	24.114	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	96.440%
21) 2-Butanone-d5	7.081	46	23992	45.307	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.620%
24) Chloroform-d	7.654	84	108495	23.966	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.880%
26) 1,2-Dichloroethane-d4	8.306	65	58808	24.888	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.560%
32) Benzene-d6	8.276	84	211312	23.269	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.080%
36) 1,2-Dichloropropane-d6	9.276	67	66598	24.383	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.520%
41) Toluene-d8	10.324	98	188479	22.634	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.520%
43) trans-1,3-Dichloroprop...	10.580	79	24602	21.655	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.640%
47) 2-Hexanone-d5	10.922	63	18479	40.971	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.940%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	45901	22.490	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.960%
66) 1,2-Dichlorobenzene-d4	13.848	152	61094	25.463	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.840%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	1937	0.485	ug/L	# 44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030363.D
Acq On : 03 Oct 2024 10:42
Operator : SY/MD
Sample : VW1003SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 04 01:06:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

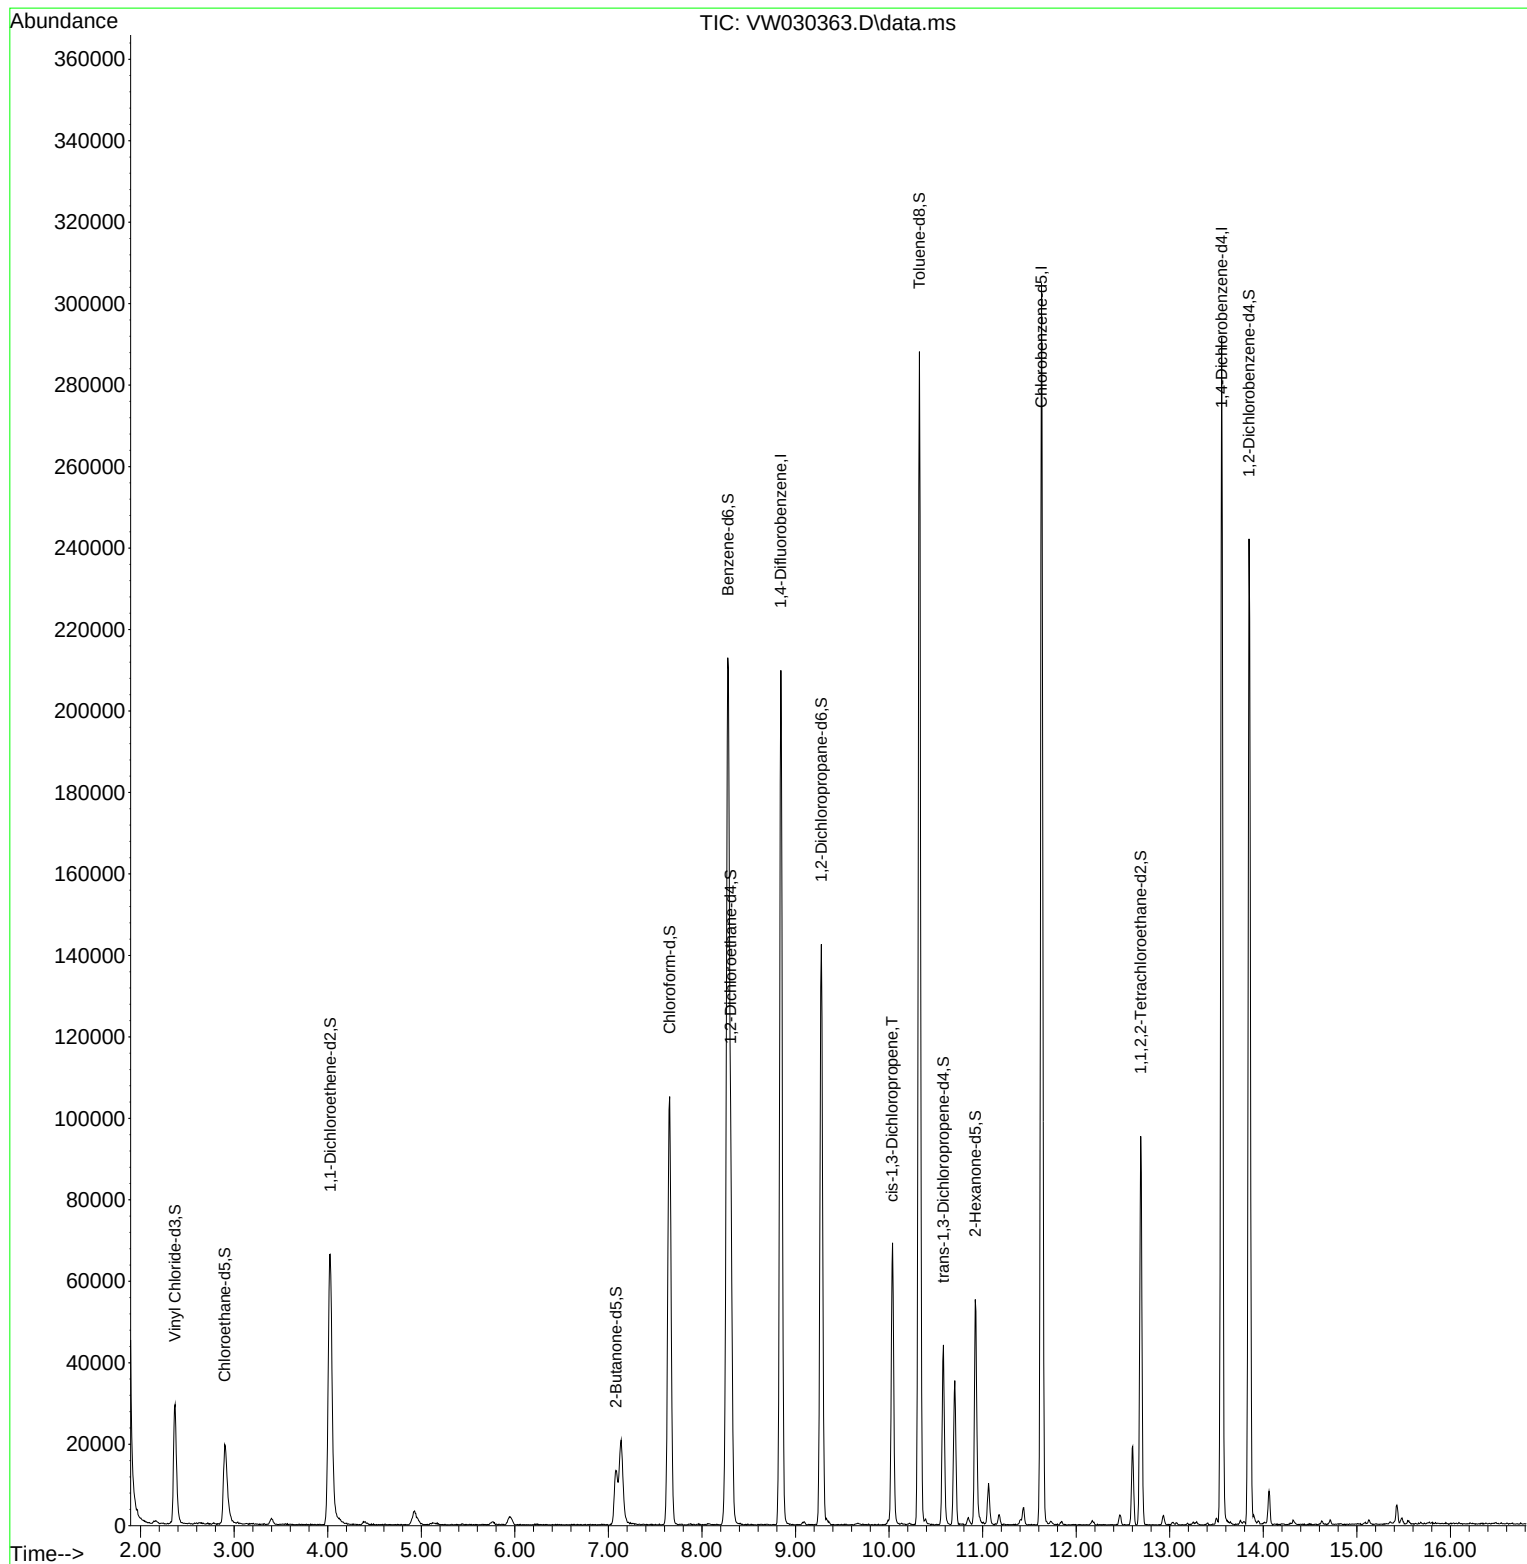

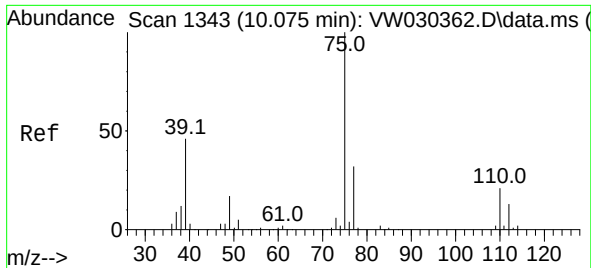

#39
cis-1,3-Dichloropropene
Concen: 0.485 ug/L
RT: 10.032 min Scan# 14
Delta R.T. -0.043 min
Lab File: VW030363.D
Acq: 03 Oct 2024 10:42

Instrument :
MSVOA_W
ClientSampleId :

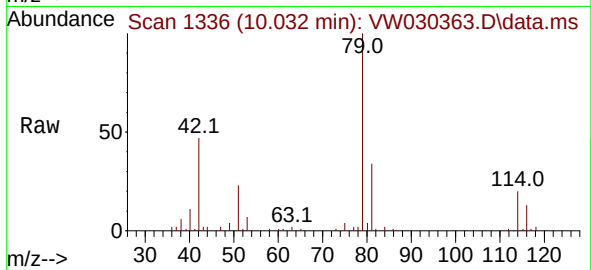

Tgt Ion: 75 Resp: 1937
Ion Ratio Lower Upper
75 100
77 62.3 22.0 40.8#

