

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030364.D
 Acq On : 03 Oct 2024 11:18
 Operator : SY/MD
 Sample : P4237-21
 Misc : 5.00g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 07 21:15:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 05 01:25:07 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.843	114	169431	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.629	117	163925	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.556	152	75816	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.363	65	40669	30.717	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.880%	
7) Chloroethane-d5		2.899	69	31381	32.576	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	130.320%	
11) 1,1-Dichloroethene-d2		4.021	65	23896	24.726	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	98.920%	
21) 2-Butanone-d5		7.081	46	28269	53.094	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.180%	
24) Chloroform-d		7.648	84	111980	24.601	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4		8.307	65	62556	26.330	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.320%	
32) Benzene-d6		8.276	84	218456	23.777	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.120%	
36) 1,2-Dichloropropane-d6		9.276	67	69890	25.292	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.160%	
41) Toluene-d8		10.325	98	193563	22.976	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.920%	
43) trans-1,3-Dichloroprop...		10.575	79	26703	23.233	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.920%	
47) 2-Hexanone-d5		10.922	63	22102	48.437	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.880%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	52232	25.296	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4		13.855	152	63726	25.316	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.280%	
Target Compounds							
39) cis-1,3-Dichloropropene		10.032	75	2075	0.514	ug/L	Qvalue # 55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030364.D
Acq On : 03 Oct 2024 11:18
Operator : SY/MD
Sample : P4237-21
Misc : 5.00g/10mL/MSVOA_W/SOIL/A
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 07 21:15:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 05 01:25:07 2024
Response via : Initial Calibration

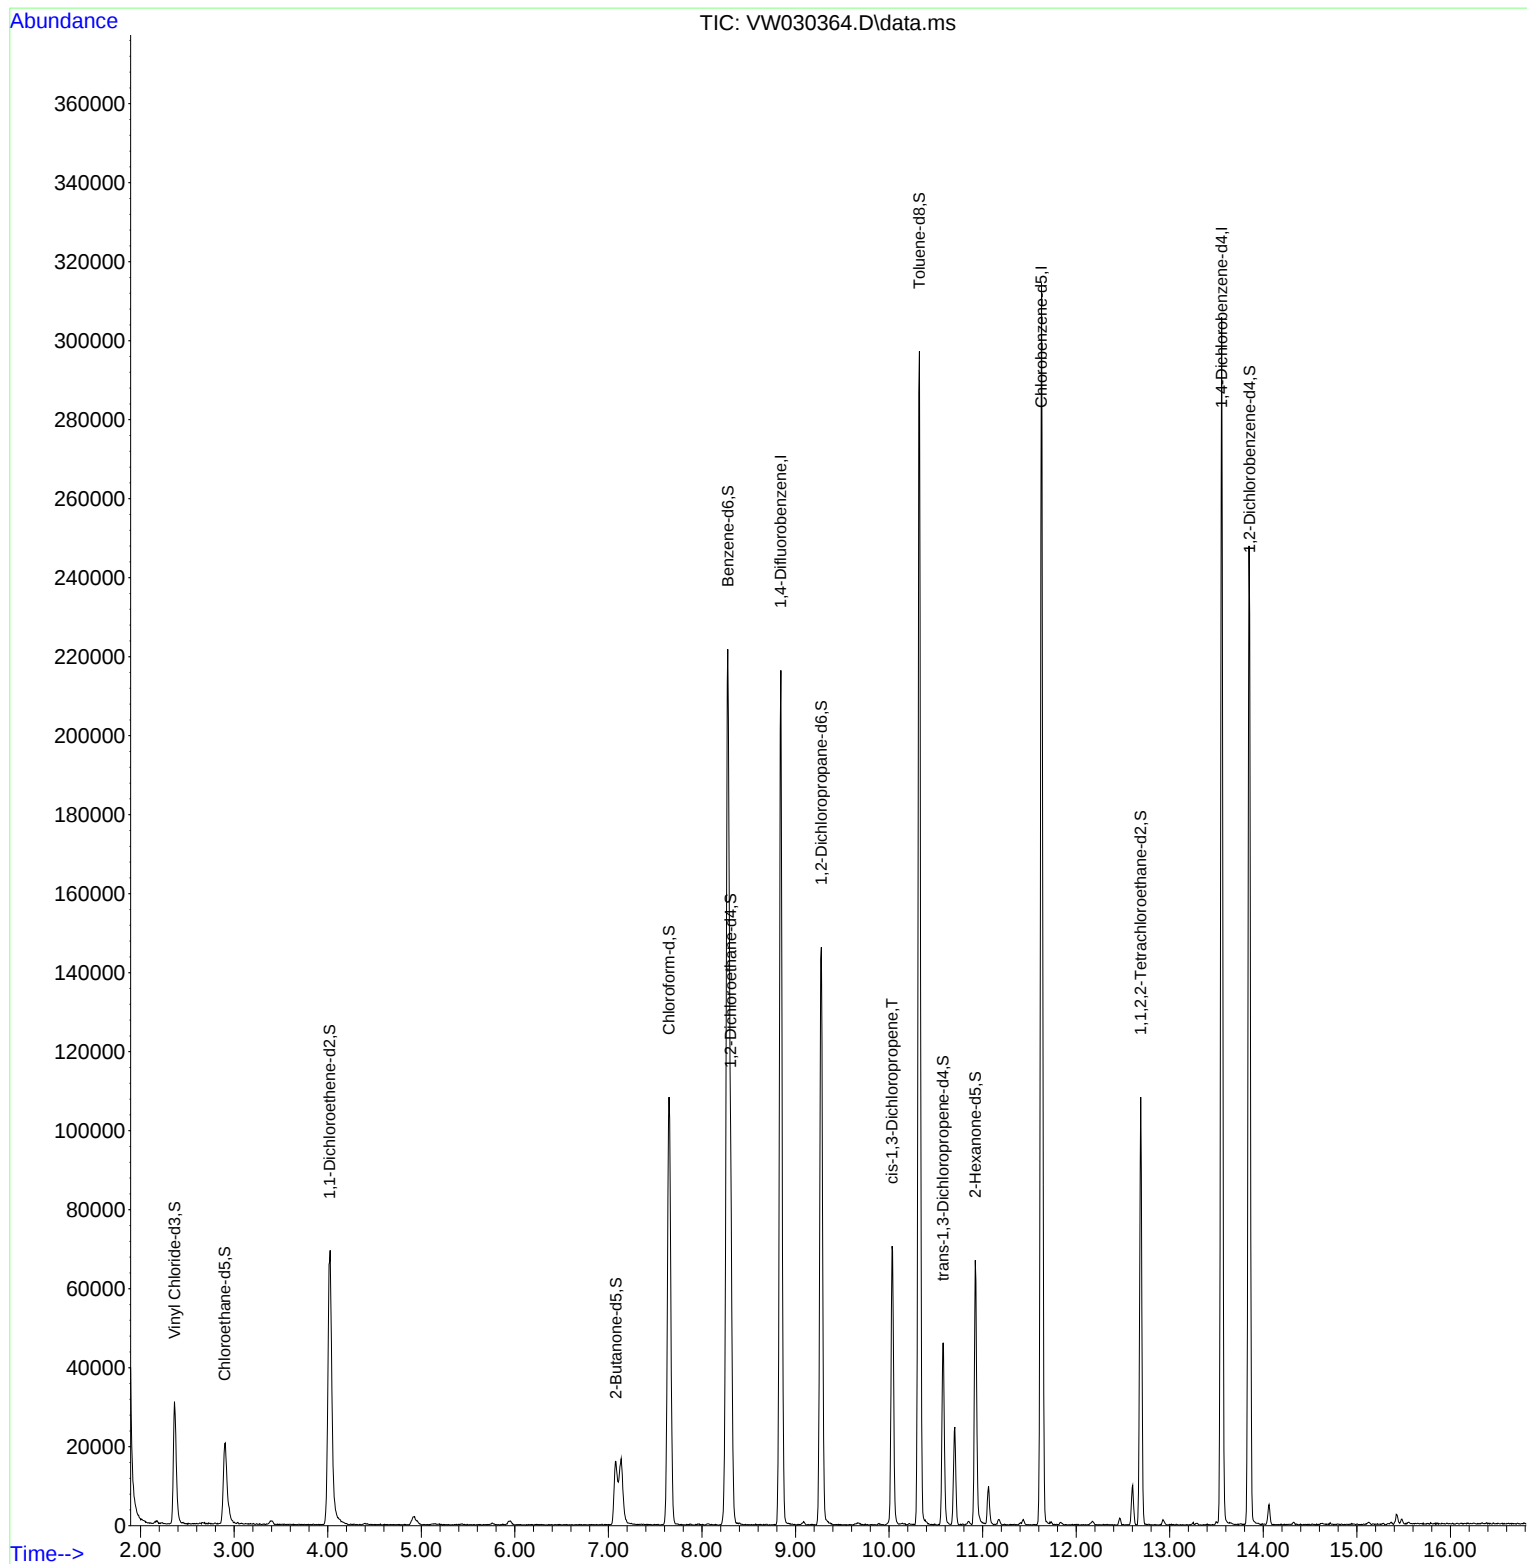

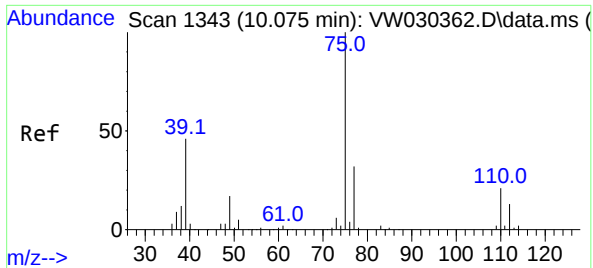

#39
cis-1,3-Dichloropropene
Concen: 0.514 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.043 min
Lab File: VW030364.D
Acq: 03 Oct 2024 11:18

Instrument :
MSVOA_W
ClientSampleId :

Tgt Ion: 75 Resp: 2075
Ion Ratio Lower Upper
75 100
77 56.3 22.0 40.8#

