




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030380.D
Acq On : 03 Oct 2024 18:45
Operator : SY/MD
Sample : P4284-01
Misc : 5.01g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EQ1

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:10:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
Supervised By :Semsettin Yesilyurt 10/04/2024

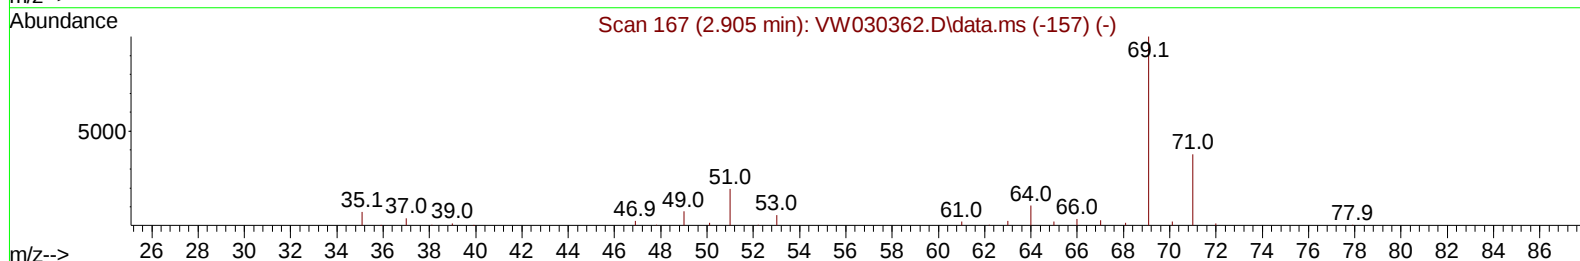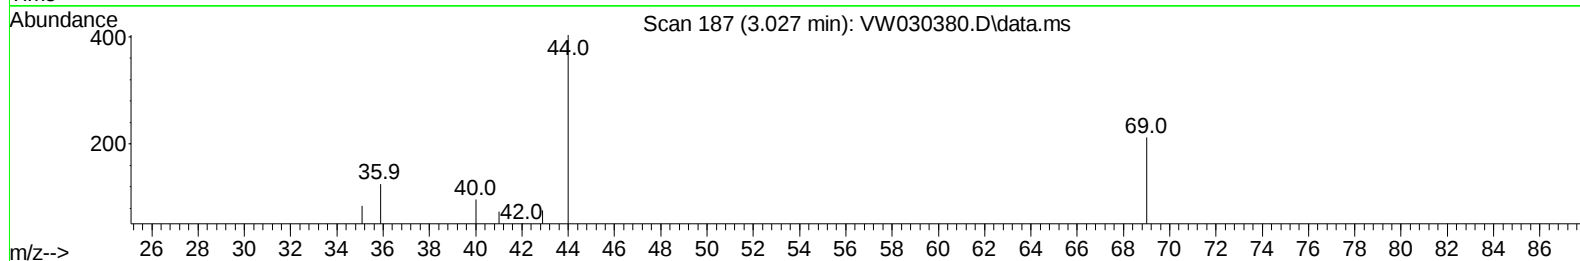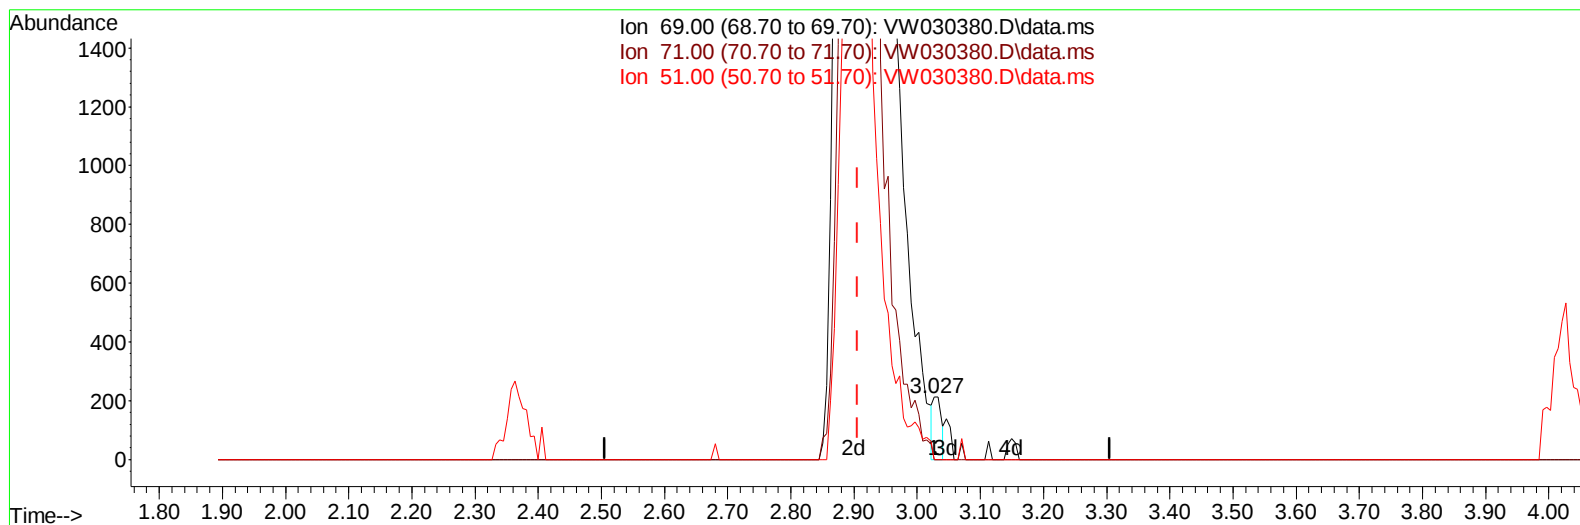

TIC: VW030380.D\data.ms

(7) Chloroethane-d5 (S)

3.027min (+ 0.122) 0.09 ug/L

response 196

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	22.45
51.00	28.00	30.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030380.D
 Acq On : 03 Oct 2024 18:45
 Operator : SY/MD
 Sample : P4284-01
 Misc : 5.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ1

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:10:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
 Supervised By :Semsettin Yesilyurt 10/04/2024

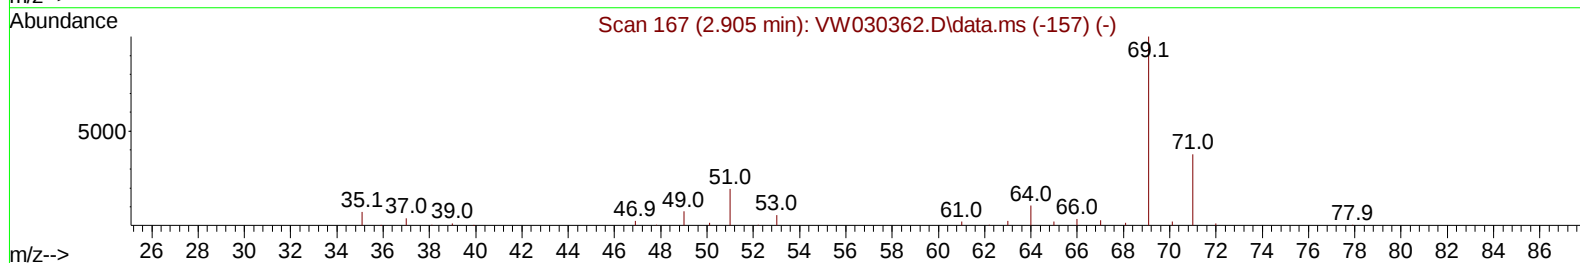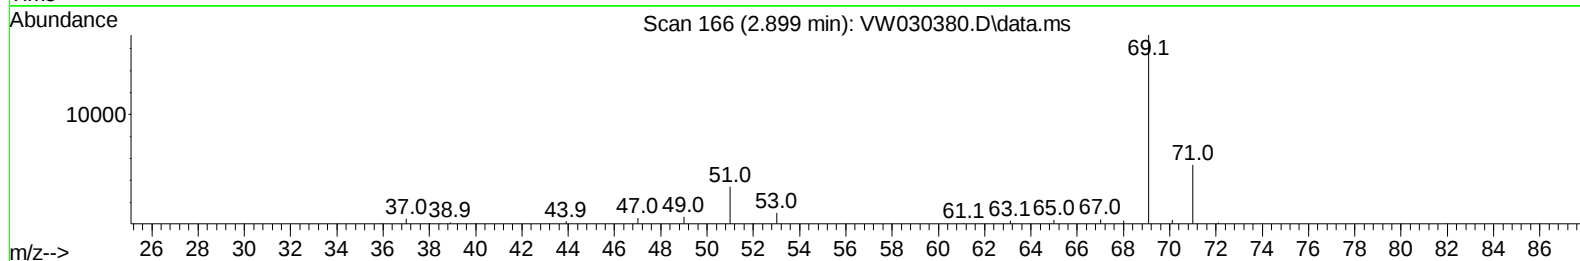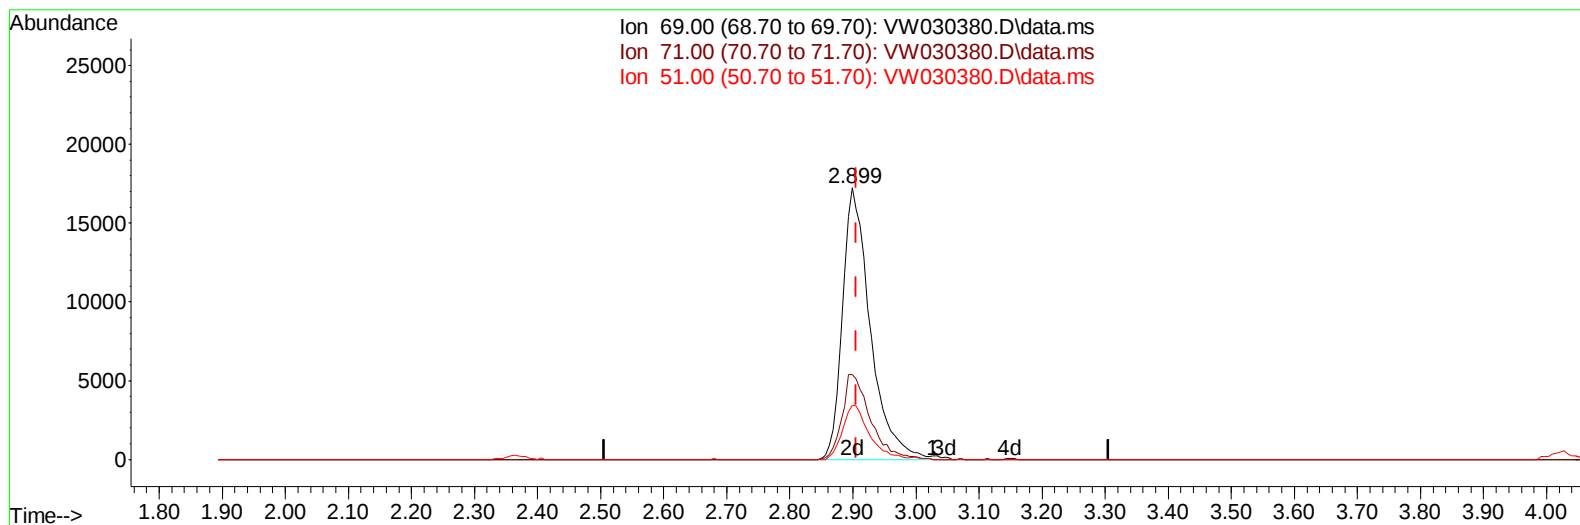

TIC: VW030380.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.006) 25.41 ug/L m

response 52998

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	0.08#
51.00	28.00	0.11#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100324\
 Data File : VW030380.D
 Acq On : 03 Oct 2024 18:45
 Operator : SY/MD
 Sample : P4284-01
 Misc : 5.01g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ1

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:10:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
 Supervised By :Semsettin Yesilyurt 10/04/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	366832	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	329164	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	145468	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	69589	24.276	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	97.120%		
7) Chloroethane-d5	2.899	69	52998m	25.411	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery =	101.640%		
11) 1,1-Dichloroethene-d2	4.021	65	41473	19.820	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery =	79.280%		
21) 2-Butanone-d5	7.075	46	37137	32.216	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	64.440%		
24) Chloroform-d	7.648	84	187431	19.019	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery =	76.080%		
26) 1,2-Dichloroethane-d4	8.307	65	97166	18.890	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery =	75.560%		
32) Benzene-d6	8.276	84	365619	19.818	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery =	79.280%		
36) 1,2-Dichloropropane-d6	9.270	67	113825	20.514	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery =	82.040%		
41) Toluene-d8	10.325	98	327041	19.332	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery =	77.320%		
43) trans-1,3-Dichloroprop...	10.575	79	41103	17.809	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery =	71.240%		
47) 2-Hexanone-d5	10.922	63	29888	32.620	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery =	65.240%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	73809	17.801	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery =	71.200%		
66) 1,2-Dichlorobenzene-d4	13.855	152	95406	19.754	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery =	79.000%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030380.D
Acq On : 03 Oct 2024 18:45
Operator : SY/MD
Sample : P4284-01
Misc : 5.01g/10mL/MSVOA_W/SoIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EQ1

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/04/2024
Supervised By :Semsettin Yesilyurt 10/04/2024

Quant Time: Oct 04 01:10:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

