




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030382.D
 Acq On : 03 Oct 2024 19:33
 Operator : SY/MD
 Sample : P4284-03
 Misc : 5.32g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ4

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:11:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
 Supervised By :Semsettin Yesilyurt 10/04/2024

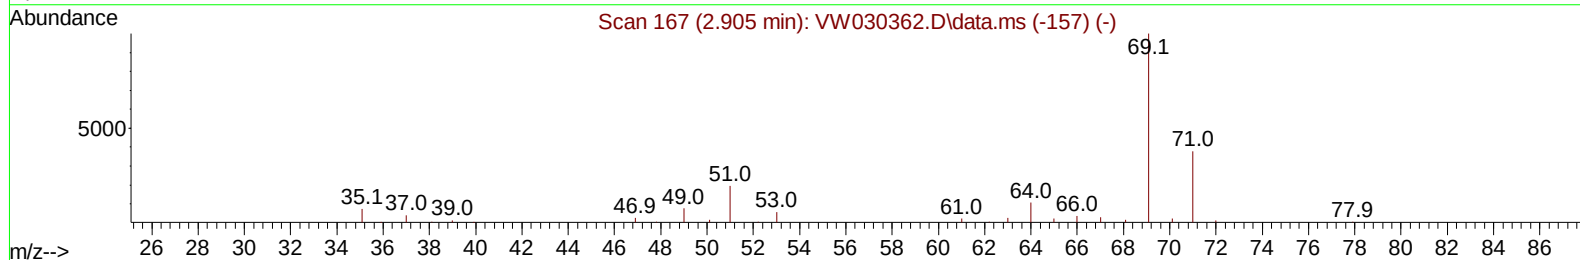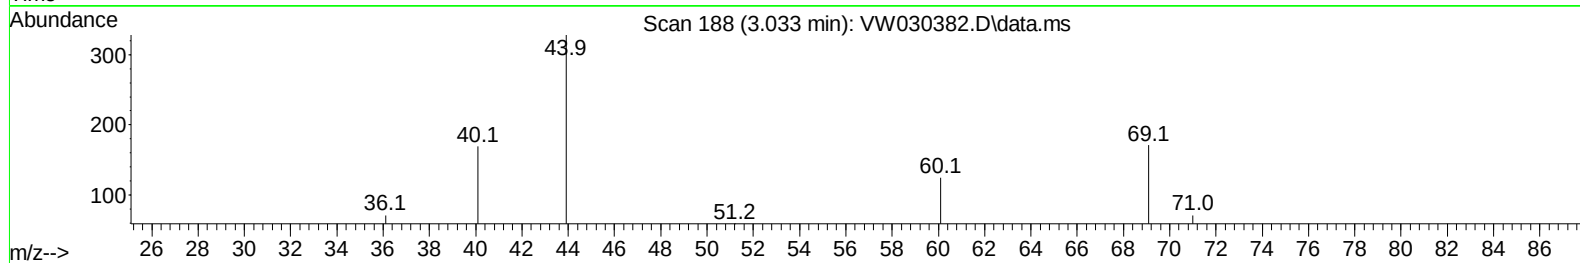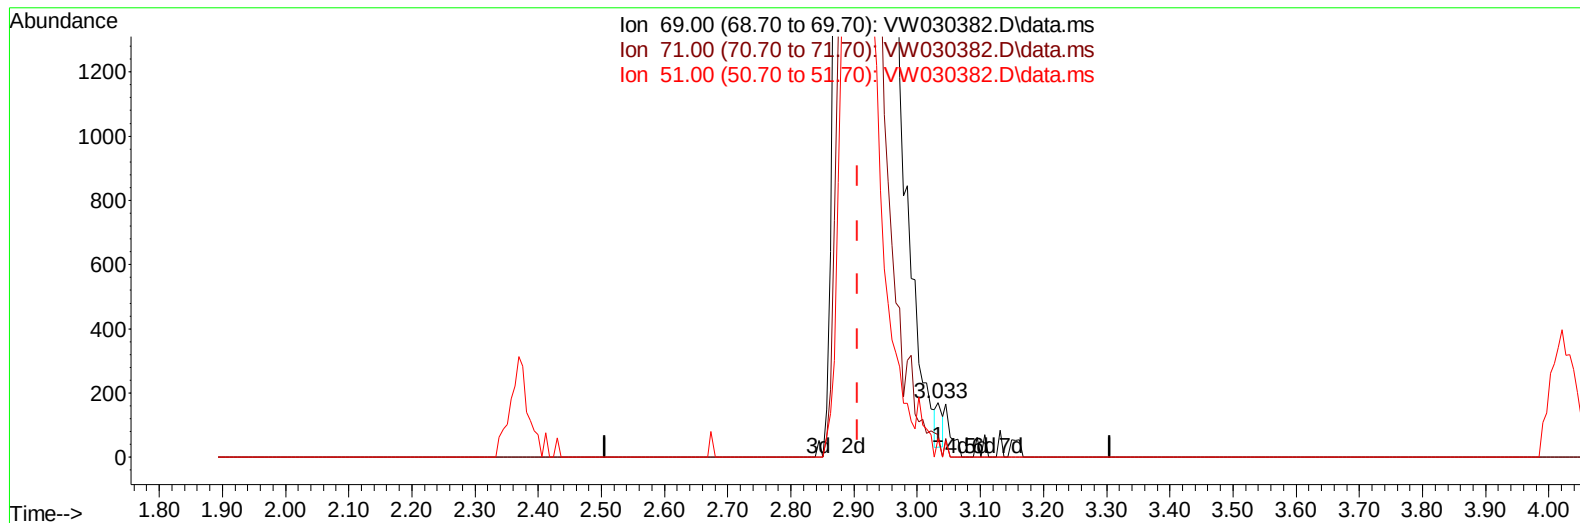

TIC: VW030382.D\data.ms

(7) Chloroethane-d5 (S)

3.033min (+ 0.128) 0.04 ug/L

response 86

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	25.58
51.00	28.00	25.58
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030382.D
 Acq On : 03 Oct 2024 19:33
 Operator : SY/MD
 Sample : P4284-03
 Misc : 5.32g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ4

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:11:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
 Supervised By :Semsettin Yesilyurt 10/04/2024

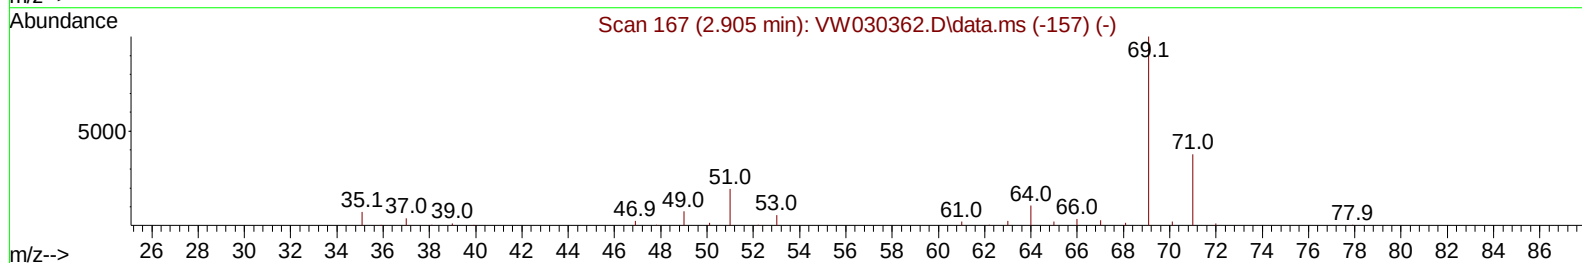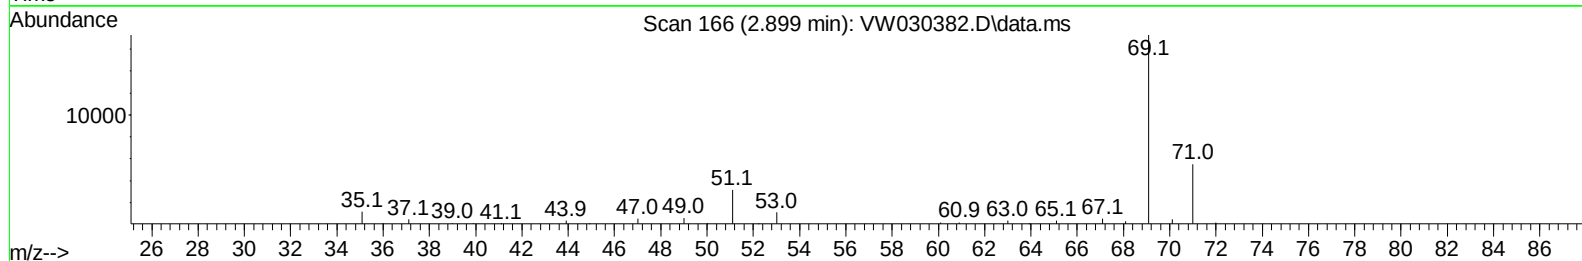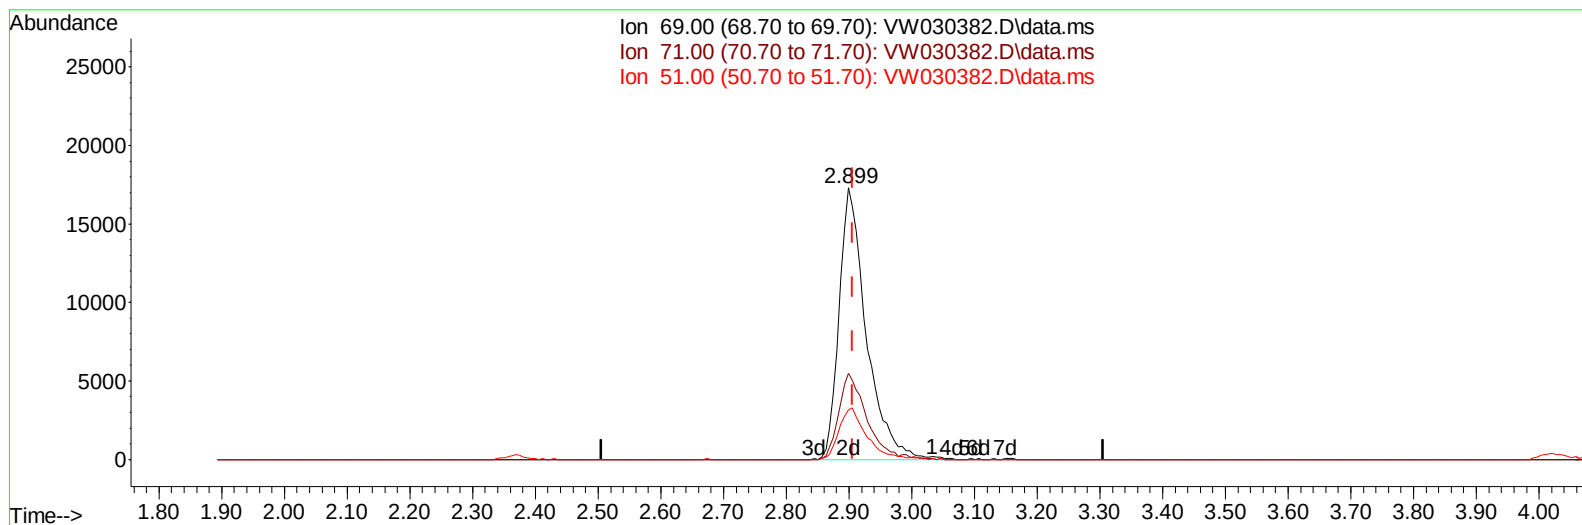

TIC: VW030382.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (-0.006) 25.18 ug/L m

response 51991

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.90	0.04#
51.00	28.00	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw100324\
 Data File : VW030382.D
 Acq On : 03 Oct 2024 19:33
 Operator : SY/MD
 Sample : P4284-03
 Misc : 5.32g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4EQ4

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:11:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
 Supervised By :Semsettin Yesilyurt 10/04/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		363191	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		332811	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		152278	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		70283	24.764	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	99.040%	
7) Chloroethane-d5	2.899	69		51991m	25.178	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	100.720%	
11) 1,1-Dichloroethene-d2	4.021	65		39103	18.875	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	75.520%	
21) 2-Butanone-d5	7.081	46		36964	32.387	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	64.780%	
24) Chloroform-d	7.648	84		183323	18.789	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	75.160%	
26) 1,2-Dichloroethane-d4	8.307	65		92817	18.225	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	72.920%	
32) Benzene-d6	8.276	84		345921	18.545	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	74.160%	
36) 1,2-Dichloropropane-d6	9.276	67		110143	19.633	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	78.520%	
41) Toluene-d8	10.325	98		313922	18.353	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	73.400%	
43) trans-1,3-Dichloroprop...	10.581	79		40827	17.496	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	70.000%	
47) 2-Hexanone-d5	10.922	63		29821	32.190	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	64.380%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		73489	17.530	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	70.120%	
66) 1,2-Dichlorobenzene-d4	13.849	152		98045	19.393	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	77.560%	
Target Compounds							
13) Acetone	4.125	43		11471	9.475	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030382.D
Acq On : 03 Oct 2024 19:33
Operator : SY/MD
Sample : P4284-03
Misc : 5.32g/10mL/MSVOA_W/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4EQ4

Manual IntegrationsAPPROVED

Quant Time: Oct 04 01:11:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/04/2024
Supervised By :Semsettin Yesilyurt 10/04/2024

