

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030367.D
 Acq On : 03 Oct 2024 13:08
 Operator : SY/MD
 Sample : P4238-03RE
 Misc : 5.10g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F13RE

Quant Time: Oct 04 01:07:35 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	229389	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	143441	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	29254	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	59662	33.284	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	133.120%	
7) Chloroethane-d5	2.899	69	43856	33.626	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	134.520%	
11) 1,1-Dichloroethene-d2	4.027	65	31192	23.839	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	95.360%	
21) 2-Butanone-d5	7.075	46	31257	43.361	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	86.720%	
24) Chloroform-d	7.654	84	137280	22.277	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	89.120%	
26) 1,2-Dichloroethane-d4	8.307	65	77655	24.142	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	96.560%	
32) Benzene-d6	8.276	84	253415	31.521	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	126.080%	
36) 1,2-Dichloropropane-d6	9.276	67	81619	33.755	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	135.000%#	
41) Toluene-d8	10.324	98	183022	24.827	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	99.320%	
43) trans-1,3-Dichloroprop...	10.581	79	28231	28.070	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	112.280%	
47) 2-Hexanone-d5	10.922	63	24159	60.506	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	121.020%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	43787	24.234	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	96.920%	
66) 1,2-Dichlorobenzene-d4	13.848	152	22067	22.720	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	90.880%	
Target Compounds					Qvalue	
13) Acetone	4.118	43	6484	8.479	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030367.D
Acq On : 03 Oct 2024 13:08
Operator : SY/MD
Sample : P4238-03RE
Misc : 5.10g/10mL/MSVOA_W/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F13RE

Quant Time: Oct 04 01:07:35 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

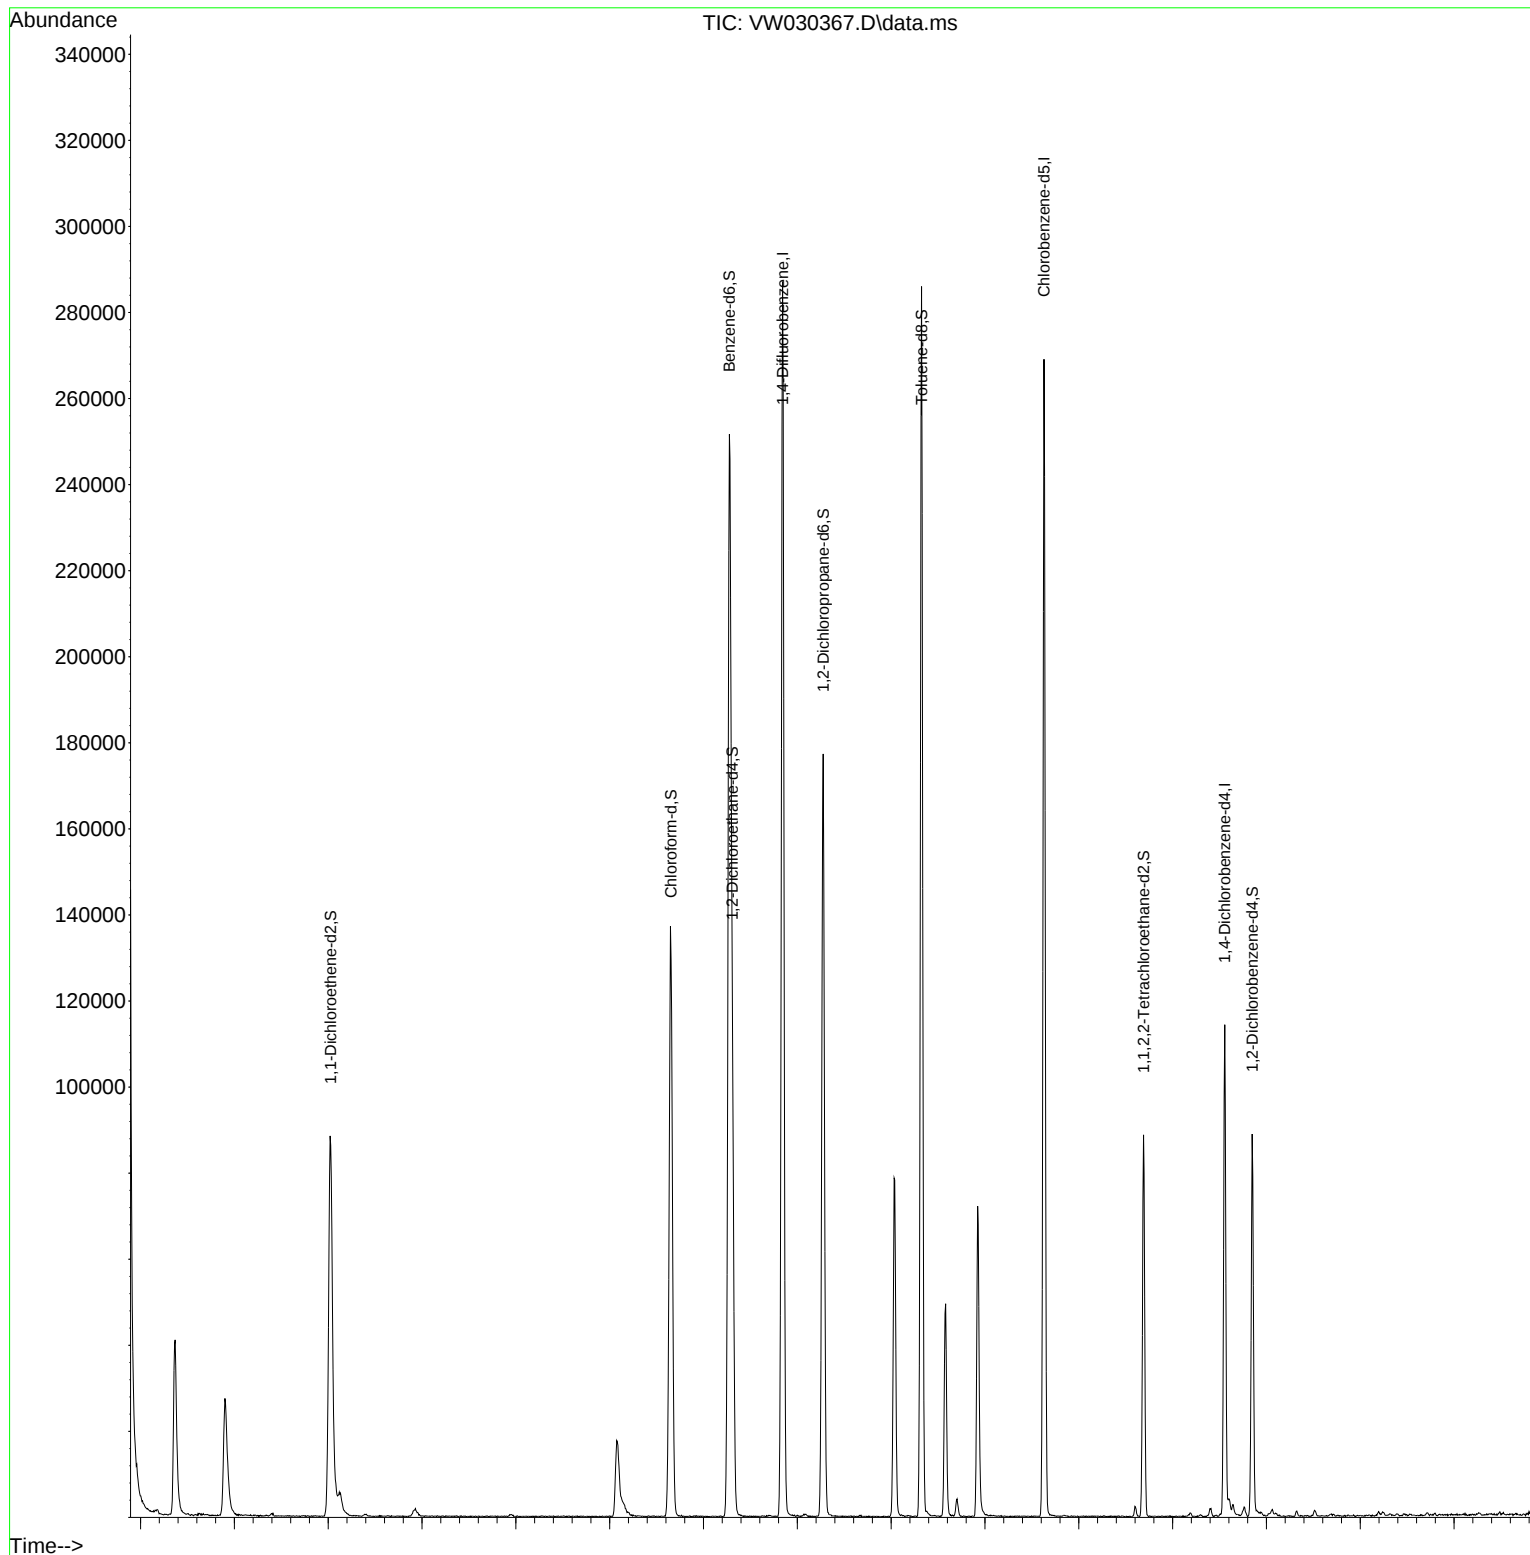

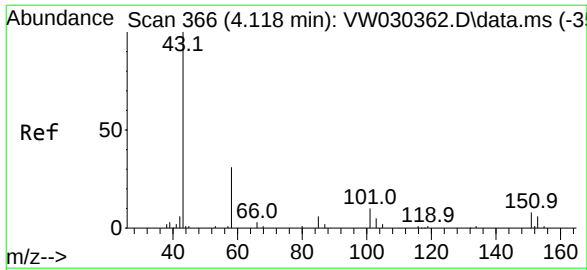

#13
 Acetone
 Concen: 8.479 ug/L
 RT: 4.118 min Scan# 36
 Delta R.T. -0.000 min
 Lab File: VW030367.D
 Acq: 03 Oct 2024 13:08

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F13RE

Tgt Ion: 43 Resp: 6484
 Ion Ratio Lower Upper
 43 100
 58 31.1 0.0 64.0

