

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
 Data File : VW030378.D
 Acq On : 03 Oct 2024 17:57
 Operator : SY/MD
 Sample : P4239-10
 Misc : 5.17g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4ET4

Quant Time: Oct 04 01:10:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 04 01:05:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	336157	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	296372	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	125156	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	60320	22.963	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.840%
7) Chloroethane-d5	2.905	69	44716	23.396	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.600%
11) 1,1-Dichloroethene-d2	4.027	65	33484	17.463	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.840%
21) 2-Butanone-d5	7.075	46	33016	31.254	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.500%
24) Chloroform-d	7.654	84	156323	17.310	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.240%
26) 1,2-Dichloroethane-d4	8.307	65	82354	17.471	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	69.880%#
32) Benzene-d6	8.276	84	293124	17.647	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	70.600%
36) 1,2-Dichloropropane-d6	9.276	67	94155	18.846	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.400%
41) Toluene-d8	10.324	98	245488	16.117	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	64.480%
43) trans-1,3-Dichloroprop...	10.574	79	34420	16.564	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.240%
47) 2-Hexanone-d5	10.922	63	25762	31.227	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.460%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	63687	17.060	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	68.240%
66) 1,2-Dichlorobenzene-d4	13.848	152	70832	17.046	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	68.200%#
Target Compounds					Qvalue	
13) Acetone	4.130	43	5531	4.936	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW100324\
Data File : VW030378.D
Acq On : 03 Oct 2024 17:57
Operator : SY/MD
Sample : P4239-10
Misc : 5.17g/10mL/MSVOA_W/SOIL/A
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4ET4

Quant Time: Oct 04 01:10:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM092724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 04 01:05:34 2024
Response via : Initial Calibration

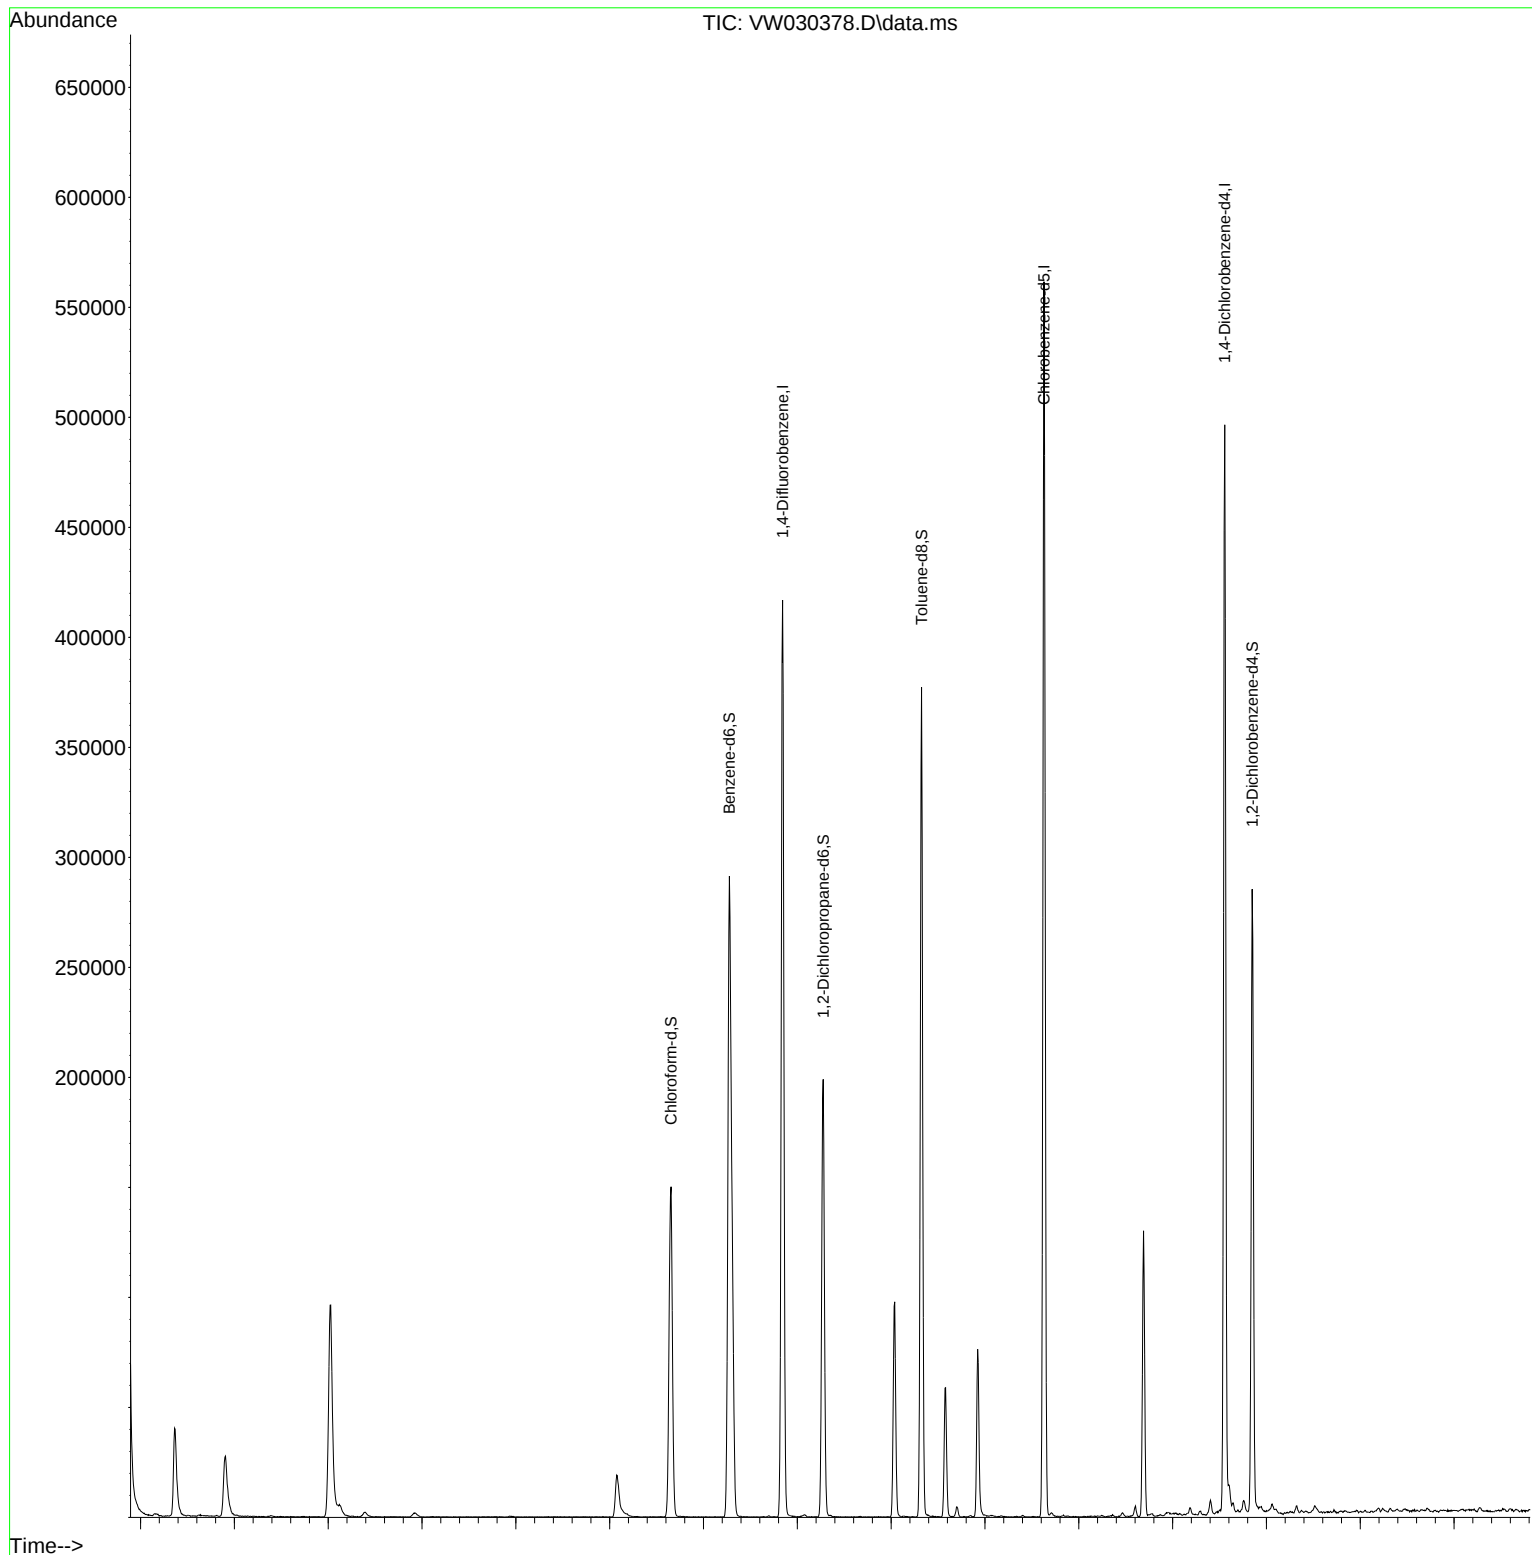

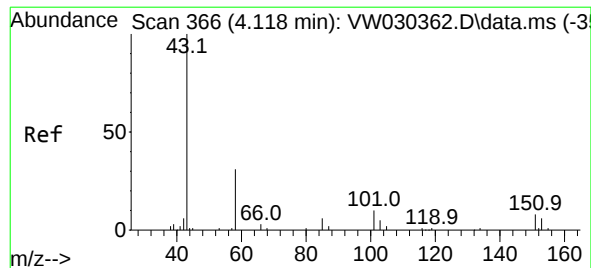

#13

Acetone

Concen: 4.936 ug/L

RT: 4.130 min Scan# 36

Delta R.T. 0.012 min

Lab File: VW030378.D

Acq: 03 Oct 2024 17:57

Instrument :

MSVOA_W

ClientSampleId :

A4ET4

Tgt Ion: 43 Resp: 5531

Ion Ratio Lower Upper

43 100

58 33.0 0.0 64.0

